


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110518\
 Data File : BG037795.D
 Acq On : 5 Nov 2018 9:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

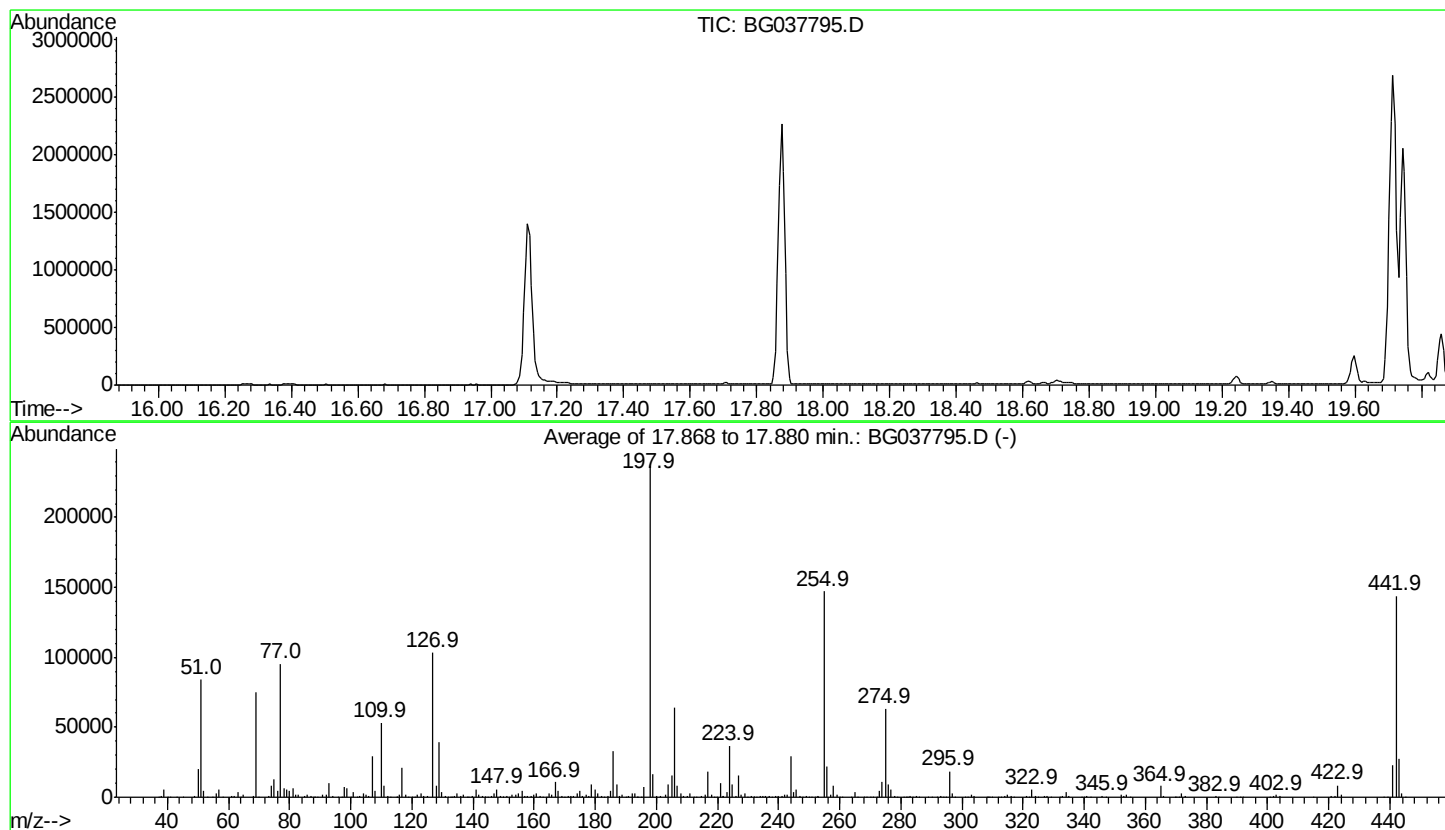

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	83816	PASS
68	69	0.00	2	1.5	1157	PASS
69	198	0.00	100	31.7	75176	PASS
70	69	0.00	2	0.5	353	PASS
127	198	10	80	43.6	103304	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	237056	PASS
199	198	5	9	7.1	16840	PASS
275	198	10	60	26.7	63210	PASS
365	198	1	100	3.3	7863	PASS
441	198	0.01	100	9.8	23114	PASS
442	198	50	100	60.6	143682	PASS
443	442	15	24	19.4	27896	PASS