


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110518\
Data File : BG037796.D
Acq On : 5 Nov 2018 10:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 18 14:06:42 2018

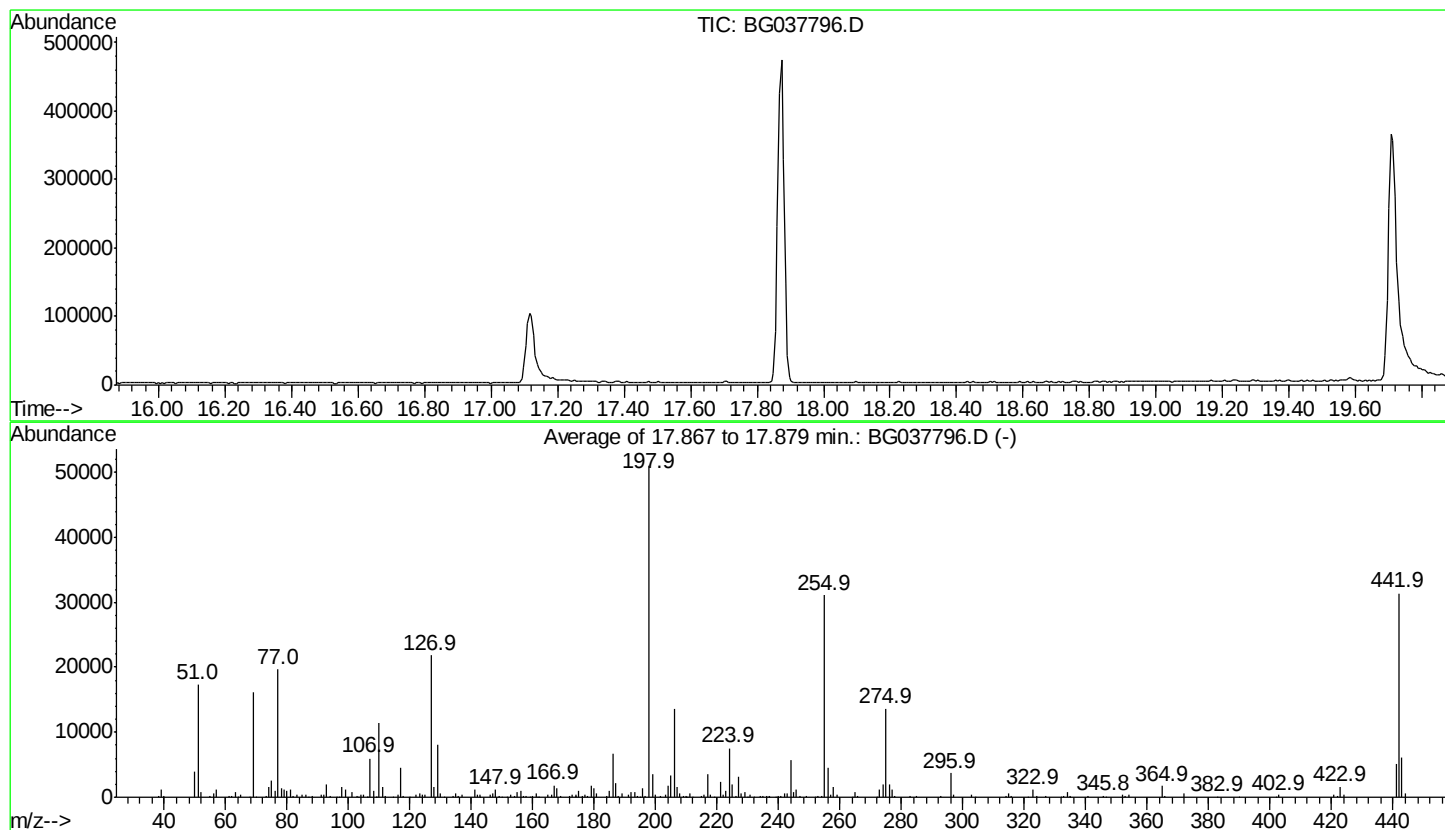

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	17274	PASS
68	69	0.00	2	0.5	79	PASS
69	198	0.00	100	31.8	16230	PASS
70	69	0.00	2	0.4	60	PASS
127	198	10	80	42.8	21818	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51018	PASS
199	198	5	9	6.9	3506	PASS
275	198	10	60	26.8	13653	PASS
365	198	1	100	3.3	1709	PASS
441	198	0.01	100	10.1	5152	PASS
442	198	50	100	61.4	31325	PASS
443	442	15	24	19.3	6051	PASS