


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110518\
 Data File : BG037805.D
 Acq On : 5 Nov 2018 16:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

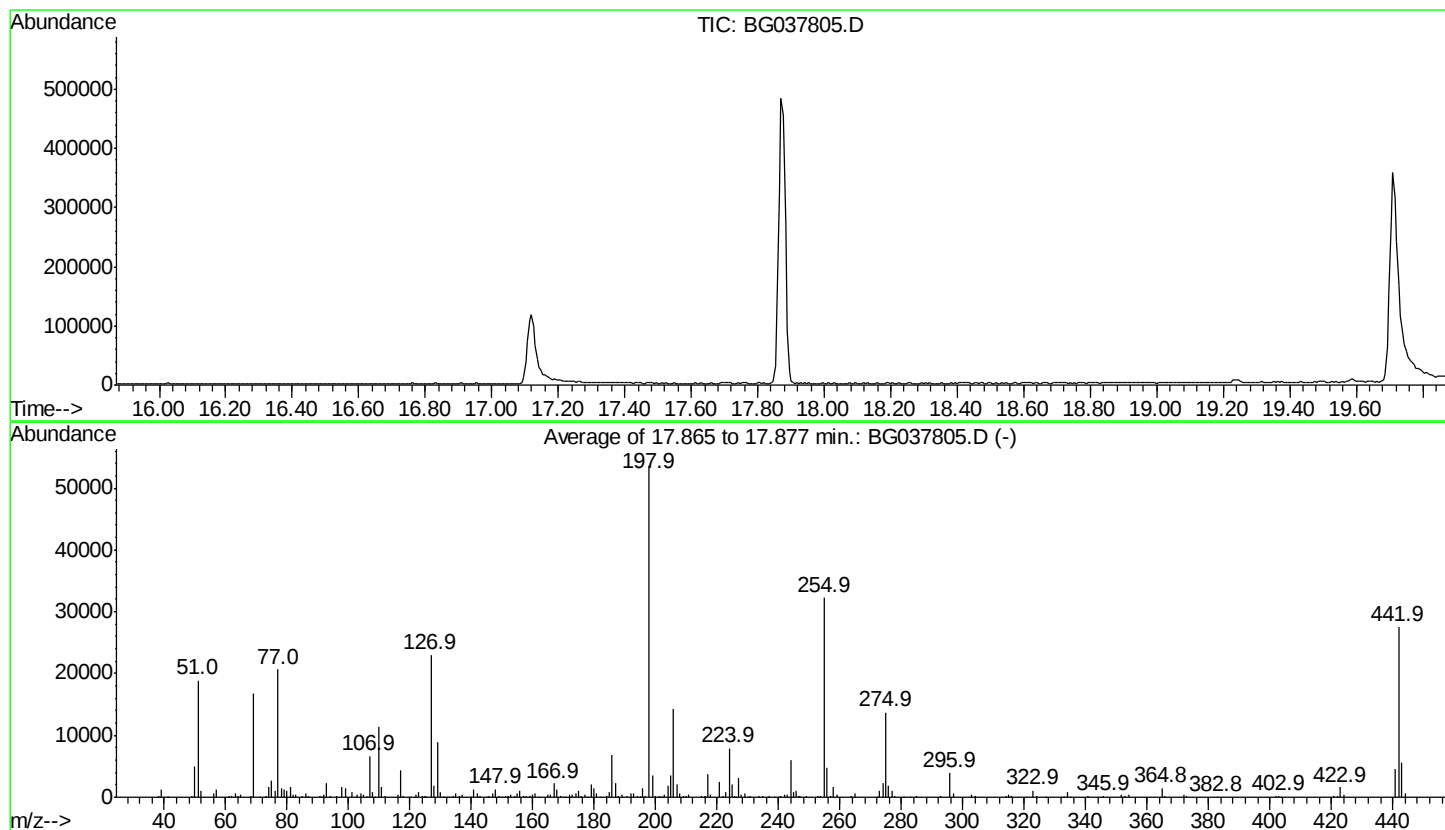

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	18923	PASS
68	69	0.00	2	0.8	138	PASS
69	198	0.00	100	31.2	16749	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	23080	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53629	PASS
199	198	5	9	6.7	3614	PASS
275	198	10	60	25.6	13708	PASS
365	198	1	100	2.8	1476	PASS
441	198	0.01	100	8.7	4660	PASS
442	198	50	100	51.5	27598	PASS
443	442	15	24	20.1	5545	PASS