
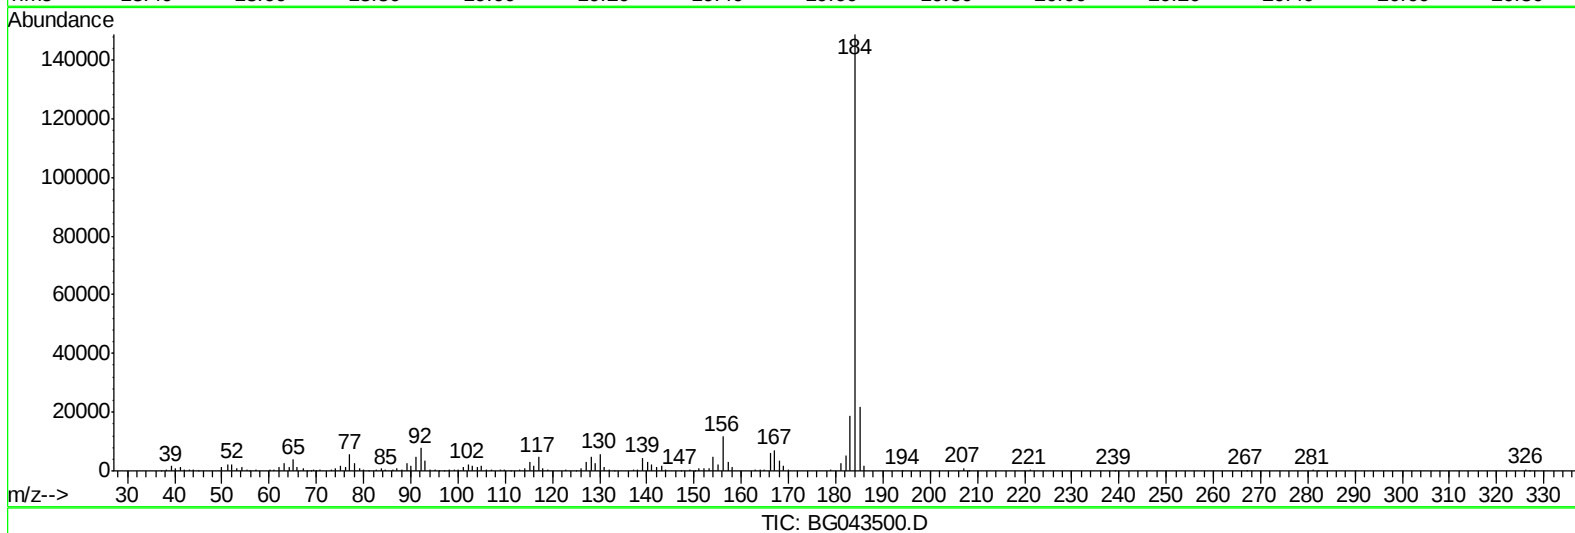


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110519\
 Data File : BG043500.D
 Acq On : 5 Nov 2019 10:08
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 06:14:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

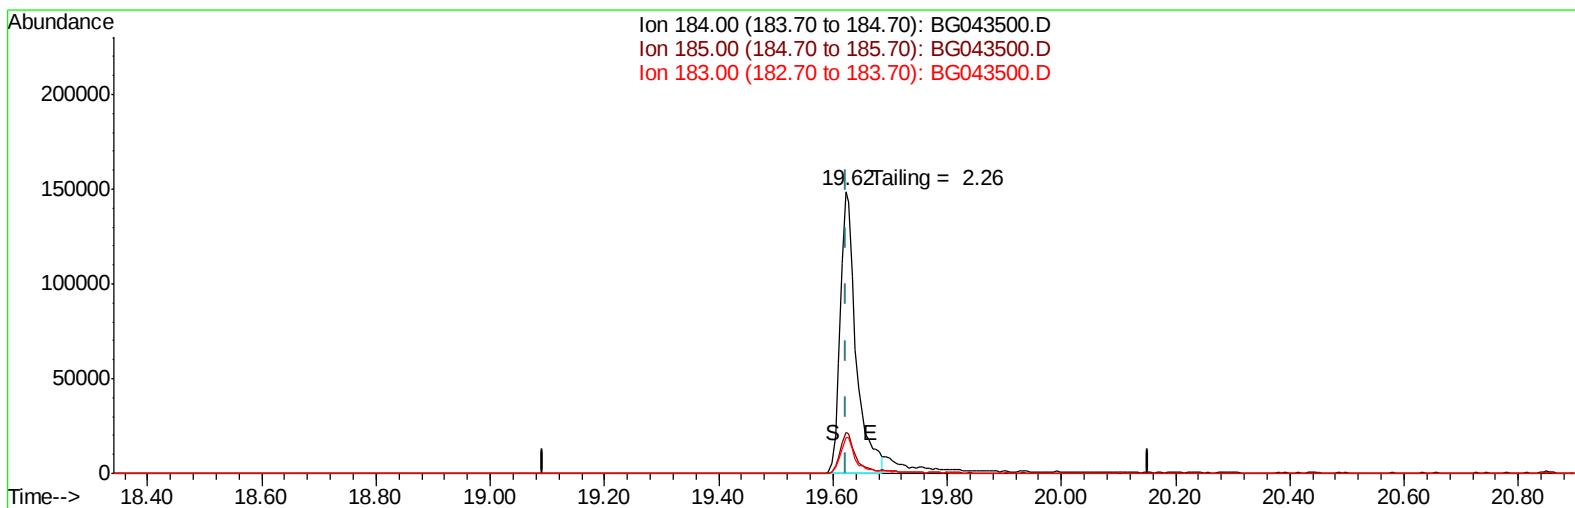

TIC: BG043500.D

(77) Benzidine



19.622min (-0.002) 227852.96ng

response 307236

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	14.65
183.00	12.50	12.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110519\
Data File : BG043500.D
Acq On : 5 Nov 2019 10:08
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 06:14:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

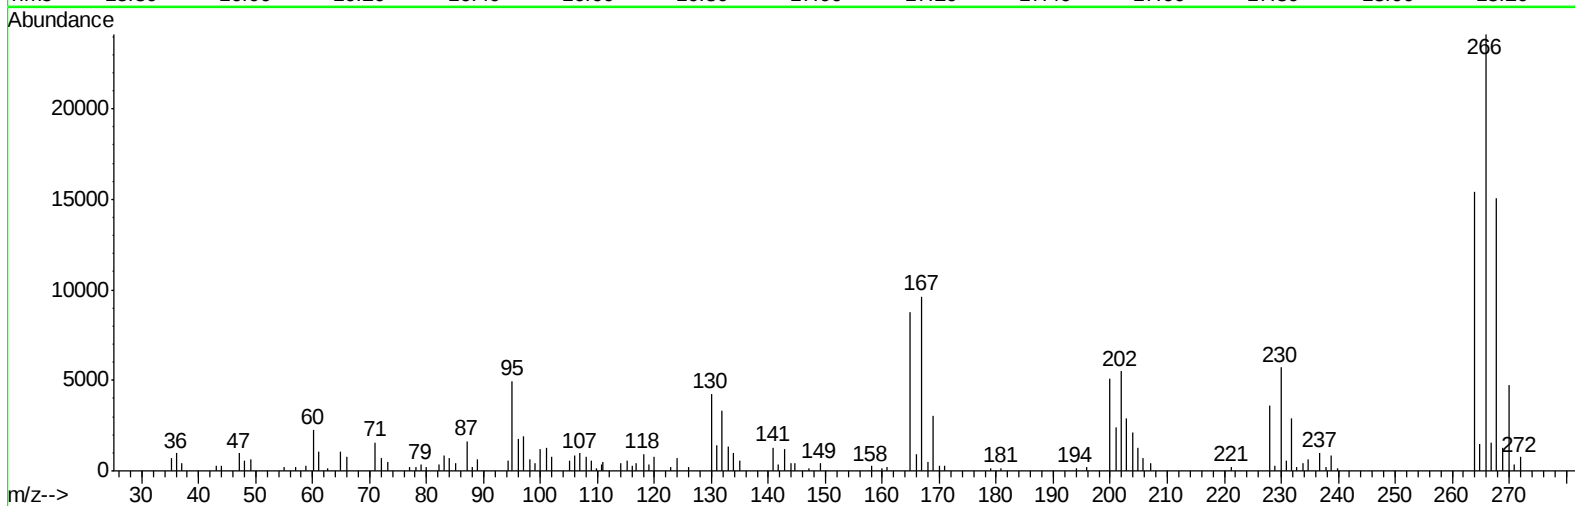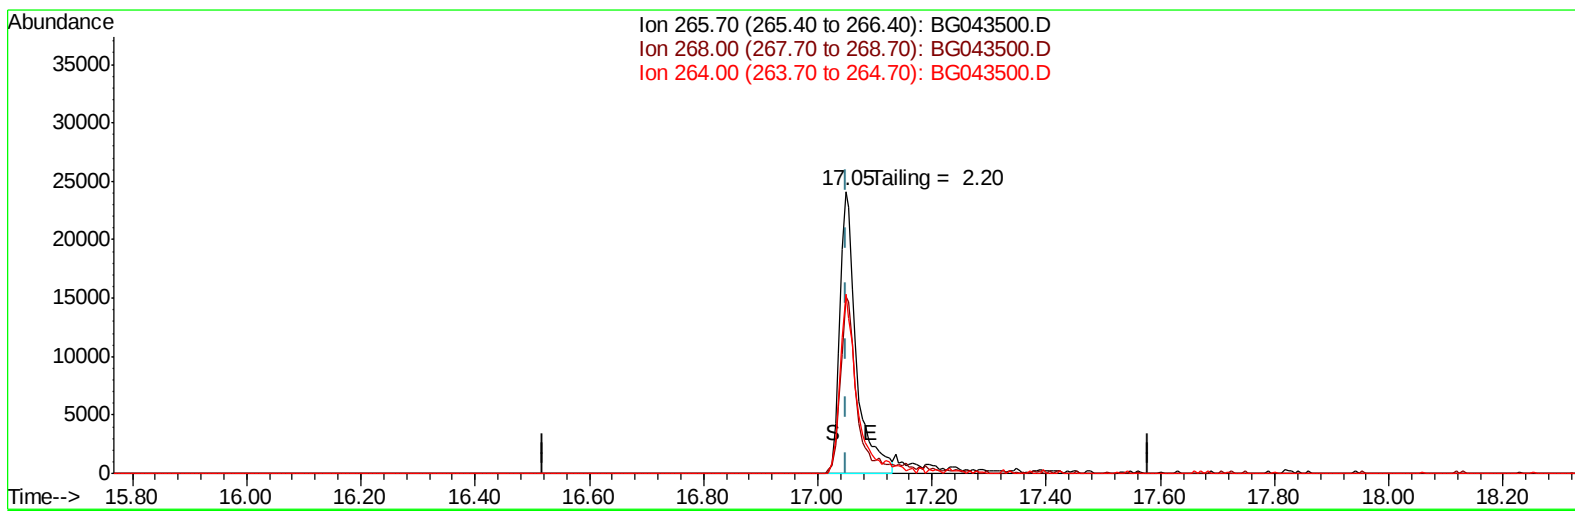

TIC: BG043500.D

(70) Pentachlorophenol (C)

17.048min (-0.002) 18322.37ng

response 48880

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	62.52
264.00	61.10	63.80
0.00	0.00	0.00