

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110519\
 Data File : BG043508.D
 Acq On : 5 Nov 2019 15:15
 Operator : JU
 Sample : PB124558BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB124558BL

Quant Time: Nov 06 02:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	32007	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	107938	20.00	ng	0.00
39) Acenaphthene-d10	14.64	164	80156	20.00	ng	0.00
64) Phenanthrene-d10	17.39	188	211090	20.00	ng	0.00
76) Chrysene-d12	21.65	240	245217	20.00	ng	0.00
87) Perylene-d12	24.85	264	289644	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	245493	140.55	ng	0.00
7) Phenol-d6	7.19	99	333955	132.89	ng	0.00
23) Nitrobenzene-d5	9.17	82	192976	92.17	ng	0.00
42) 2,4,6-Tribromophenol	16.13	330	212729	139.46	ng	0.00
45) 2-Fluorobiphenyl	13.26	172	534308	92.11	ng	0.00
79) Terphenyl-d14	20.00	244	1289243	98.63	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110519\
Data File : BG043508.D
Acq On : 5 Nov 2019 15:15
Operator : JU
Sample : PB124558BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124558BL

Quant Time: Nov 06 02:16:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

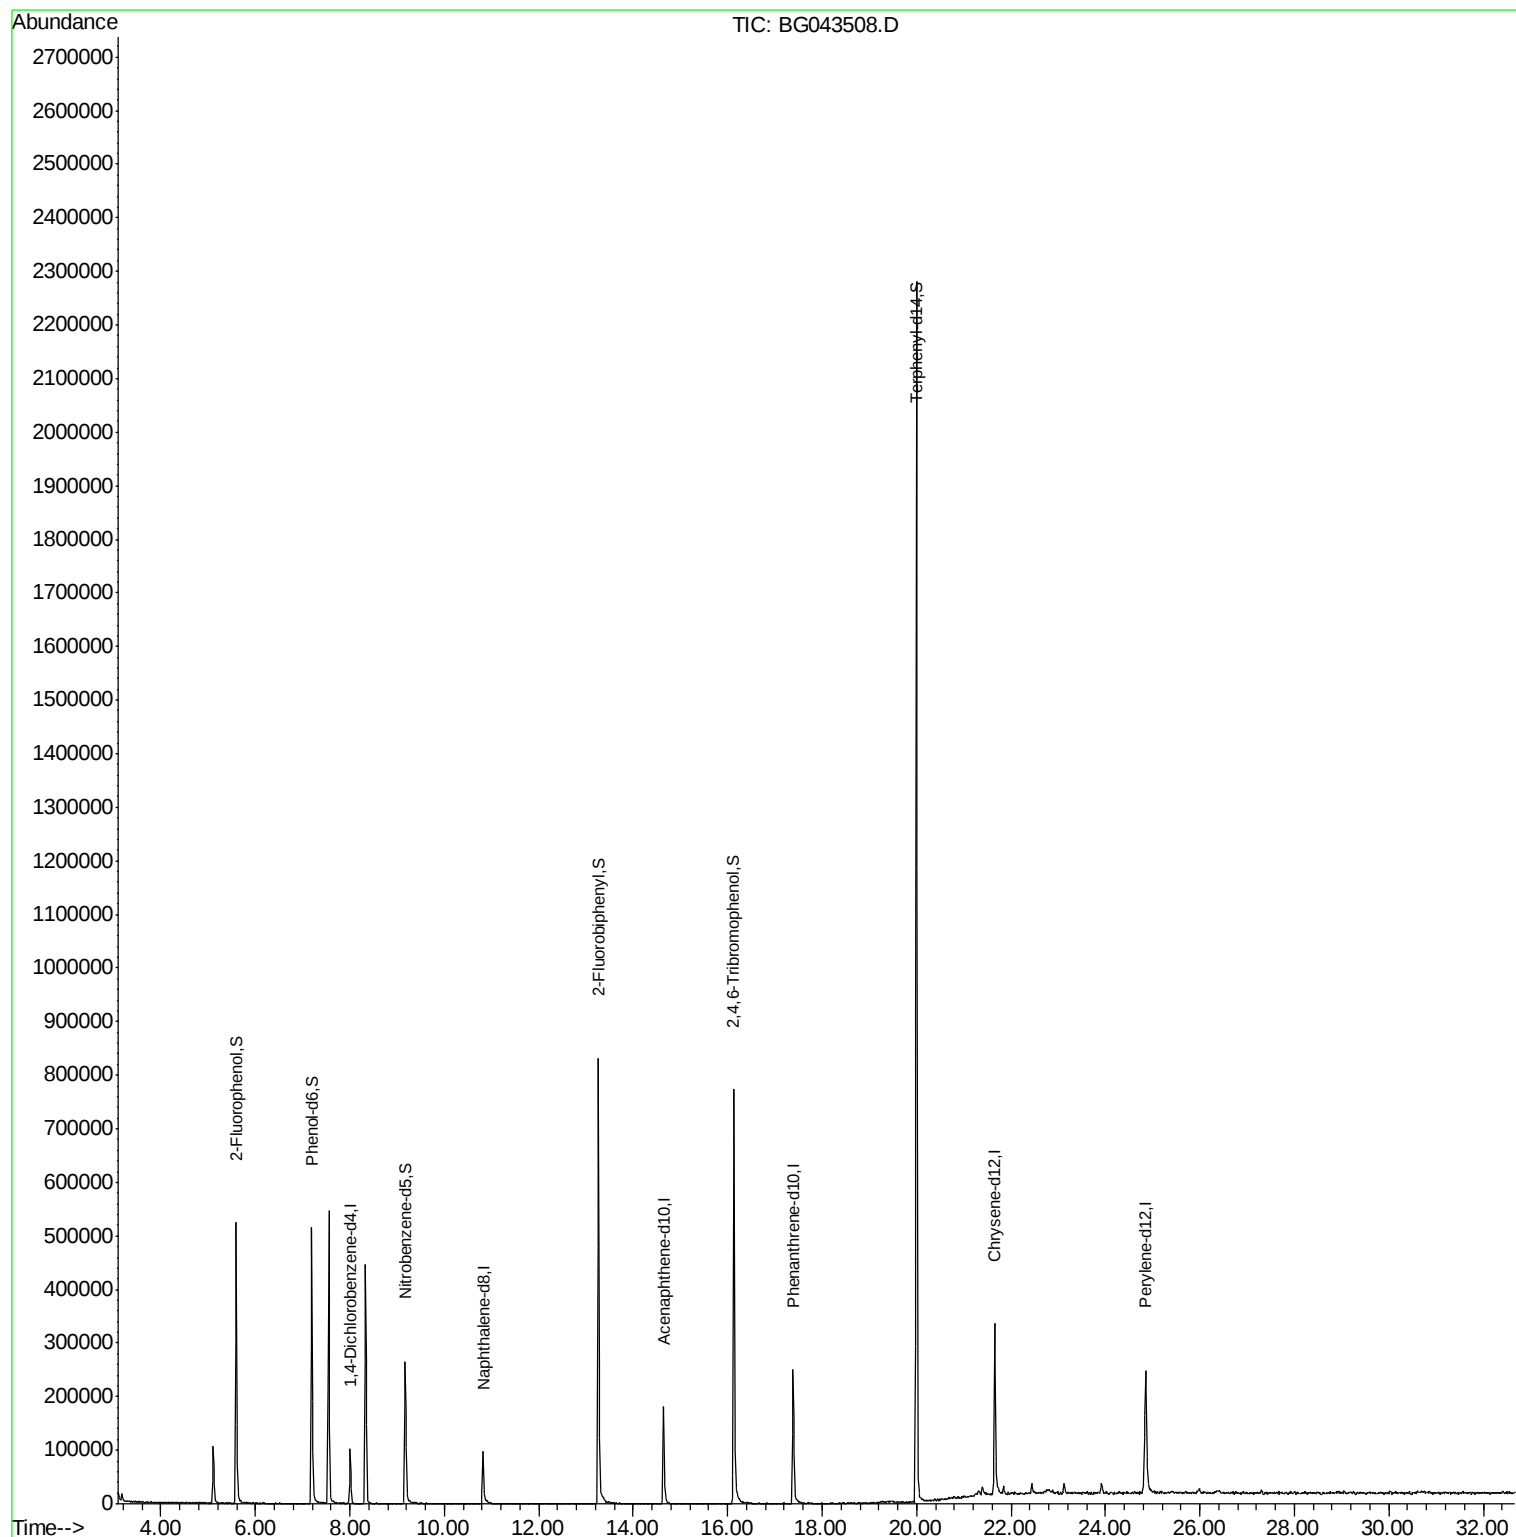




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 838
Delta R.T. 0.00 min
Lab File: BG043508.D
Acq: 5 Nov 2019 15:15

Instrument :
BNA_G
ClientSampleId :
PB124558BL

Tot Ion:152 Resp: 32007
Ion Ratio Lower Upper
152 100
150 138.6 129.4 194.0
115 48.7 48.8 73.2#

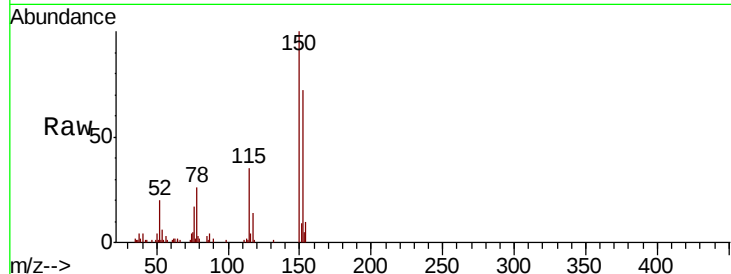


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

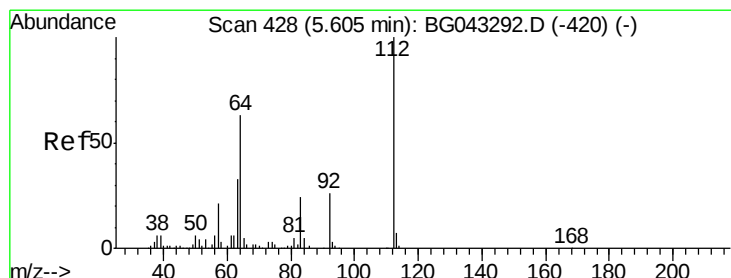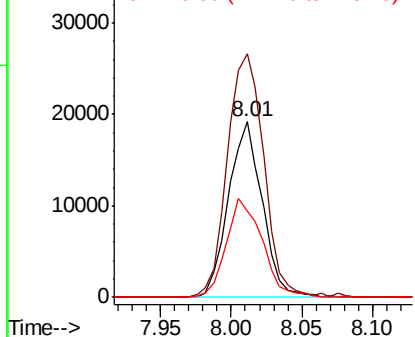



#5

2-Fluorophenol
Concen: 140.548 ng
RT: 5.60 min Scan# 427
Delta R.T. 0.00 min
Lab File: BG043508.D
Acq: 5 Nov 2019 15:15

Tgt Ion:112 Resp: 245493
Ion Ratio Lower Upper
112 100
64 61.7 50.0 75.0
63 35.3 26.6 40.0

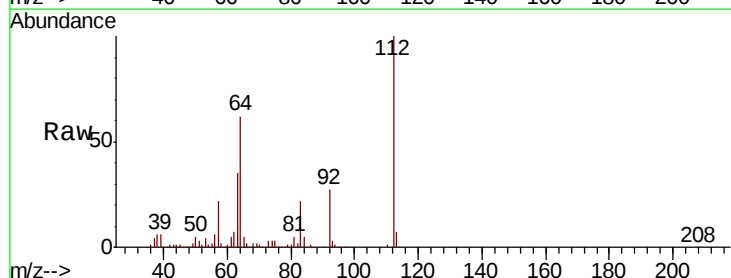

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

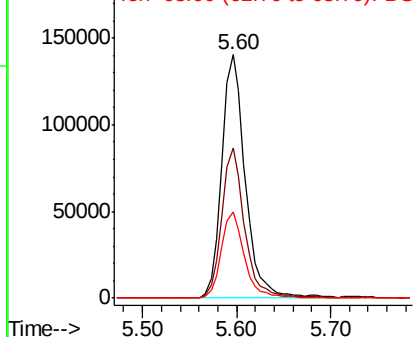



#7

Phenol-d6

Concen: 132.888 ng

RT: 7.19 min Scan# 699

Delta R.T. -0.00 min

Lab File: BG043508.D

Acq: 5 Nov 2019 15:15

Instrument :

BNA_G

ClientSampleId :

PB124558BL


Tot Ion: 99 Resp: 333955

Ion Ratio Lower Upper




99 100

42 16.7 14.6 21.8

71 40.2 32.5 48.7

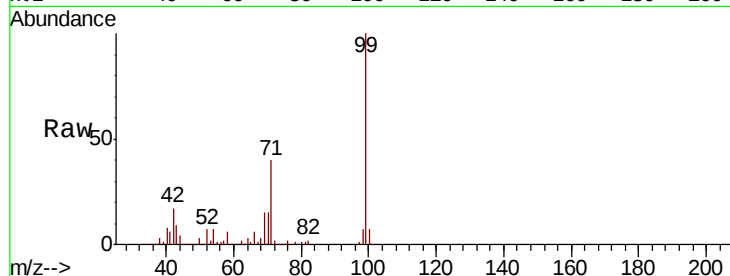

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

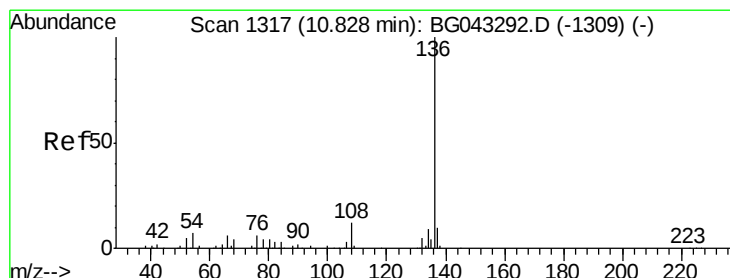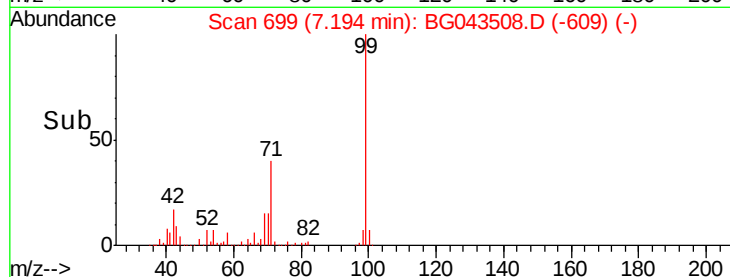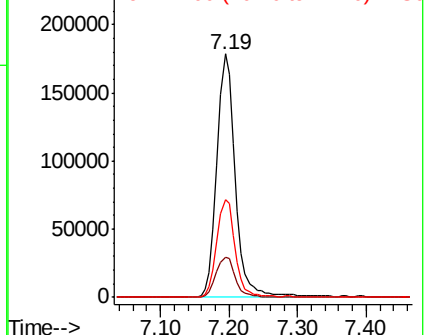

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. 0.00 min

Lab File: BG043508.D

Acq: 5 Nov 2019 15:15

Tgt Ion: 136 Resp: 107938


Ion Ratio Lower Upper

136 100



137 11.0 8.7 13.1


54 7.5 5.4 8.2

68 5.4 3.0 4.4#

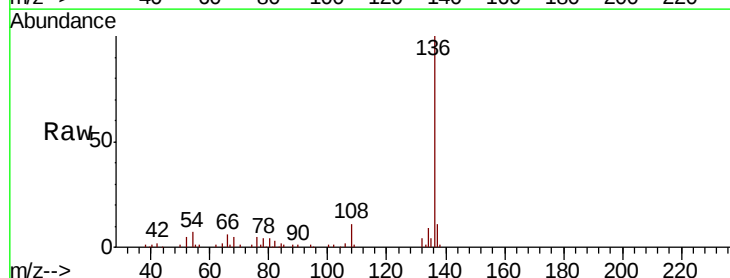

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



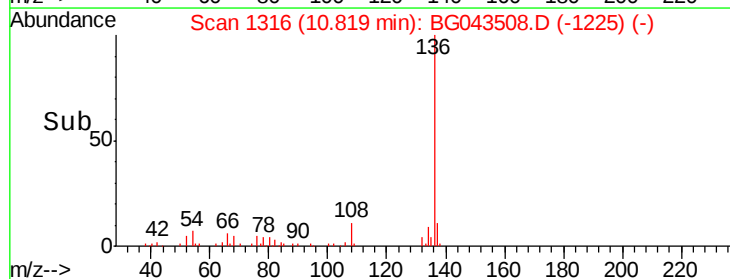
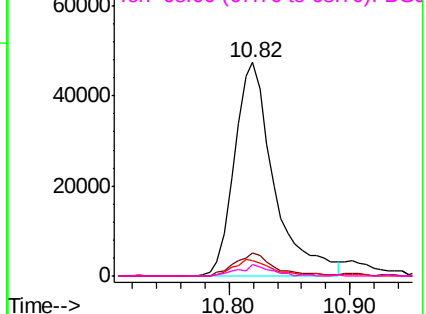




#23
Nitrobenzene-d5
Concen: 92.171 ng
RT: 9.17 min Scan# 1036
Delta R.T. -0.00 min
Lab File: BG043508.D
Acq: 5 Nov 2019 15:15




Instrument :
BNA_G
ClientSampleId :
PB124558BL


Tot Ion: 82 Resp: 192976
Ion Ratio Lower Upper
82 100
128 42.4 35.0 52.6
54 48.6 40.2 60.2

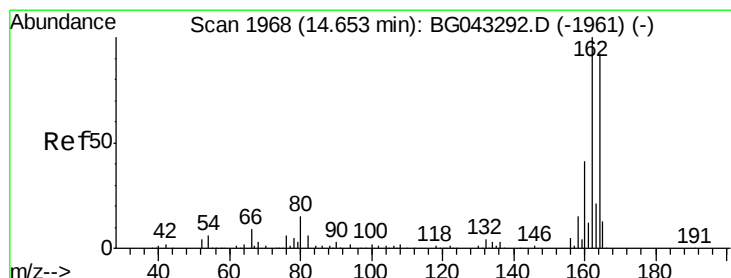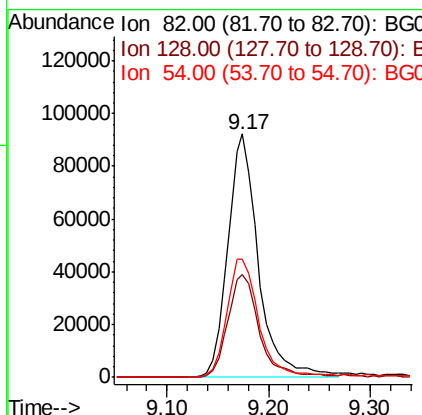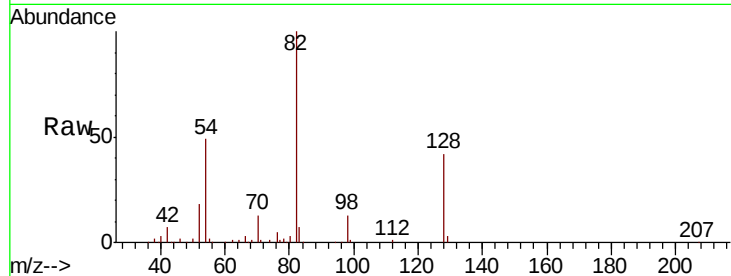

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.64 min Scan# 1966
Delta R.T. -0.00 min
Lab File: BG043508.D
Acq: 5 Nov 2019 15:15

Tgt Ion:164 Resp: 80156
Ion Ratio Lower Upper
164 100
162 109.4 83.5 125.3
160 42.8 36.5 54.7

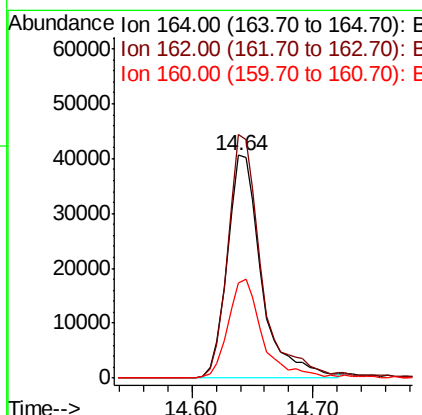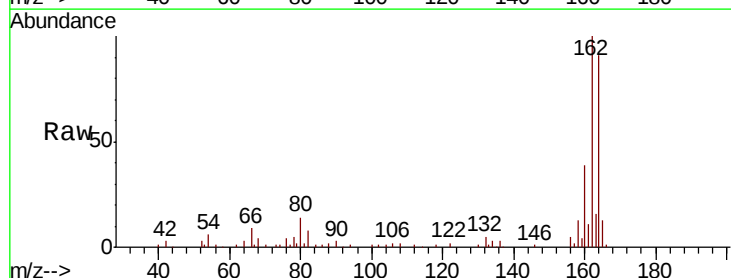







#42
 2,4,6-Tribromophenol
 Concen: 139.460 ng
 RT: 16.13 min Scan# 2220
 Delta R.T. -0.00 min
 Lab File: BG043508.D
 Acq: 5 Nov 2019 15:15

Instrument :
 BNA_G
 ClientSampleId :
 PB124558BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.5	77.4	116.0
141	27.0	22.8	34.2

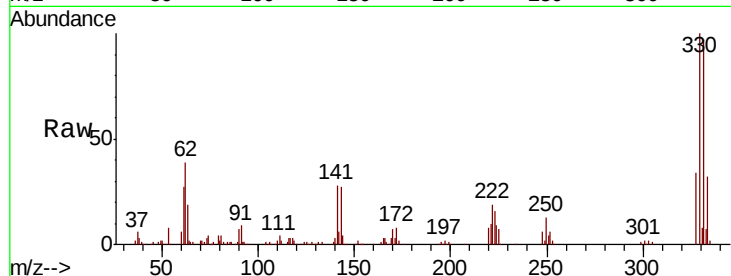


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

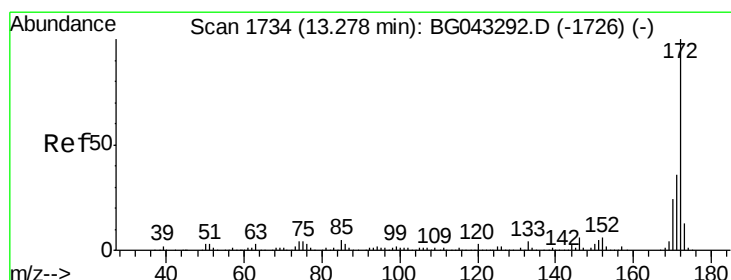
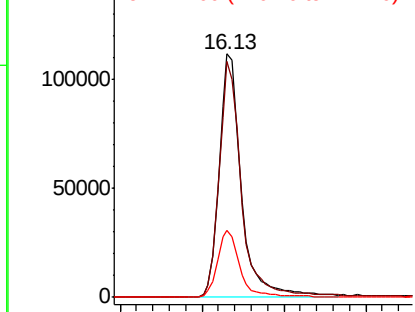



#45
 2-Fluorobiphenyl
 Concen: 92.109 ng
 RT: 13.26 min Scan# 1732
 Delta R.T. -0.00 min
 Lab File: BG043508.D
 Acq: 5 Nov 2019 15:15

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	28.9	43.3
170	22.4	18.5	27.7

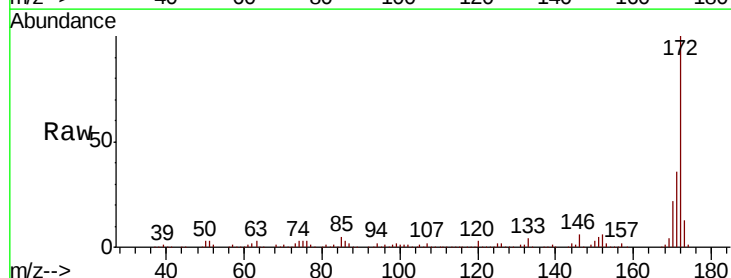

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

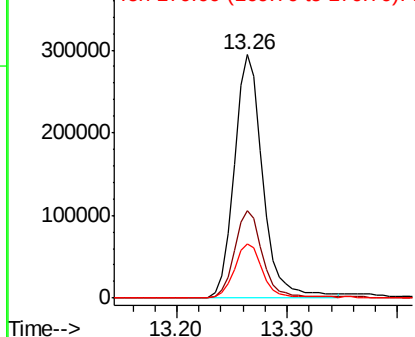

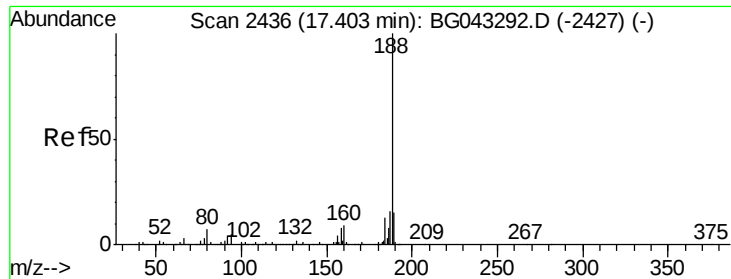

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.39 min Scan# 2434

Delta R.T. -0.00 min

Lab File: BG043508.D

Acq: 5 Nov 2019 15:15

Instrument :

BNA_G

ClientSampleId :

PB124558BL


Tot Ion:188 Resp: 211090

Ion Ratio Lower Upper

188 100

94 5.1 4.2 6.4




80 6.5 4.5 6.7

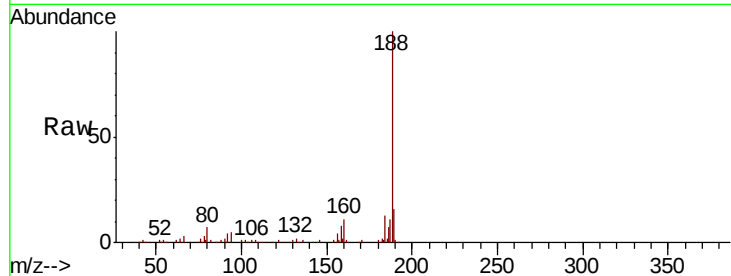

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

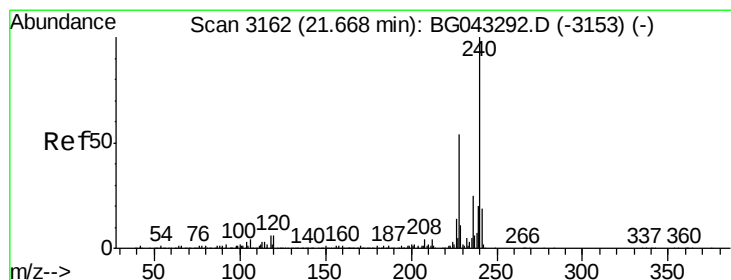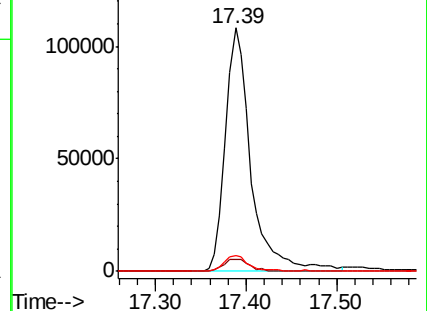

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.65 min Scan# 3160

Delta R.T. -0.00 min

Lab File: BG043508.D

Acq: 5 Nov 2019 15:15


Tgt Ion:240 Resp: 245217

Ion Ratio Lower Upper

240 100

120 6.3 4.6 6.8



236 25.5 19.8 29.8

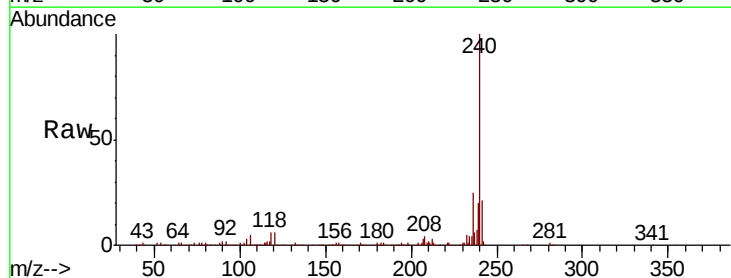


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

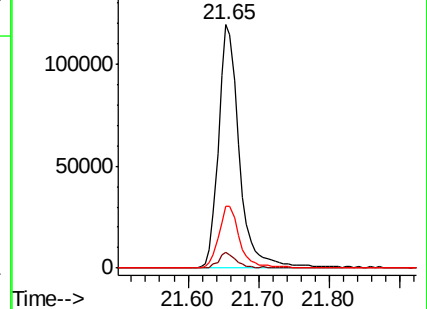







#79
 Terphenyl-d14
 Concen: 98.635 ng
 RT: 20.00 min Scan# 2878
 Delta R.T. -0.00 min
 Lab File: BG043508.D
 Acq: 5 Nov 2019 15:15

Instrument :
 BNA_G
 ClientSampleId :
 PB124558BL

Tot Ion:244 Resp: 1289243
 Ion Ratio Lower Upper
 244 100
 212 7.5 5.8 8.6
 122 7.3 5.4 8.2

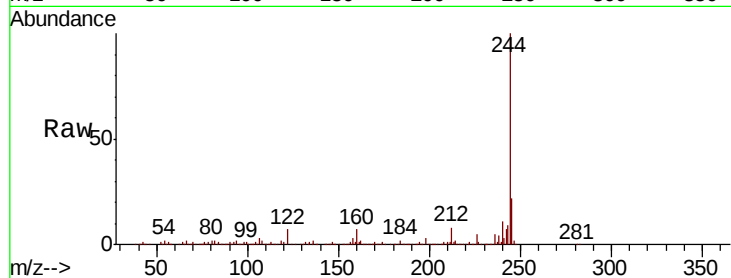


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

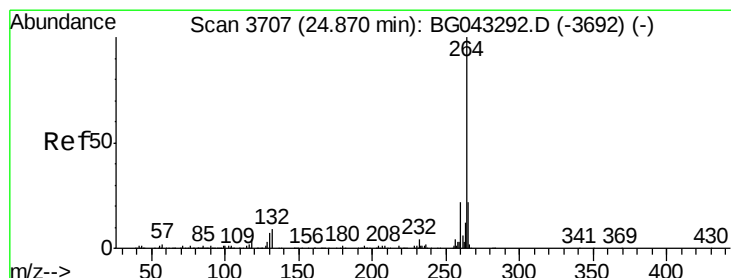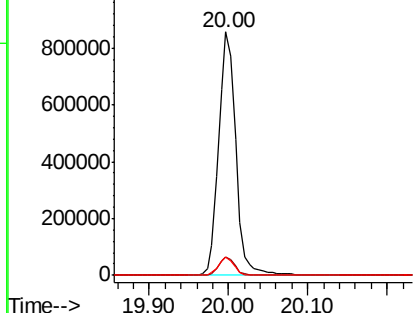

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.85 min Scan# 3704
 Delta R.T. -0.00 min
 Lab File: BG043508.D
 Acq: 5 Nov 2019 15:15

Tgt Ion:264 Resp: 289644
 Ion Ratio Lower Upper
 264 100
 260 23.1 17.5 26.3
 265 21.5 17.4 26.0

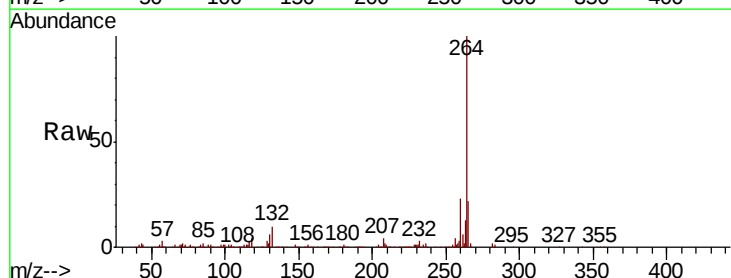

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

