


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110519\
 Data File : BG043500.D
 Acq On : 5 Nov 2019 10:08
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

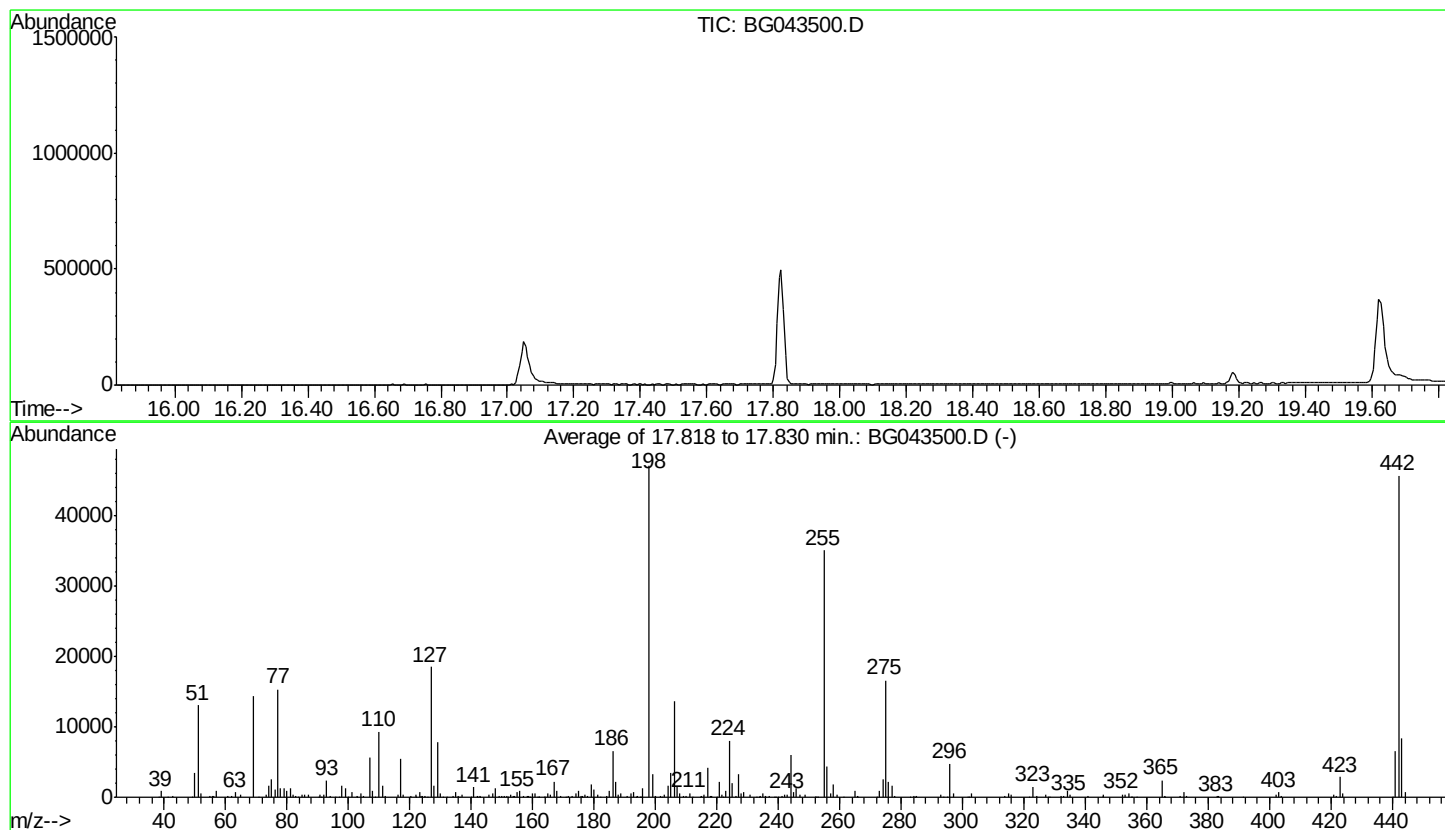

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	13073	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.6	14401	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.2	18456	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47074	PASS
199	198	5	9	7.1	3338	PASS
275	198	10	60	35.2	16590	PASS
365	198	1	100	5.1	2403	PASS
441	198	0.01	100	13.9	6544	PASS
442	198	50	100	97.0	45645	PASS
443	442	15	24	18.3	8354	PASS