
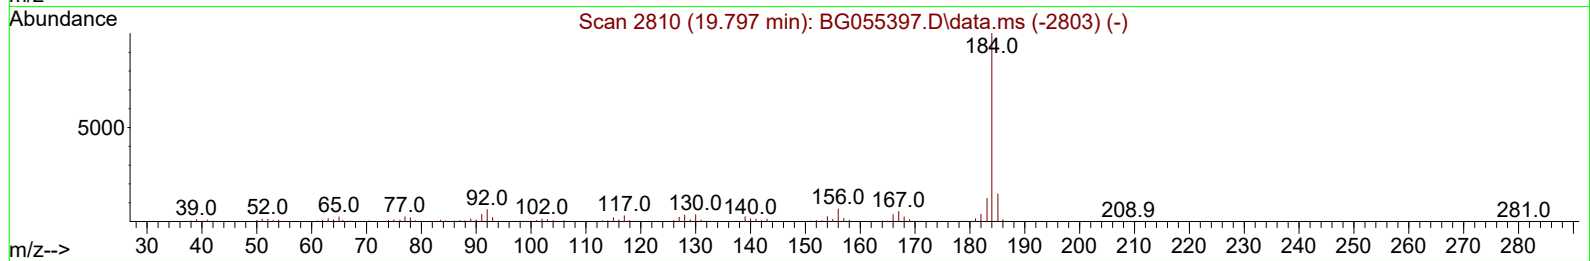
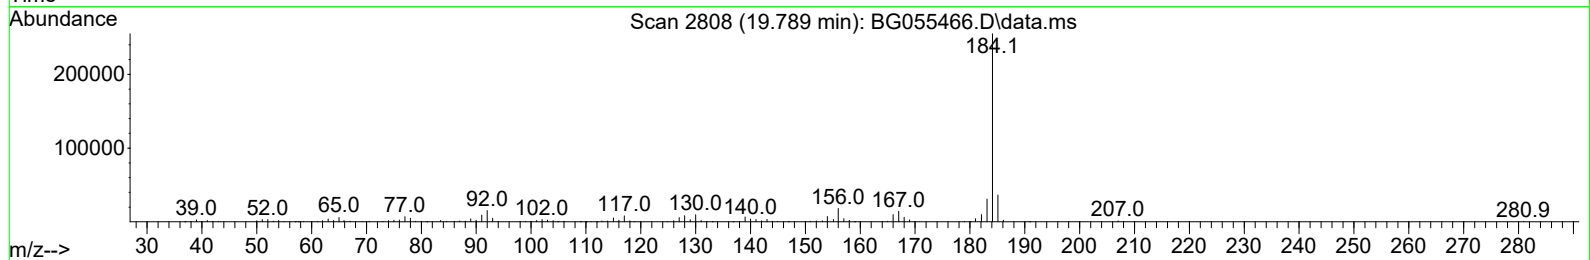


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110522\
Data File : BG055466.D
Acq On : 5 Nov 2022 11:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 12:27:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

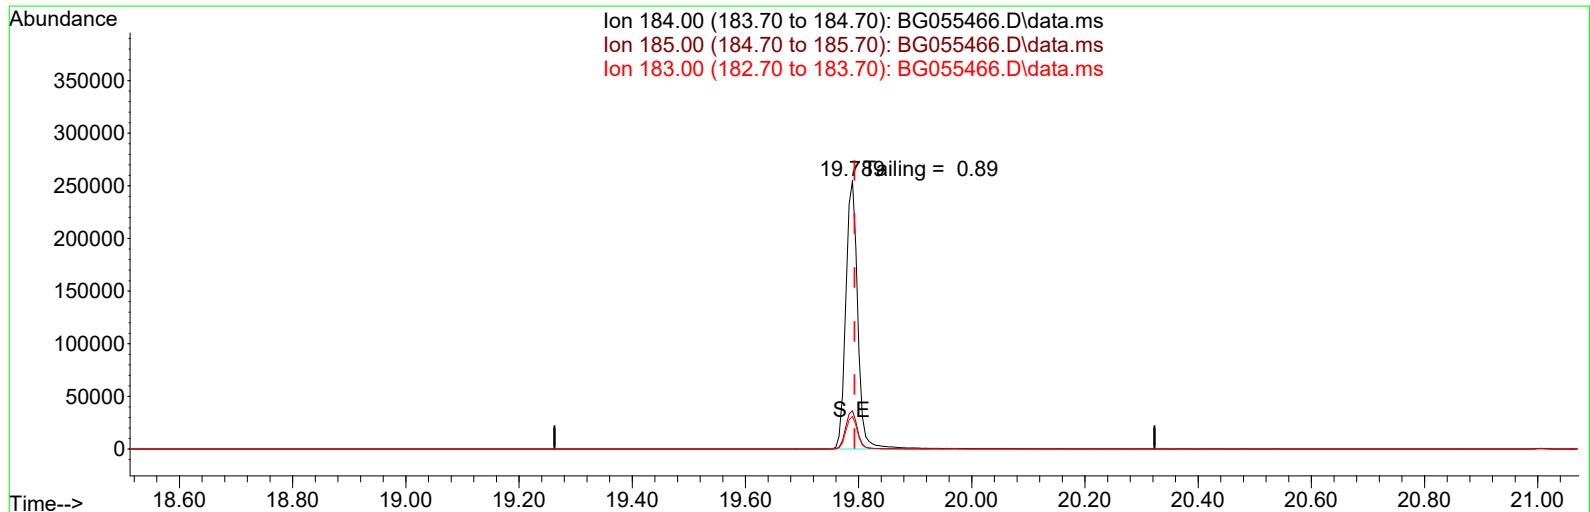

TIC: BG055466.D\data.ms

(77) Benzidine




19.789min (-0.004) 0.00 ng

response 370984

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.29
183.00	12.30	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110522\
Data File : BG055466.D
Acq On : 5 Nov 2022 11:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 12:27:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

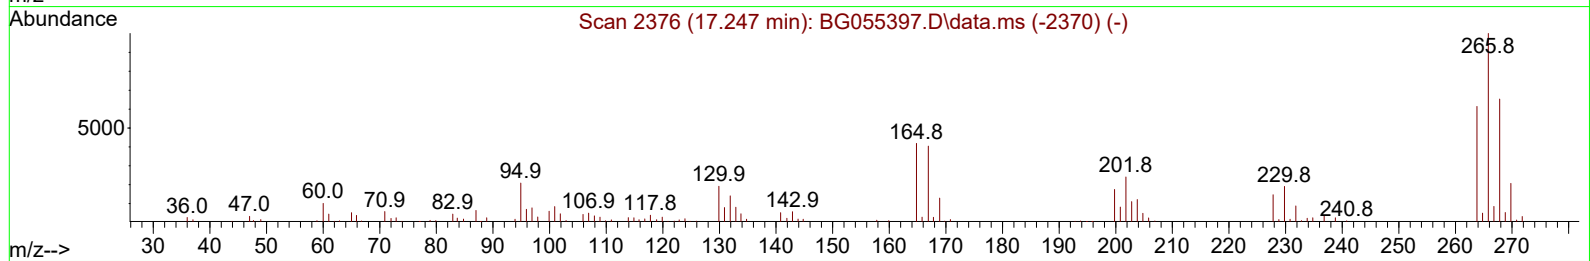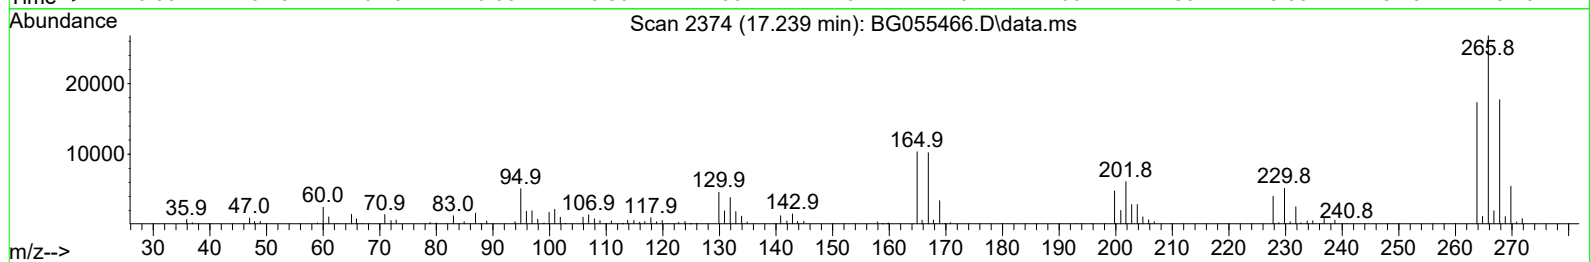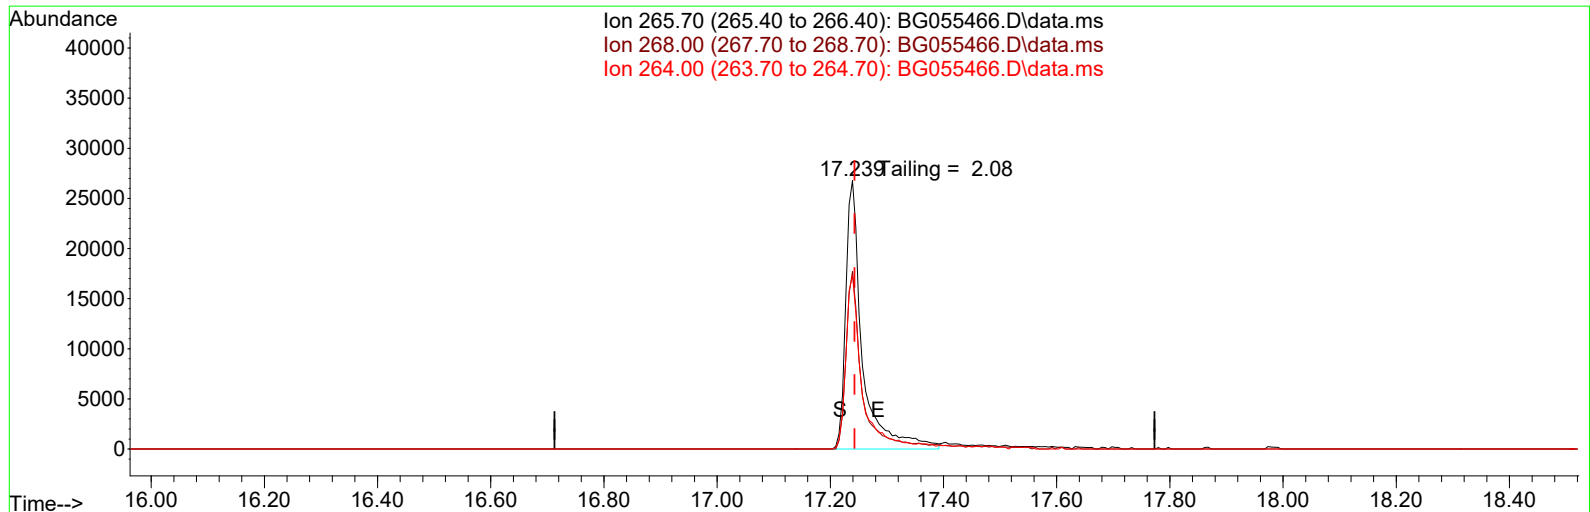

TIC: BG055466.D\data.ms

(70) Pentachlorophenol (C)

17.239min (-0.004) 47995.62 ng

response 55211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	66.15
264.00	61.50	64.74
0.00	0.00	0.00