


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110522\
 Data File : BG055466.D
 Acq On : 5 Nov 2022 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:51:08 2022

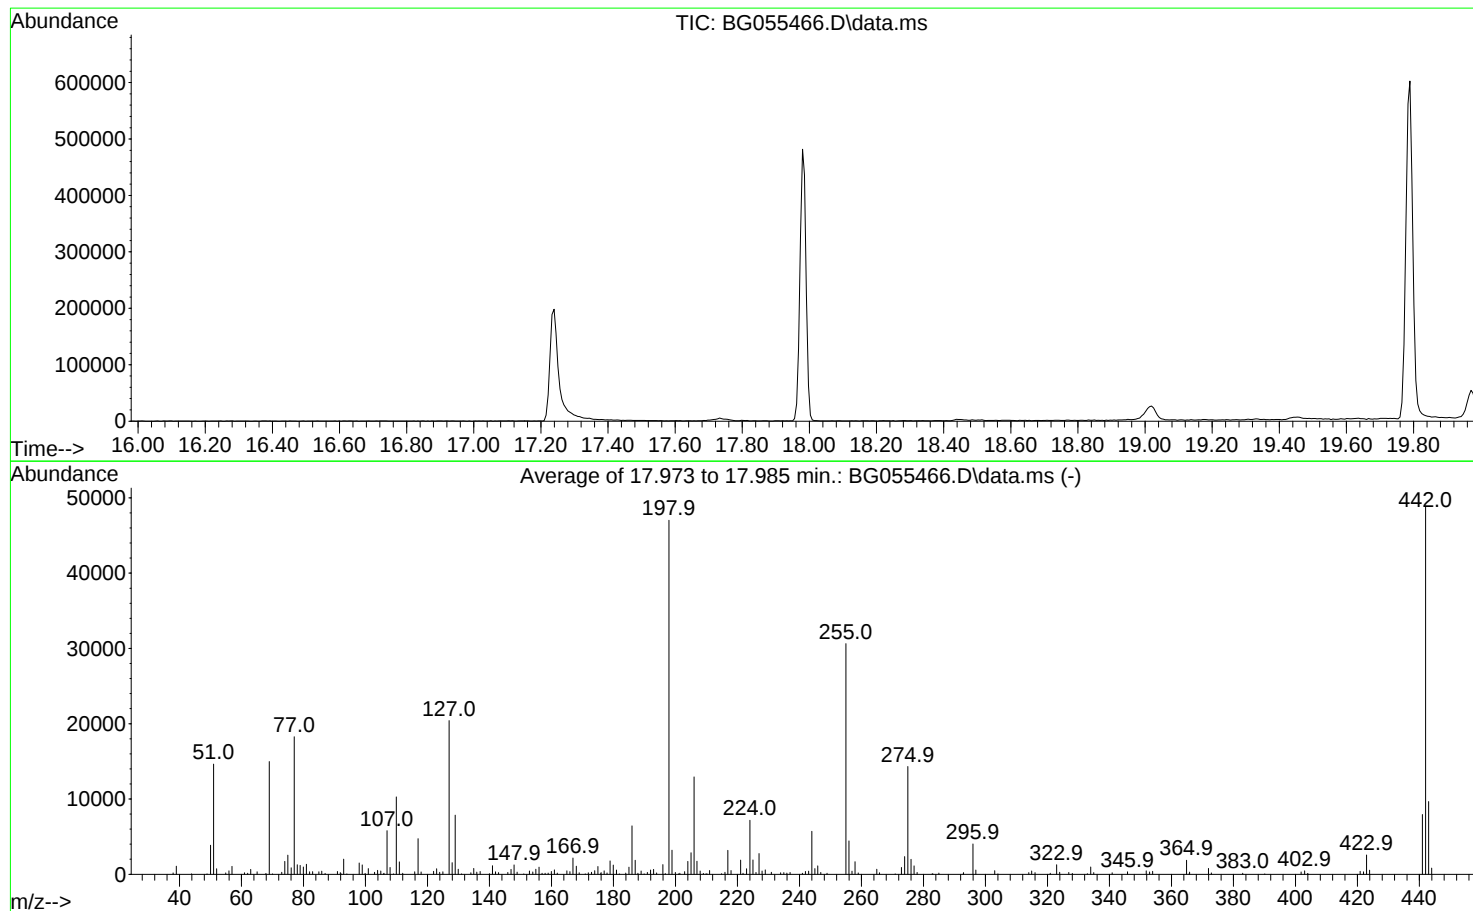




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	14632	PASS
68	69	0.00	2	0.8	127	PASS
69	198	0.00	100	31.8	14976	PASS
70	69	0.00	2	0.4	57	PASS
127	198	10	80	43.4	20421	PASS
197	198	0.00	2	0.2	102	PASS
198	198	100	100	100.0	47027	PASS
199	198	5	9	6.8	3197	PASS
275	198	10	60	30.5	14324	PASS
365	198	1	100	4.0	1858	PASS
441	198	0.01	100	16.9	7937	PASS
442	442	50	100	100.0	48864	PASS
443	442	15	24	19.8	9652	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110522\
 Data File : BG055466.D
 Acq On : 5 Nov 2022 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 05 12:27:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 05:28:43 2022
 Response via : Initial Calibration

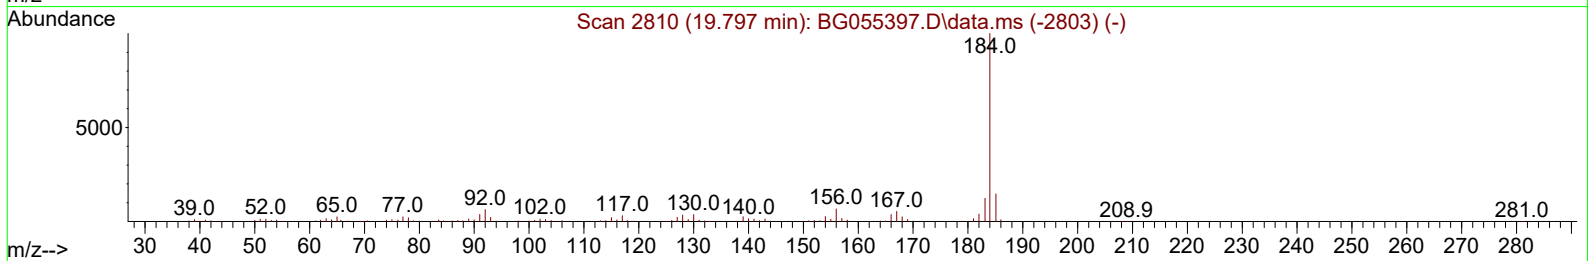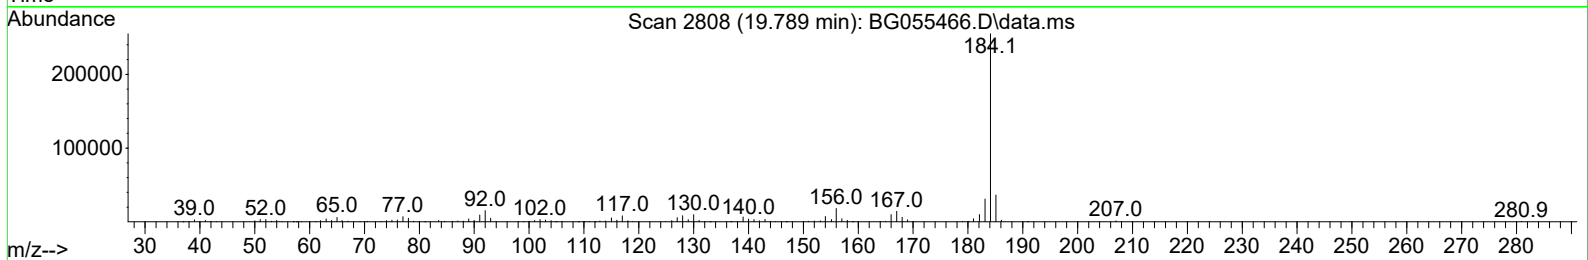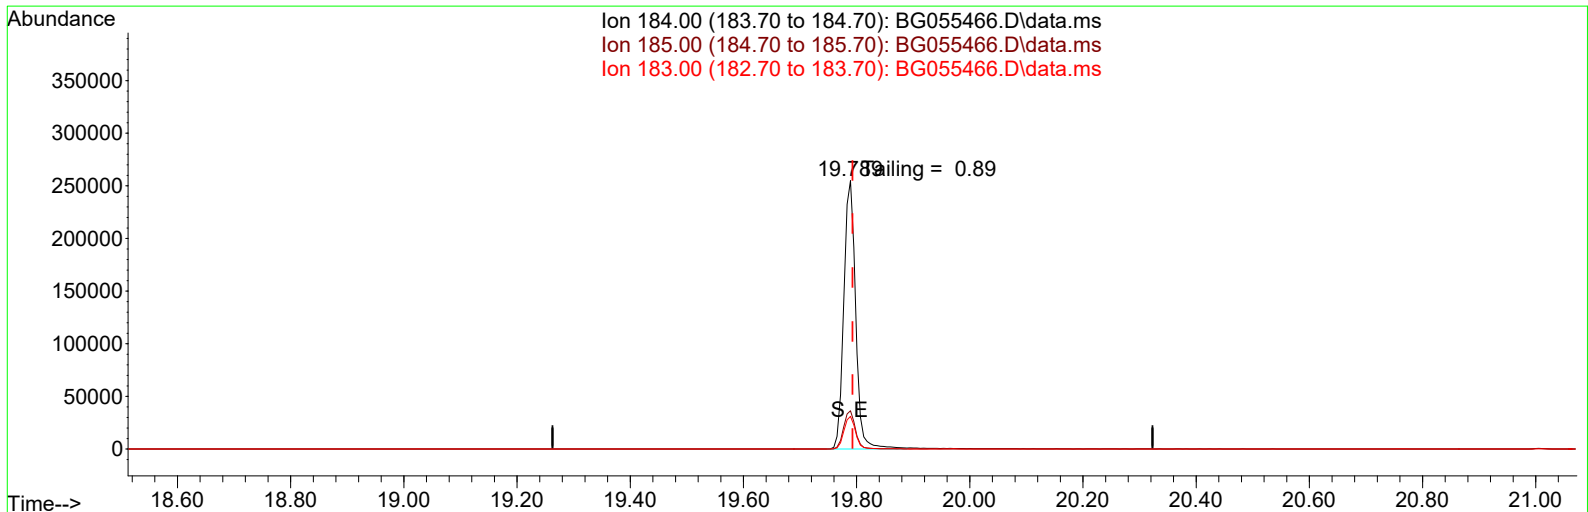

TIC: BG055466.D\data.ms

(77) Benzidine

19.789min (-0.004) 0.00 ng




response 370984

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.29
183.00	12.30	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110522\
 Data File : BG055466.D
 Acq On : 5 Nov 2022 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 05 12:27:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 05:28:43 2022
 Response via : Initial Calibration

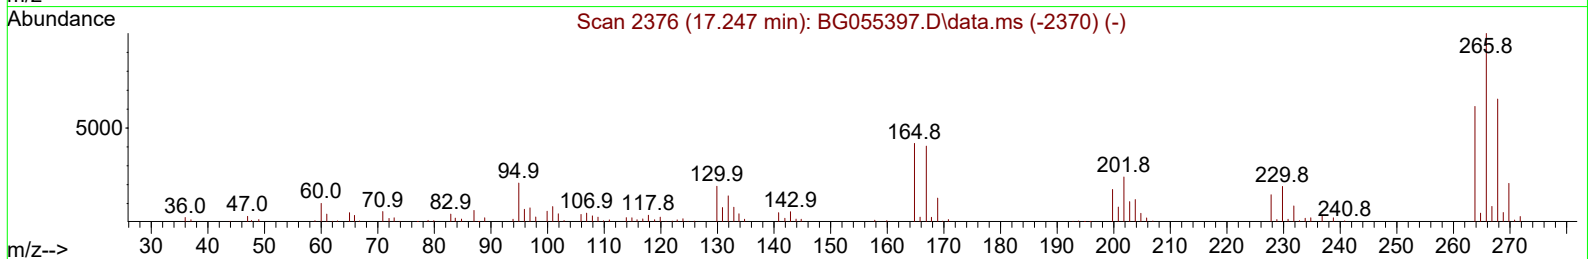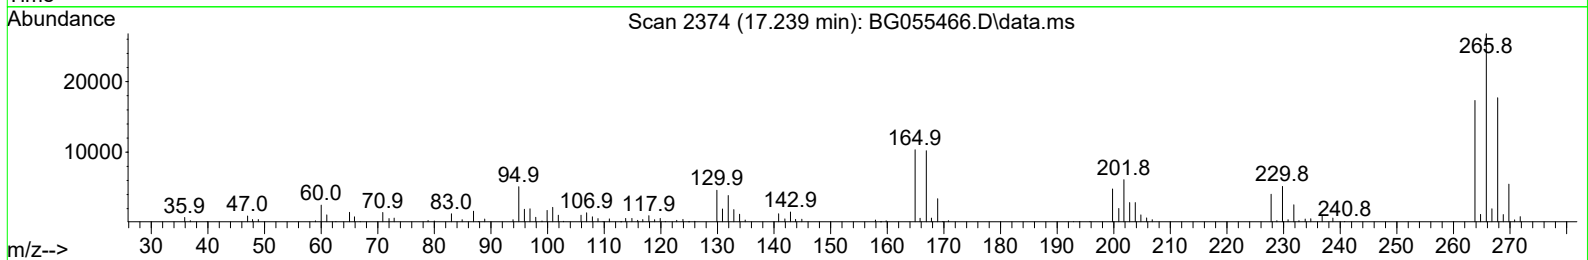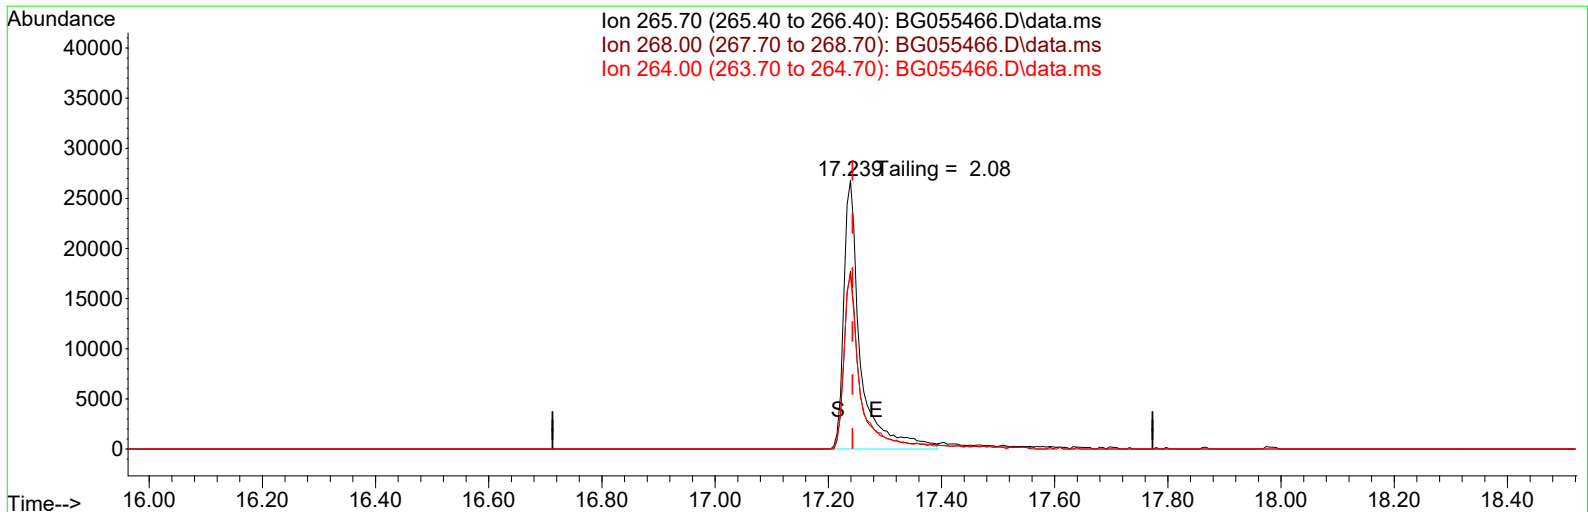

TIC: BG055466.D\data.ms

(70) Pentachlorophenol (C)

17.239min (-0.004) 47995.62 ng

response 55211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	66.15
264.00	61.50	64.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/5/2022	BNA_G	<u>BG055466.D</u>
Compound Name	Response	Retention Time
DDT	178656	21.005
DDD	2235	20.612
DDE	69	20.065
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2304	180960	1.27

Instrument :
BNA_G
ClientSampleId :
DFTPP