
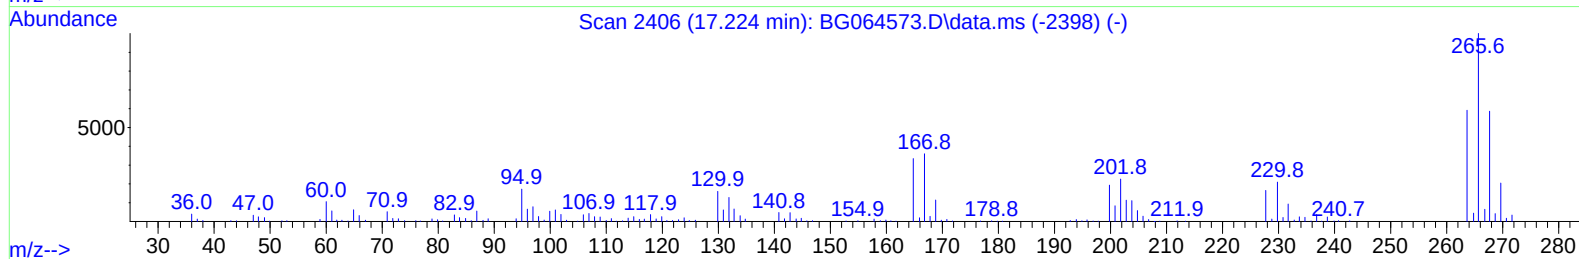
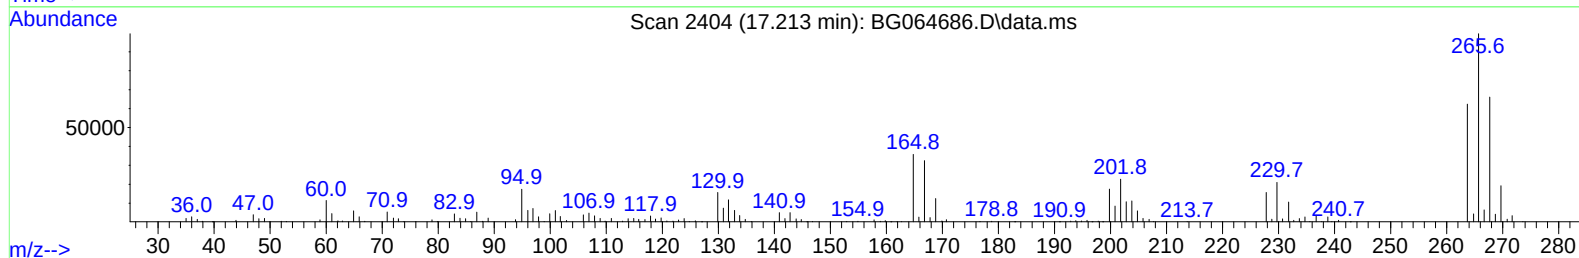


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064686.D
Acq On : 5 Nov 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 15:34:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

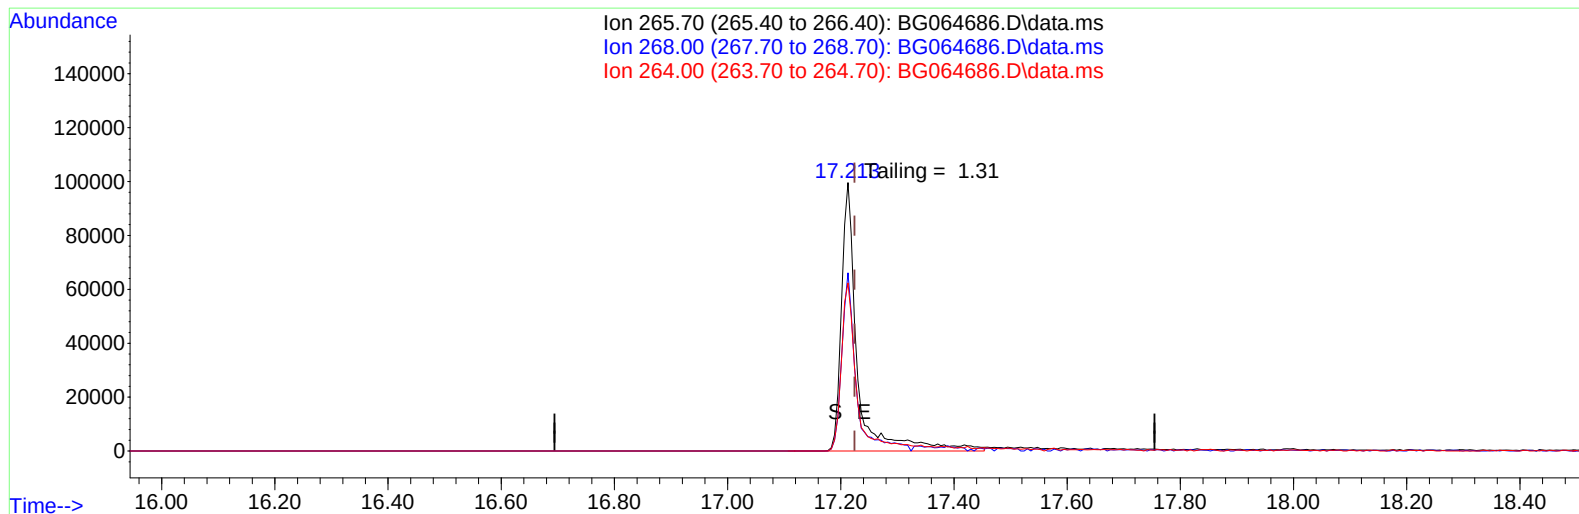

TIC: BG064686.D\data.ms

(70) Pentachlorophenol (C)




17.213min (-0.012) 114892.15 ng

response 187907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	70.51
264.00	59.10	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064686.D
Acq On : 5 Nov 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 15:34:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

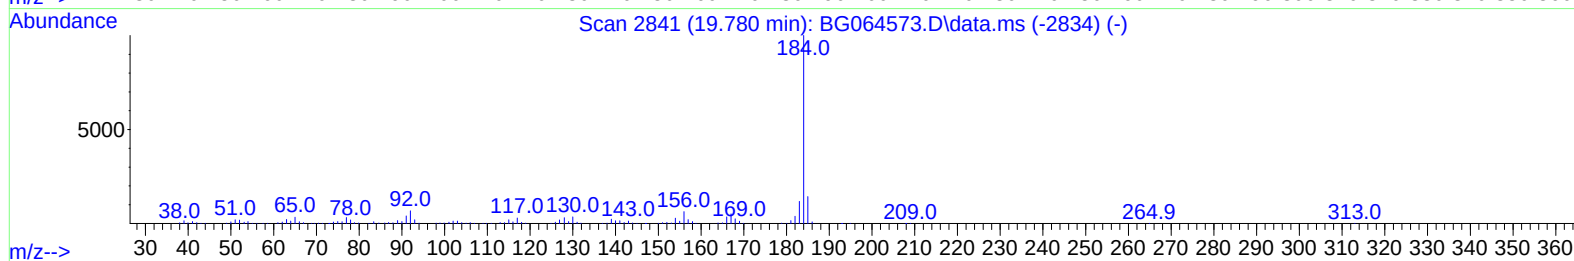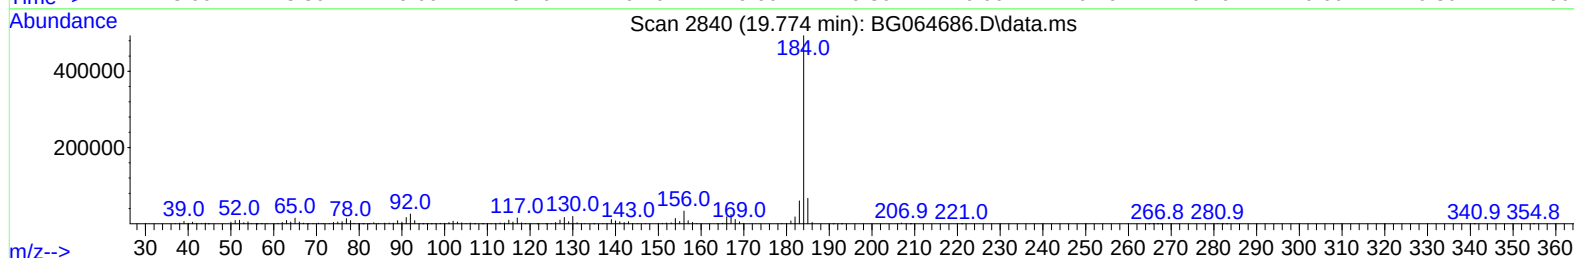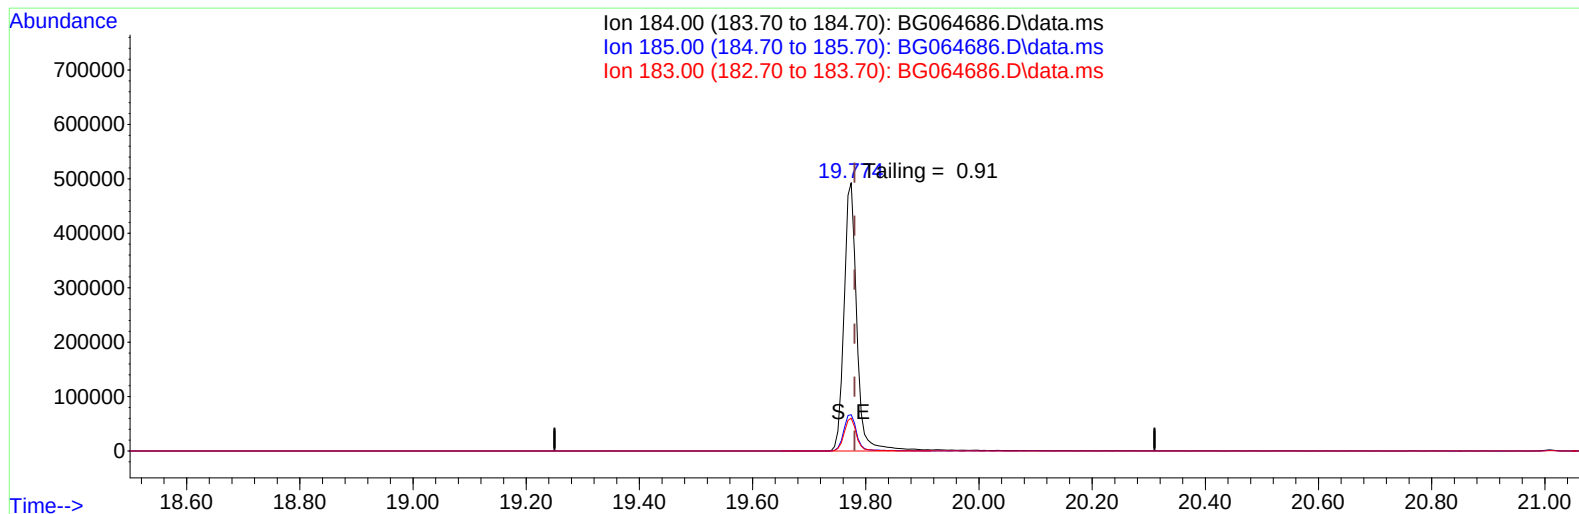

TIC: BG064686.D\data.ms

(77) Benzidine

19.774min (-0.006) 30048.03 ng

response 773507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.55
183.00	11.80	12.24
0.00	0.00	0.00