

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
 Data File : BG064688.D
 Acq On : 5 Nov 2025 16:40
 Operator : RC/JU
 Sample : PB170325BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB170325BL

Quant Time: Nov 05 17:28:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 03 18:16:26 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.206	152	21793	20.000	ng	-0.02
21) Naphthalene-d8	11.032	136	87361	20.000	ng	-0.02
39) Acenaphthene-d10	14.827	164	87640	20.000	ng	-0.02
64) Phenanthrene-d10	17.565	188	303868	20.000	ng	-0.02
76) Chrysene-d12	21.837	240	367288	20.000	ng	#-0.02
86) Perylene-d12	25.168	264	367617	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.738	112	195231	150.367	ng	-0.01
7) Phenol-d6	7.342	99	272999	153.230	ng	-0.01
23) Nitrobenzene-d5	9.363	82	156148	107.355	ng	-0.02
42) 2,4,6-Tribromophenol	16.308	330	279538	220.995	ng	-0.01
45) 2-Fluorobiphenyl	13.458	172	511729	88.504	ng	-0.02
79) Terphenyl-d14	20.156	244	2038037	104.717	ng	-0.02


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064688.D
Acq On : 5 Nov 2025 16:40
Operator : RC/JU
Sample : PB170325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170325BL


Quant Time: Nov 05 17:28:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

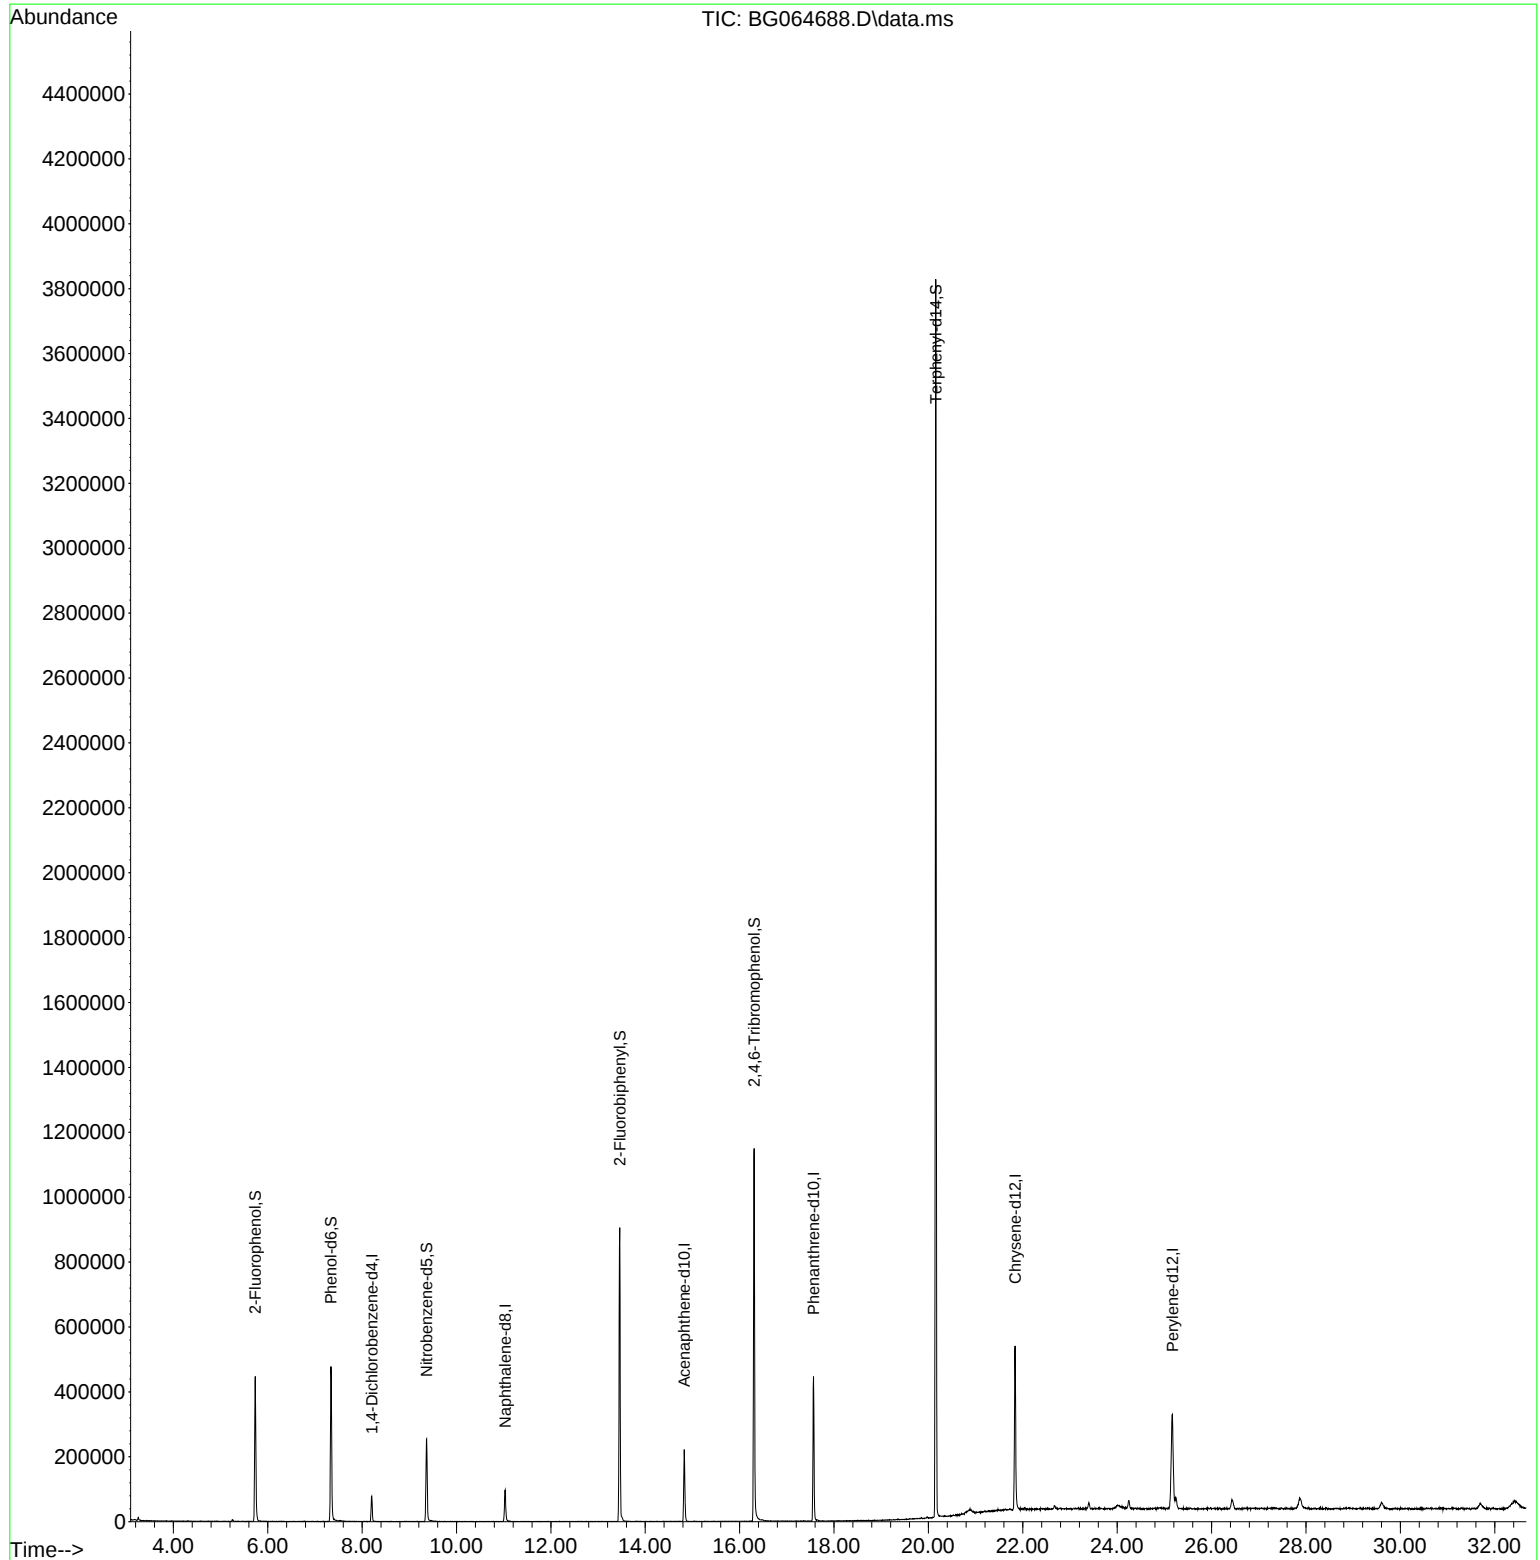



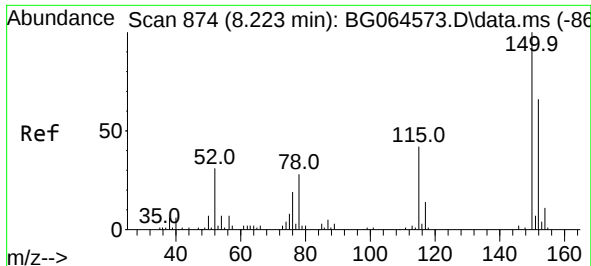


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.206 min Scan# 81
Delta R.T. -0.017 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40

Instrument :
BNA_G
ClientSampleId :
PB170325BL



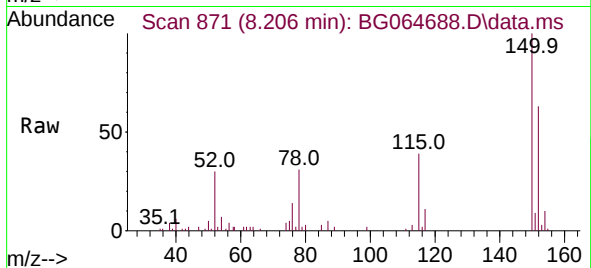



Tgt Ion:152 Resp: 21793
Ion Ratio Lower Upper
152 100
150 158.2 122.2 183.4
115 61.1 50.8 76.2

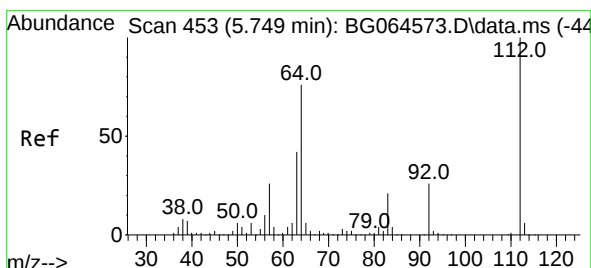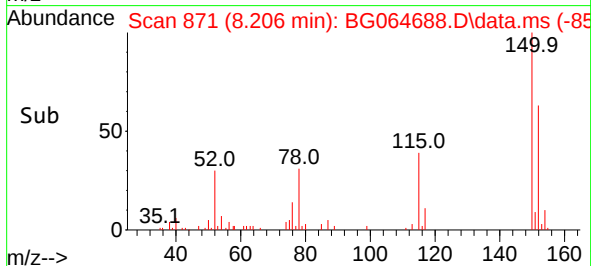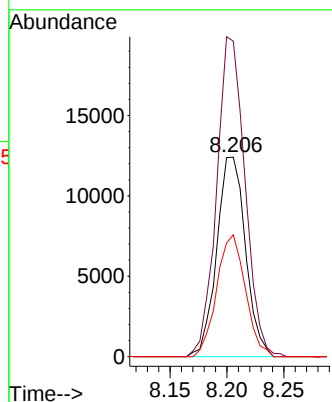

#5
2-Fluorophenol
Concen: 150.367 ng
RT: 5.738 min Scan# 451
Delta R.T. -0.011 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40

Tgt Ion:112 Resp: 195231
Ion Ratio Lower Upper
112 100
64 72.7 60.7 91.1
63 42.1 33.4 50.0


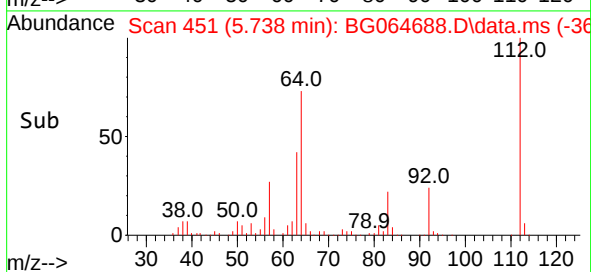
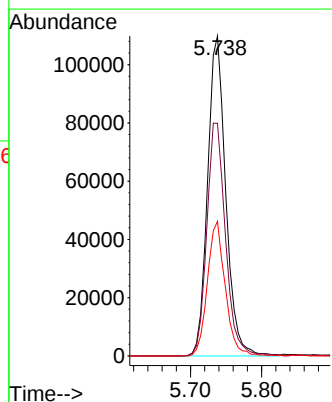
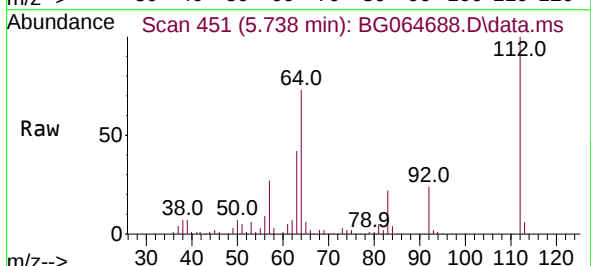


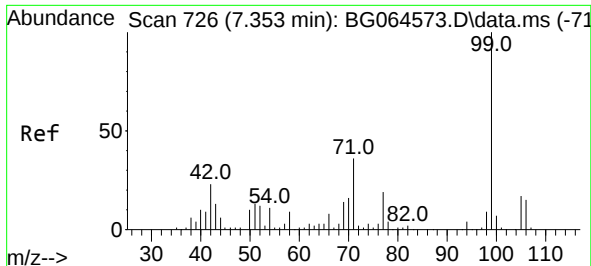

#7
Phenol-d6
Concen: 153.230 ng
RT: 7.342 min Scan# 71
Delta R.T. -0.011 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40




Instrument :
BNA_G
ClientSampleId :
PB170325BL


Tgt Ion: 99 Resp: 272999
Ion Ratio Lower Upper
99 100
42 25.0 18.3 27.5
71 39.3 28.6 43.0

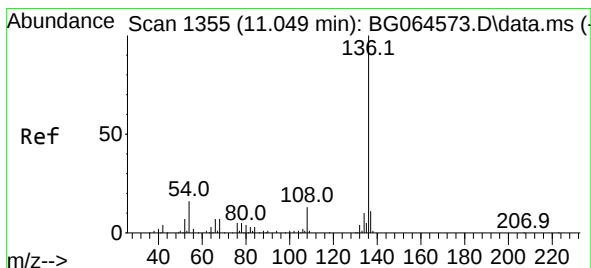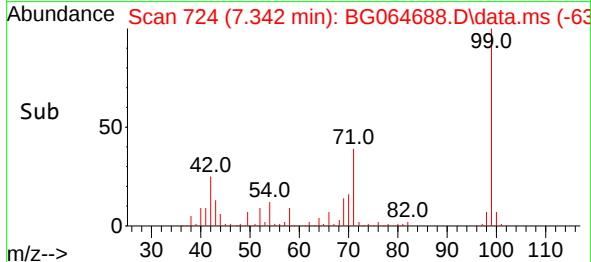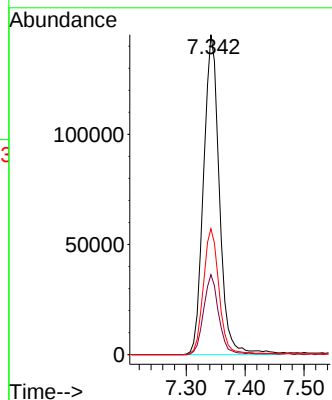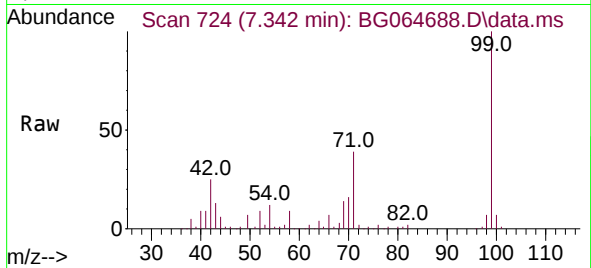

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.032 min Scan# 1352
Delta R.T. -0.017 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40

Tgt Ion:136 Resp: 87361
Ion Ratio Lower Upper
136 100
137 11.4 9.2 13.8
54 13.7 12.6 19.0
68 5.9 5.7 8.5


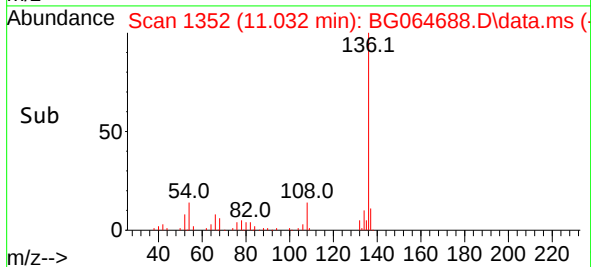
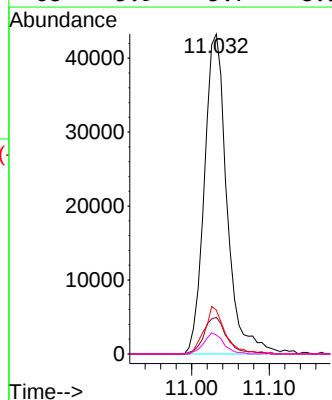
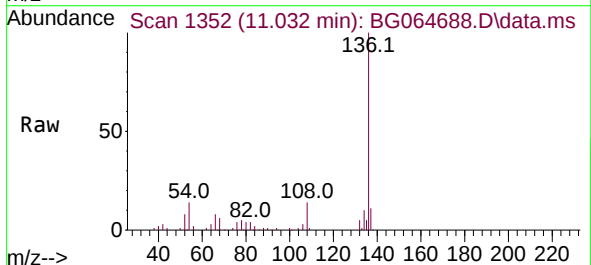


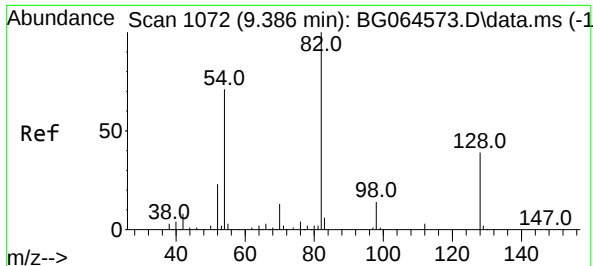

#23
Nitrobenzene-d5
Concen: 107.355 ng
RT: 9.363 min Scan# 1068
Delta R.T. -0.023 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40




Instrument :
BNA_G
ClientSampleId :
PB170325BL


Tgt Ion: 82 Resp: 156148
Ion Ratio Lower Upper
82 100
128 39.1 31.3 46.9
54 73.6 56.6 84.8

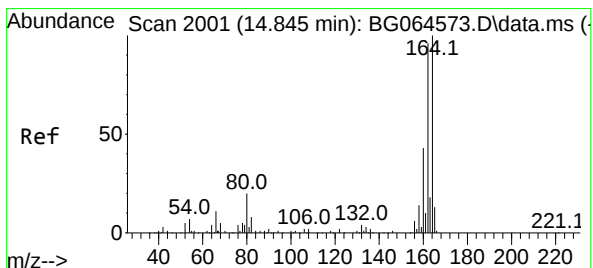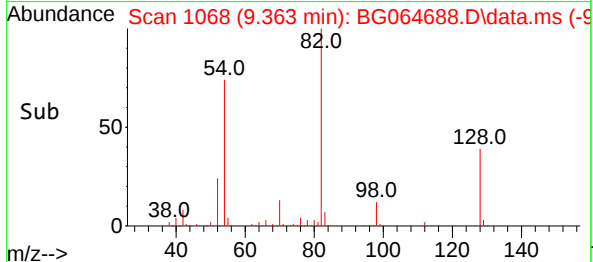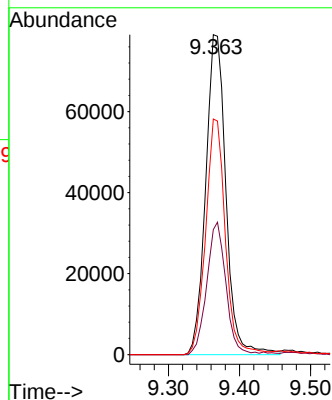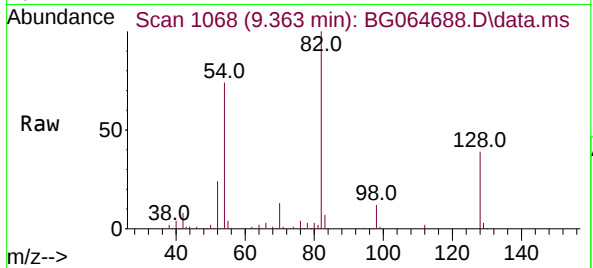

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.827 min Scan# 1998
Delta R.T. -0.017 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40

Tgt Ion: 164 Resp: 87640
Ion Ratio Lower Upper
164 100
162 101.9 77.0 115.6
160 43.9 34.4 51.6


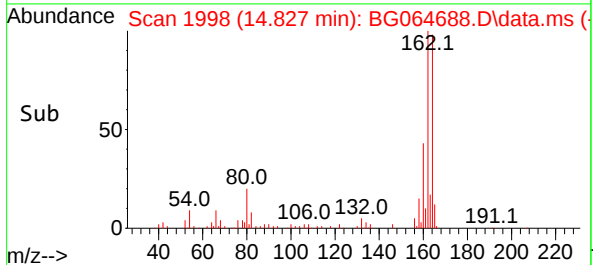
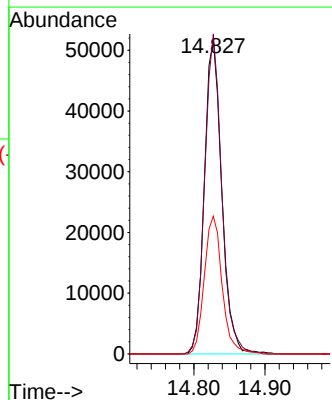
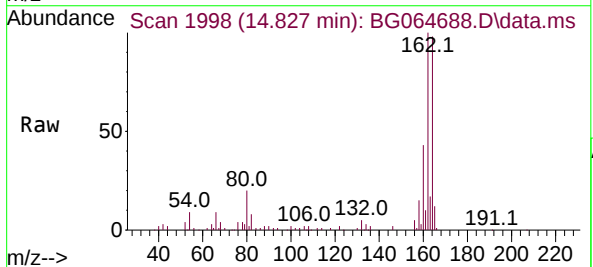


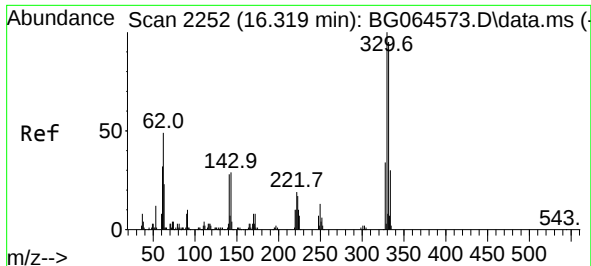

#42
2,4,6-Tribromophenol
Concen: 220.995 ng
RT: 16.308 min Scan# 21
Delta R.T. -0.011 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40




Instrument :
BNA_G
ClientSampleId :
PB170325BL


Tgt Ion:330 Resp: 279538
Ion Ratio Lower Upper
330 100
332 94.9 78.0 117.0
141 25.0 21.8 32.6

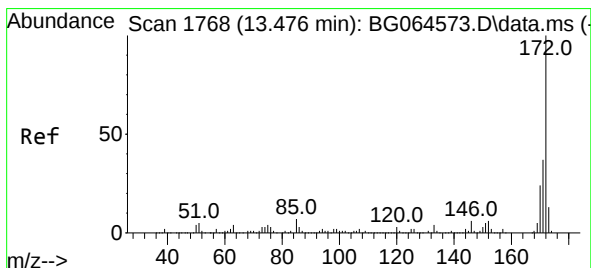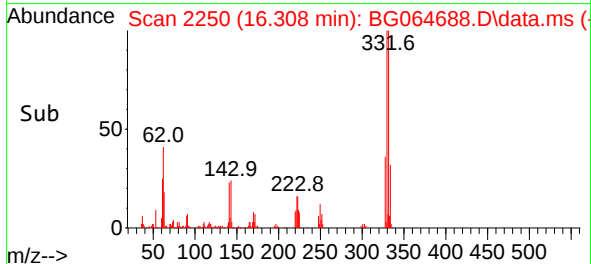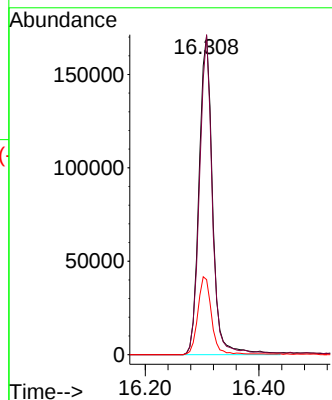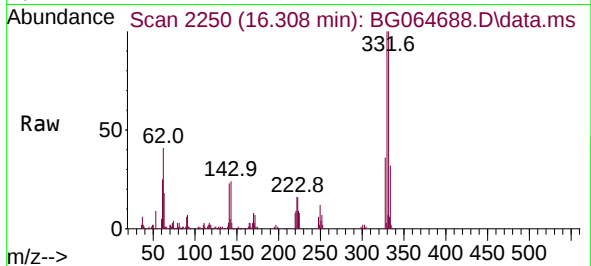

#45
2-Fluorobiphenyl
Concen: 88.504 ng
RT: 13.458 min Scan# 1765
Delta R.T. -0.017 min
Lab File: BG064688.D
Acq: 5 Nov 2025 16:40

Tgt Ion:172 Resp: 511729
Ion Ratio Lower Upper
172 100
171 36.6 29.4 44.0
170 24.5 19.1 28.7

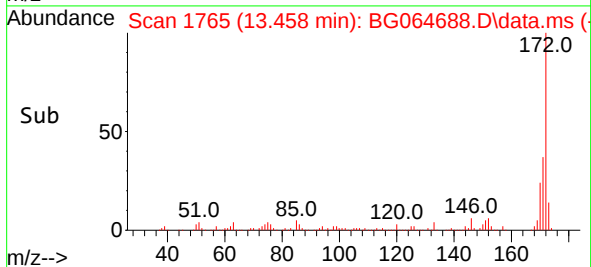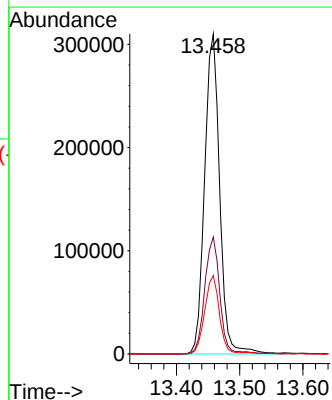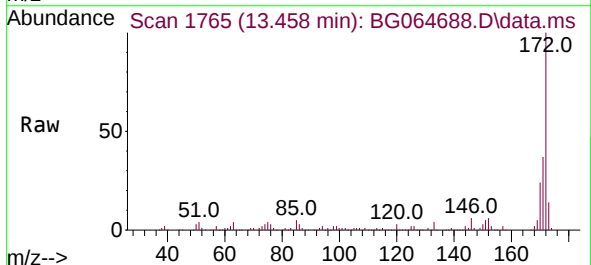

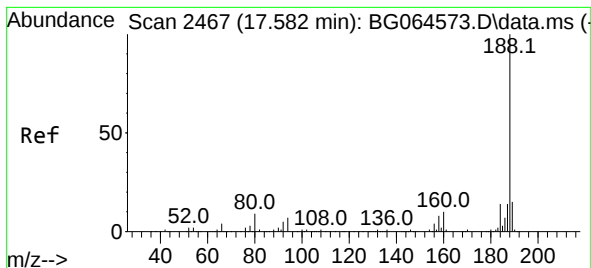

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.565 min Scan# 2464

Delta R.T. -0.017 min

Lab File: BG064688.D

Acq: 5 Nov 2025 16:40

Instrument :

BNA_G

ClientSampleId :

PB170325BL





Tgt Ion:188 Resp: 303868

Ion Ratio Lower Upper

188 100

94 6.3 5.7 8.5

80 7.2 6.8 10.2

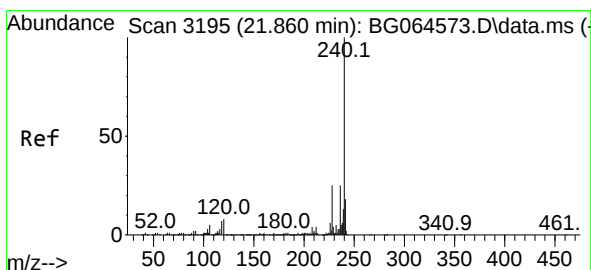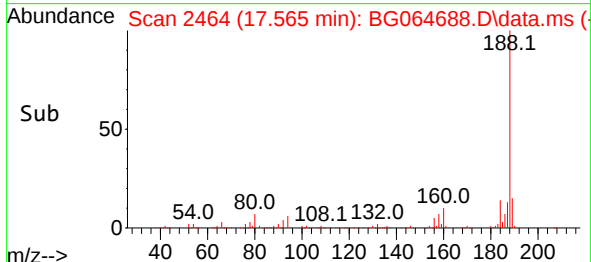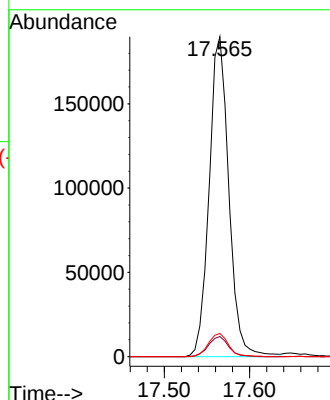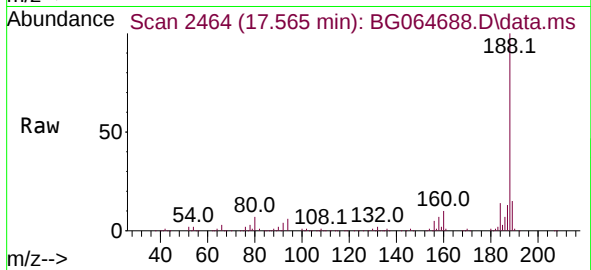

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.837 min Scan# 3191

Delta R.T. -0.023 min

Lab File: BG064688.D

Acq: 5 Nov 2025 16:40




Tgt Ion:240 Resp: 367288


Ion Ratio Lower Upper

240 100

120 5.9 6.5 9.7#

236 24.7 20.2 30.2


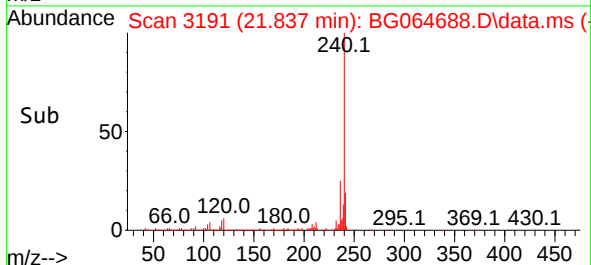
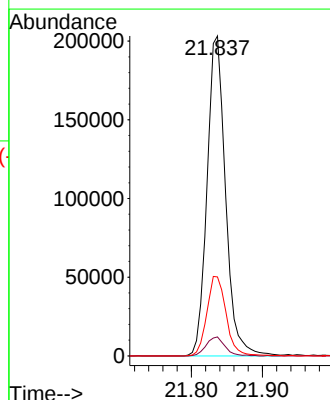
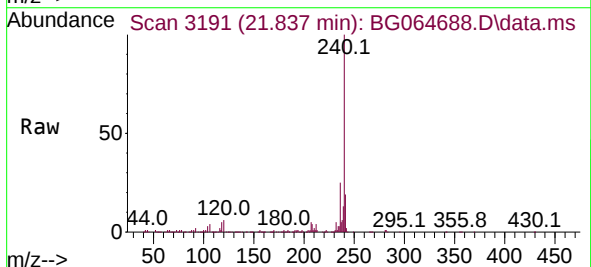


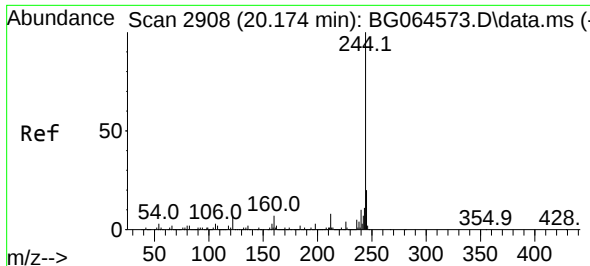

#79
 Terphenyl-d14
 Concen: 104.717 ng
 RT: 20.156 min Scan# 2905
 Delta R.T. -0.017 min
 Lab File: BG064688.D
 Acq: 5 Nov 2025 16:40

Instrument :
 BNA_G
 ClientSampleId :
 PB170325BL

Tgt Ion:244 Resp: 2038037
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.1 9.1
 122 6.2 5.6 8.4

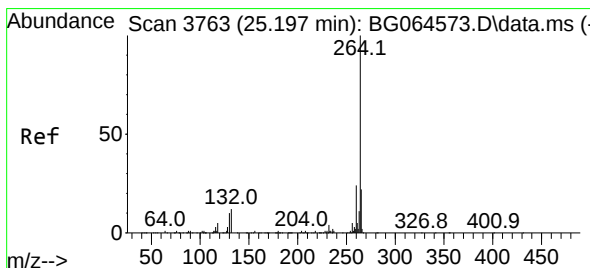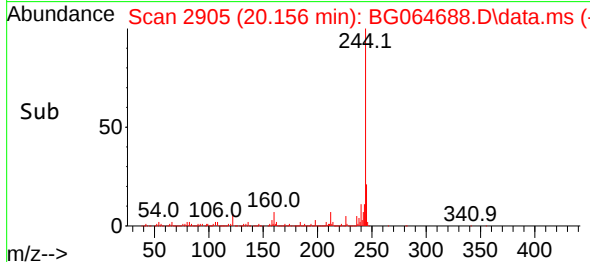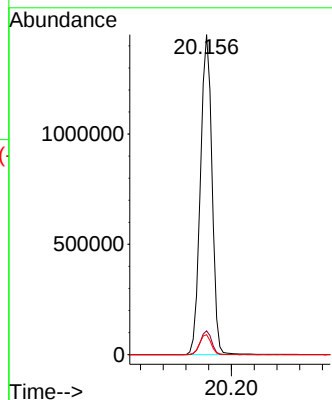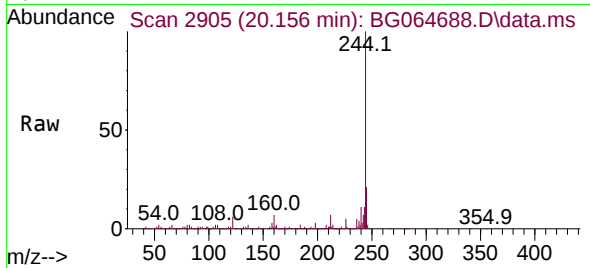

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.168 min Scan# 3758
 Delta R.T. -0.029 min
 Lab File: BG064688.D
 Acq: 5 Nov 2025 16:40

Tgt Ion:264 Resp: 367617
 Ion Ratio Lower Upper
 264 100
 260 25.1 19.0 28.4
 265 22.1 17.6 26.4

