

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064688.D
Acq On : 5 Nov 2025 16:40
Operator : RC/JU
Sample : PB170325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170325BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.738	443	451	467	rBV	446966	802084	15.32%	5.744%
2	7.342	716	724	737	rBV	477211	888003	16.96%	6.360%
3	8.206	864	871	877	rBV	77469	134551	2.57%	0.964%
4	9.369	1061	1069	1082	rBV	255049	499008	9.53%	3.574%
5	11.032	1344	1352	1365	rBV	97694	191903	3.66%	1.374%
6	13.458	1757	1765	1783	rBV	905527	1488193	28.42%	10.658%
7	14.827	1992	1998	2013	rVB	221673	369250	7.05%	2.644%
8	16.308	2243	2250	2265	rBV	1149002	1885307	36.00%	13.502%
9	17.565	2457	2464	2474	rBV2	445636	711841	13.59%	5.098%
10	20.156	2898	2905	2915	rBV	3814397	5236418	100.00%	37.502%
11	21.837	3184	3191	3203	rBV2	500909	904792	17.28%	6.480%
12	25.168	3747	3758	3767	rBV	285861	851829	16.27%	6.101%




Sum of corrected areas: 13963179

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064688.D
Acq On : 5 Nov 2025 16:40
Operator : RC/JU
Sample : PB170325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170325BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

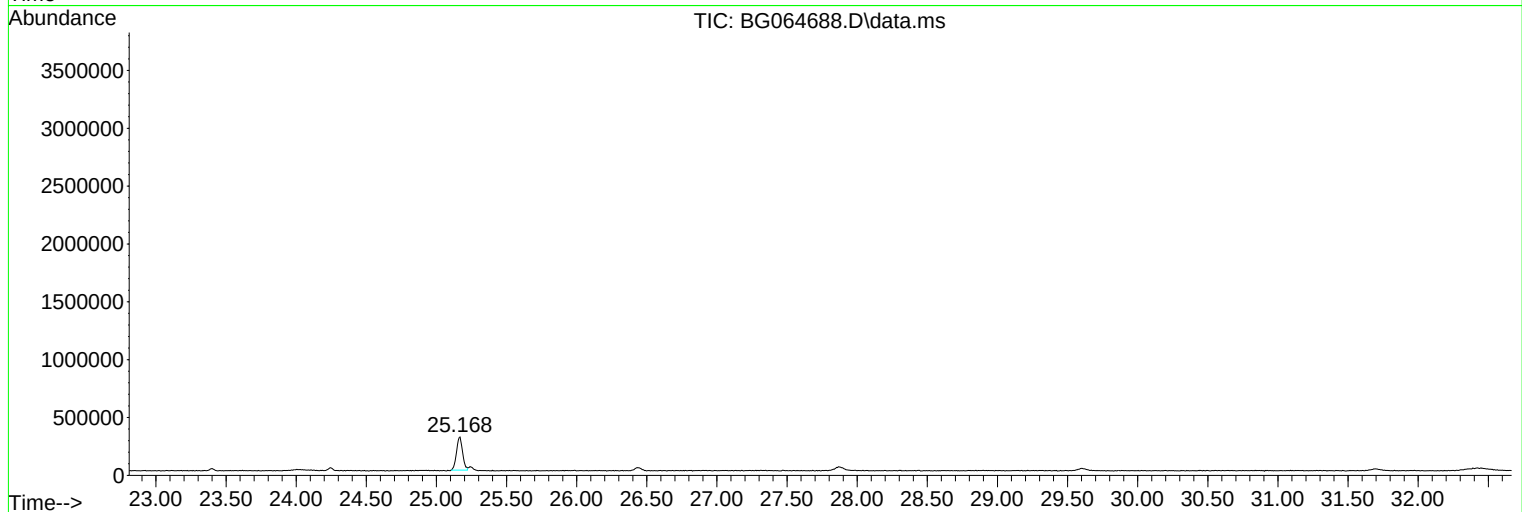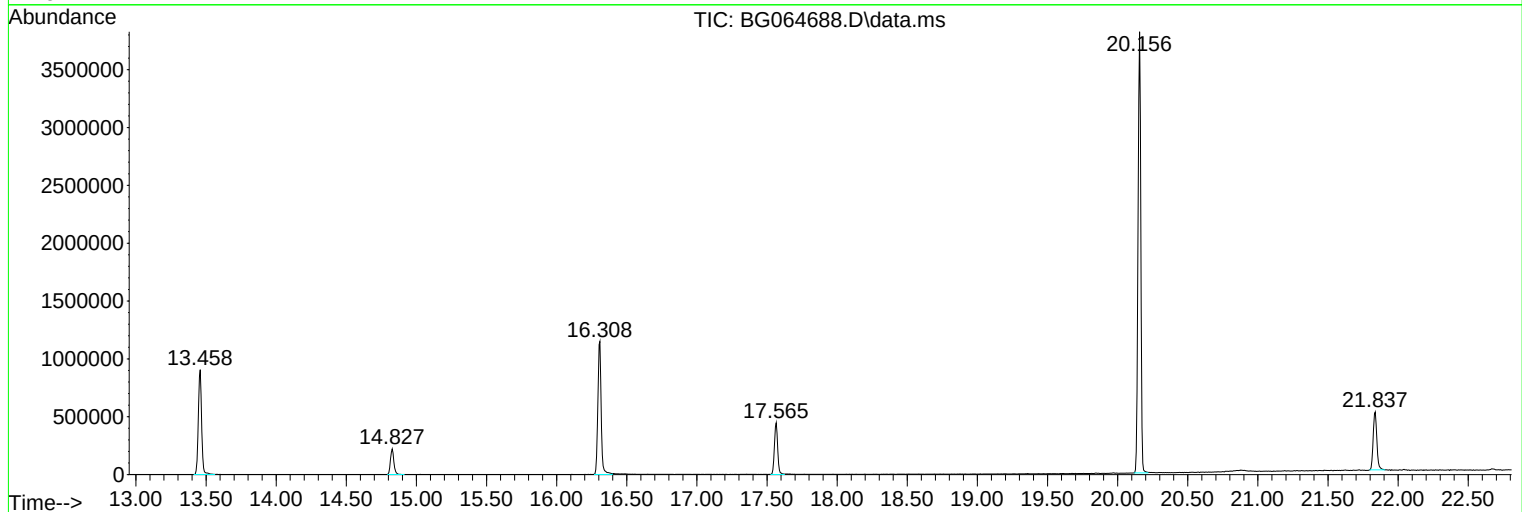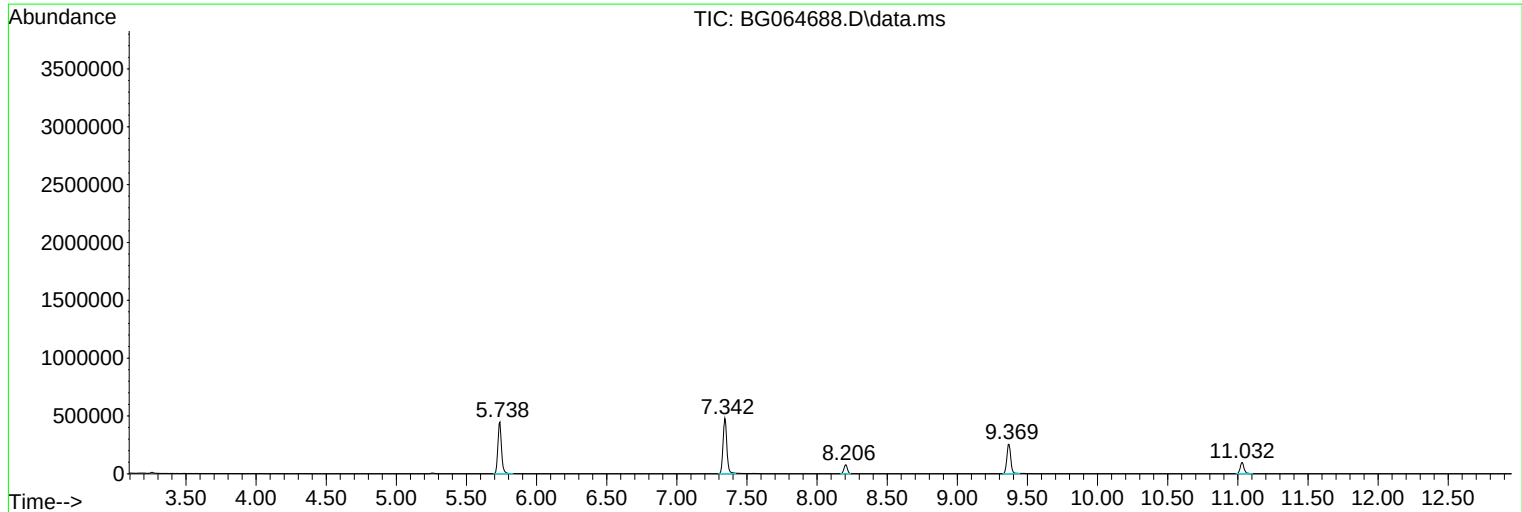

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064688.D
Acq On : 5 Nov 2025 16:40
Operator : RC/JU
Sample : PB170325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170325BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064688.D
Acq On : 5 Nov 2025 16:40
Operator : RC/JU
Sample : PB170325BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170325BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------