


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064686.D
Acq On : 5 Nov 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 03 18:16:26 2025

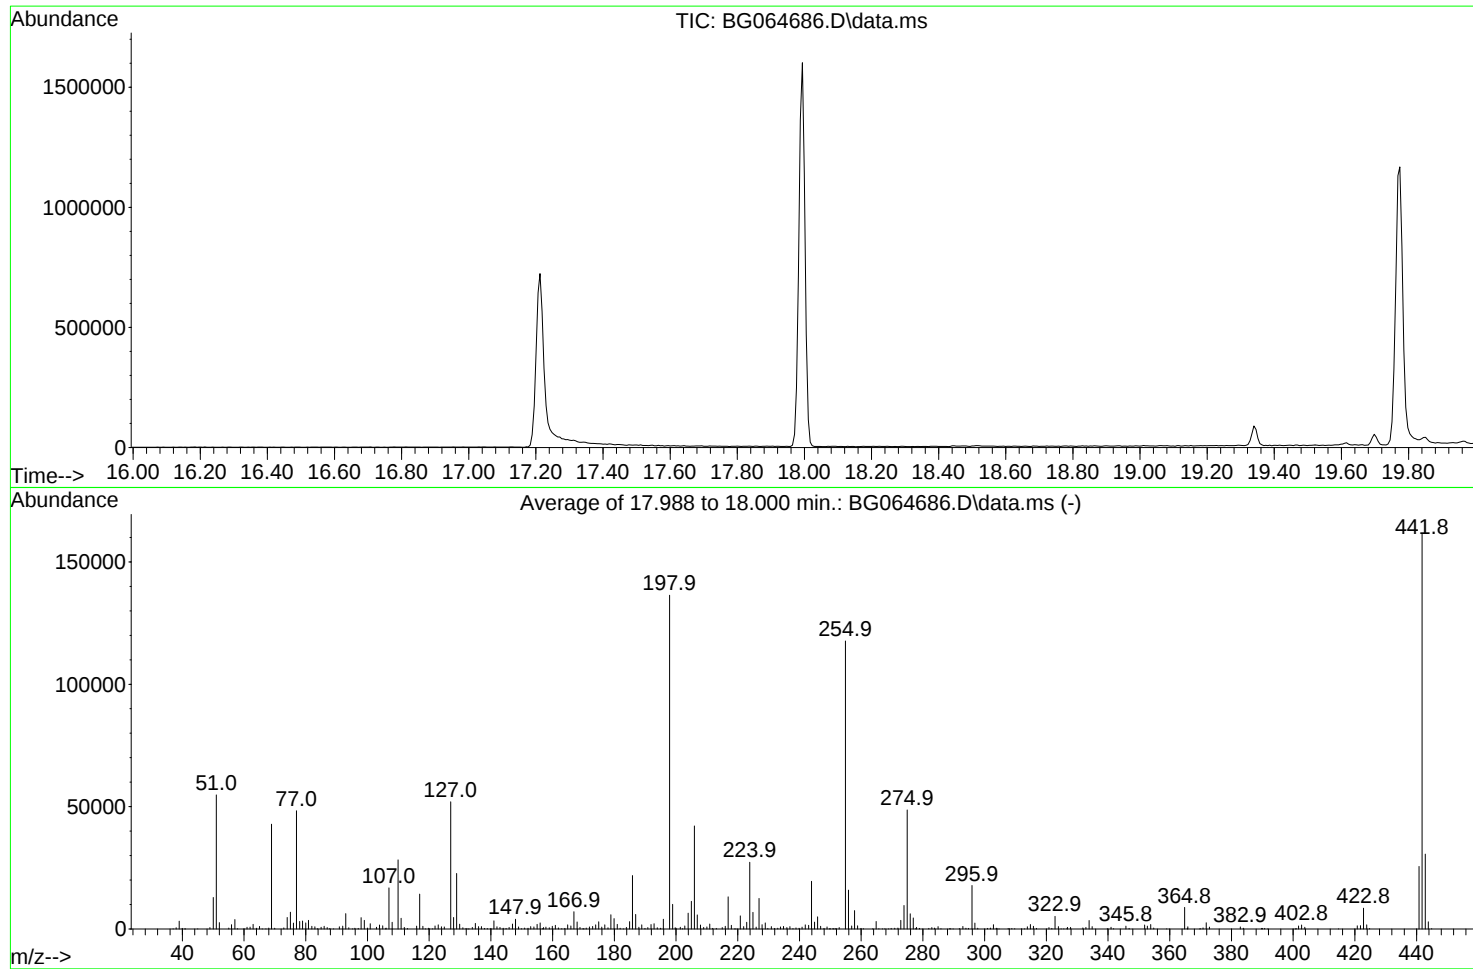




AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	377	PASS
69	69	100	100	100.0	42787	PASS
70	69	0.00	2	0.6	265	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136379	PASS
199	198	5	9	7.3	10016	PASS
365	198	1	100	6.4	8795	PASS
441	443	0.01	150	83.5	25536	PASS
442	442	100	100	100.0	161397	PASS
443	442	15	24	19.0	30597	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064686.D
Acq On : 5 Nov 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 05 15:34:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

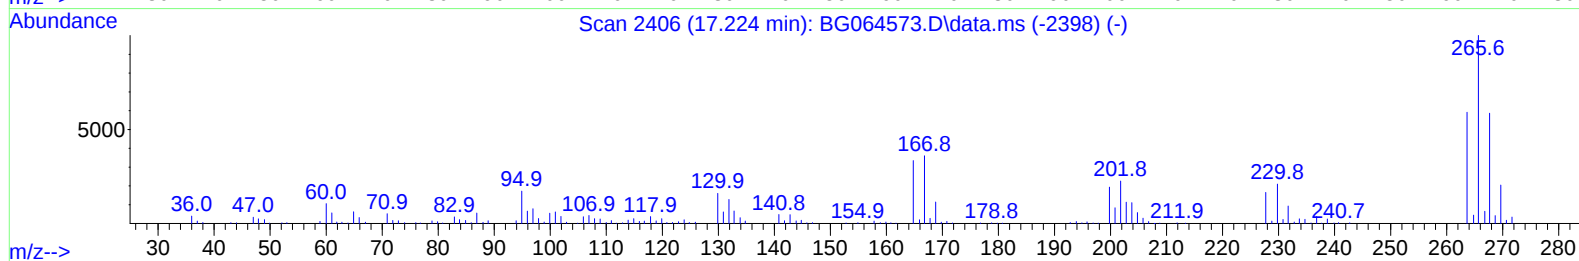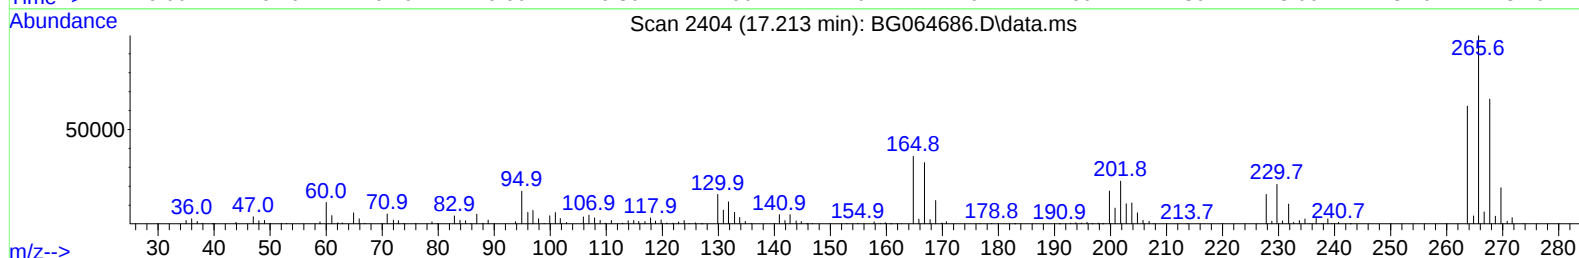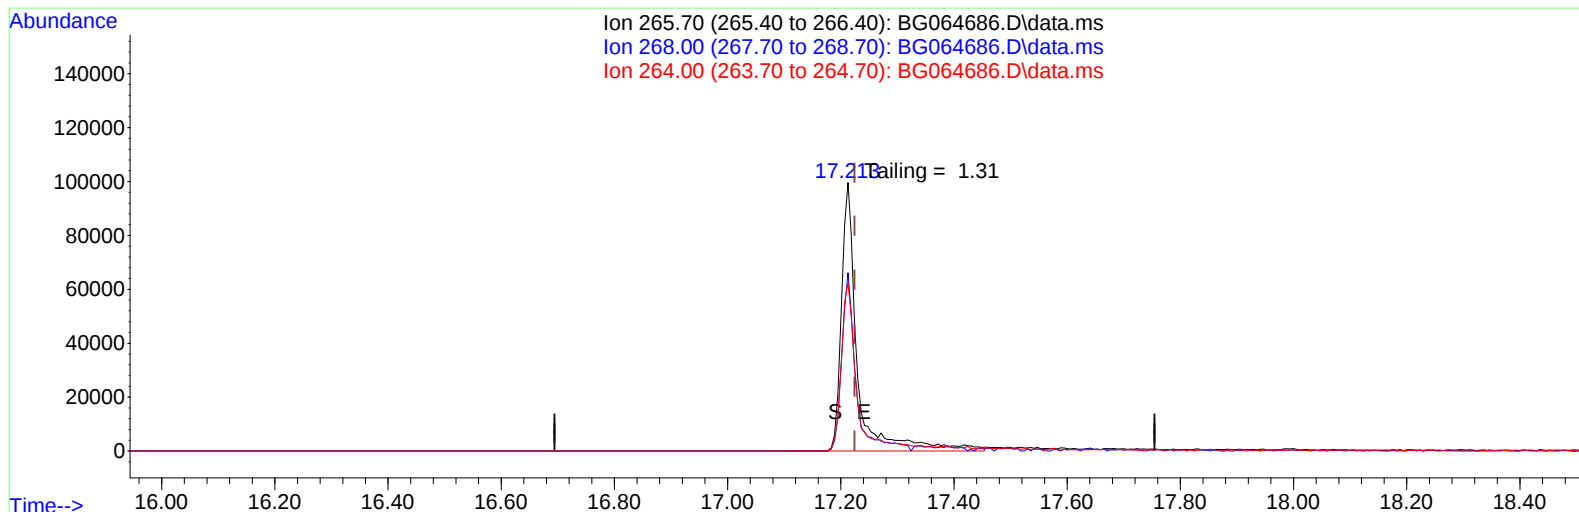

TIC: BG064686.D\data.ms

(70) Pentachlorophenol (C)

17.213min (-0.012) 114892.15 ng




response 187907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	70.51
264.00	59.10	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110525\
Data File : BG064686.D
Acq On : 5 Nov 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 05 15:34:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

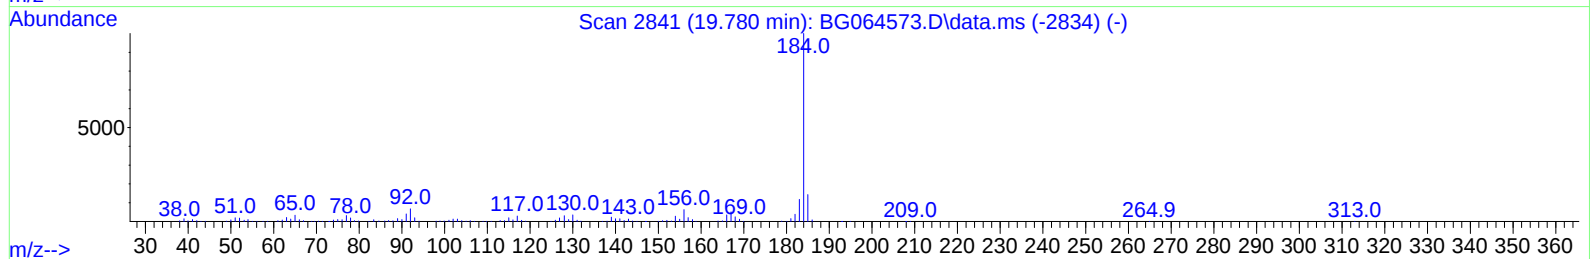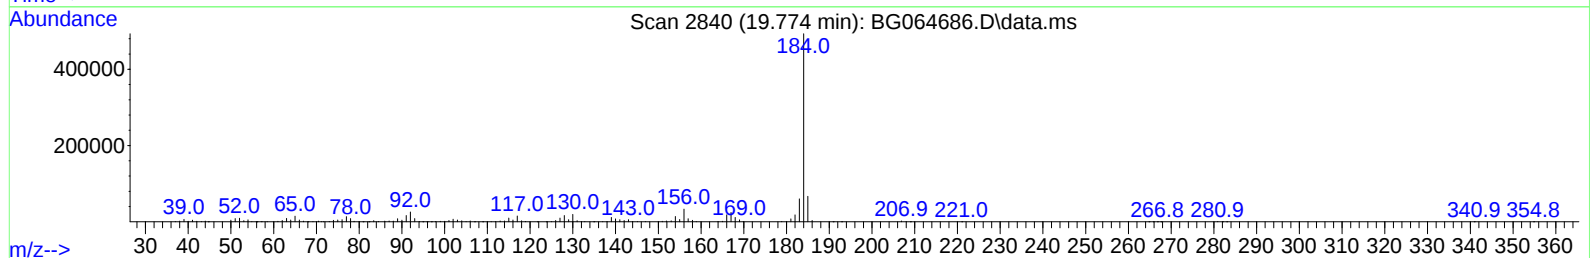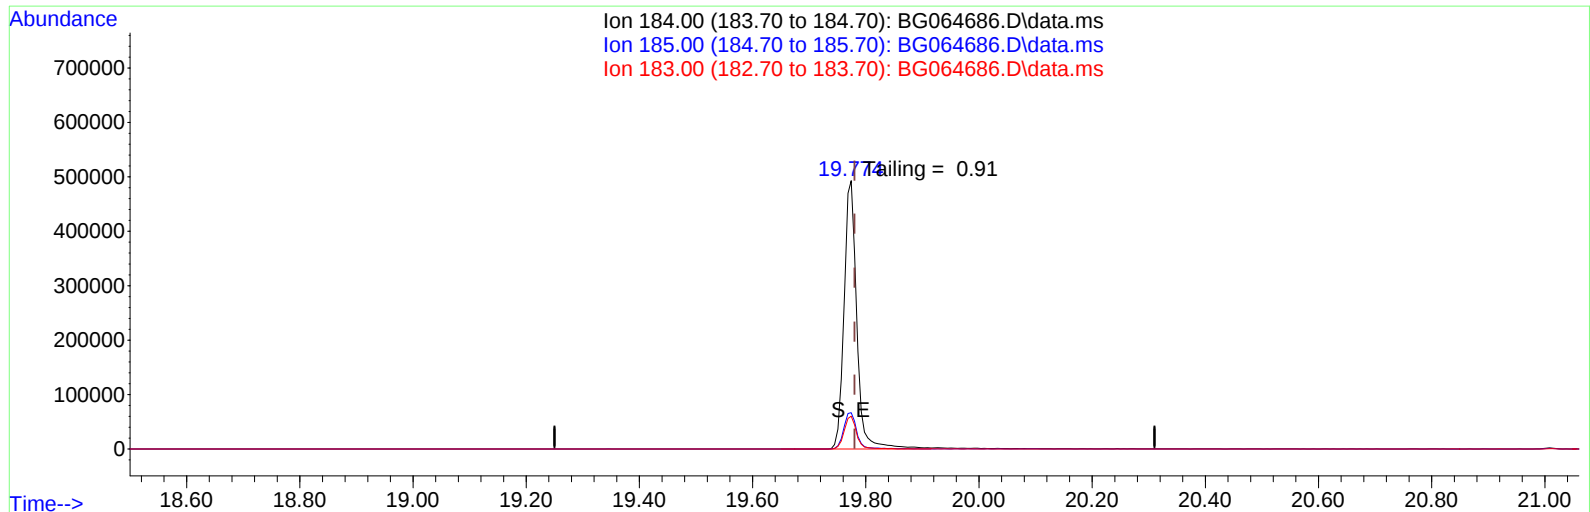

TIC: BG064686.D\data.ms

(77) Benzidine

19.774min (-0.006) 30048.03 ng

response 773507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.55
183.00	11.80	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2025	BNA_G	<u>BG064686.D</u>
Compound Name	Response	Retention Time
DDT	478799	21.008
DDD	12527	20.562
DDE	1098	20.068
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13625	492424	2.77

Instrument :
BNA_G
ClientSampleId :
DFTPP