

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110618\
 Data File : BG037851.D
 Acq On : 6 Nov 2018 23:17
 Operator : JU/SJ
 Sample : J5771-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 07 08:22:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	56137	20.00	ng	-0.02
21) Naphthalene-d8	10.91	136	250584	20.00	ng	-0.02
39) Acenaphthene-d10	14.73	164	164597	20.00	ng	-0.02
64) Phenanthrene-d10	17.48	188	361436	20.00	ng	0.00
76) Chrysene-d12	21.76	240	319235	20.00	ng	-0.02
87) Perylene-d12	25.10	264	256470	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	369591	110.07	ng	0.00
7) Phenol-d6	7.24	99	478700	94.28	ng	0.00
23) Nitrobenzene-d5	9.27	82	361471	80.81	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	168437	93.82	ng	-0.02
45) 2-Fluorobiphenyl	13.35	172	877862	80.42	ng	-0.02
79) Terphenyl-d14	20.07	244	1252097	83.81	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.27	70	45525	13.02	ng	# 69
51) 2,6-Dinitrotoluene	14.73	165	20559	7.30	ng	# 24
57) 2,4-Dinitrotoluene	14.73	165	20559	5.56	ng	# 24
65) 4,6-Dinitro-2-methylphenol	16.21	198	564	8.75	ng	# 63
67) 4-Bromophenyl-phenylether	16.22	248	11910	3.00	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110618\
Data File : BG037851.D
Acq On : 6 Nov 2018 23:17
Operator : JU/SJ
Sample : J5771-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 07 08:22:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

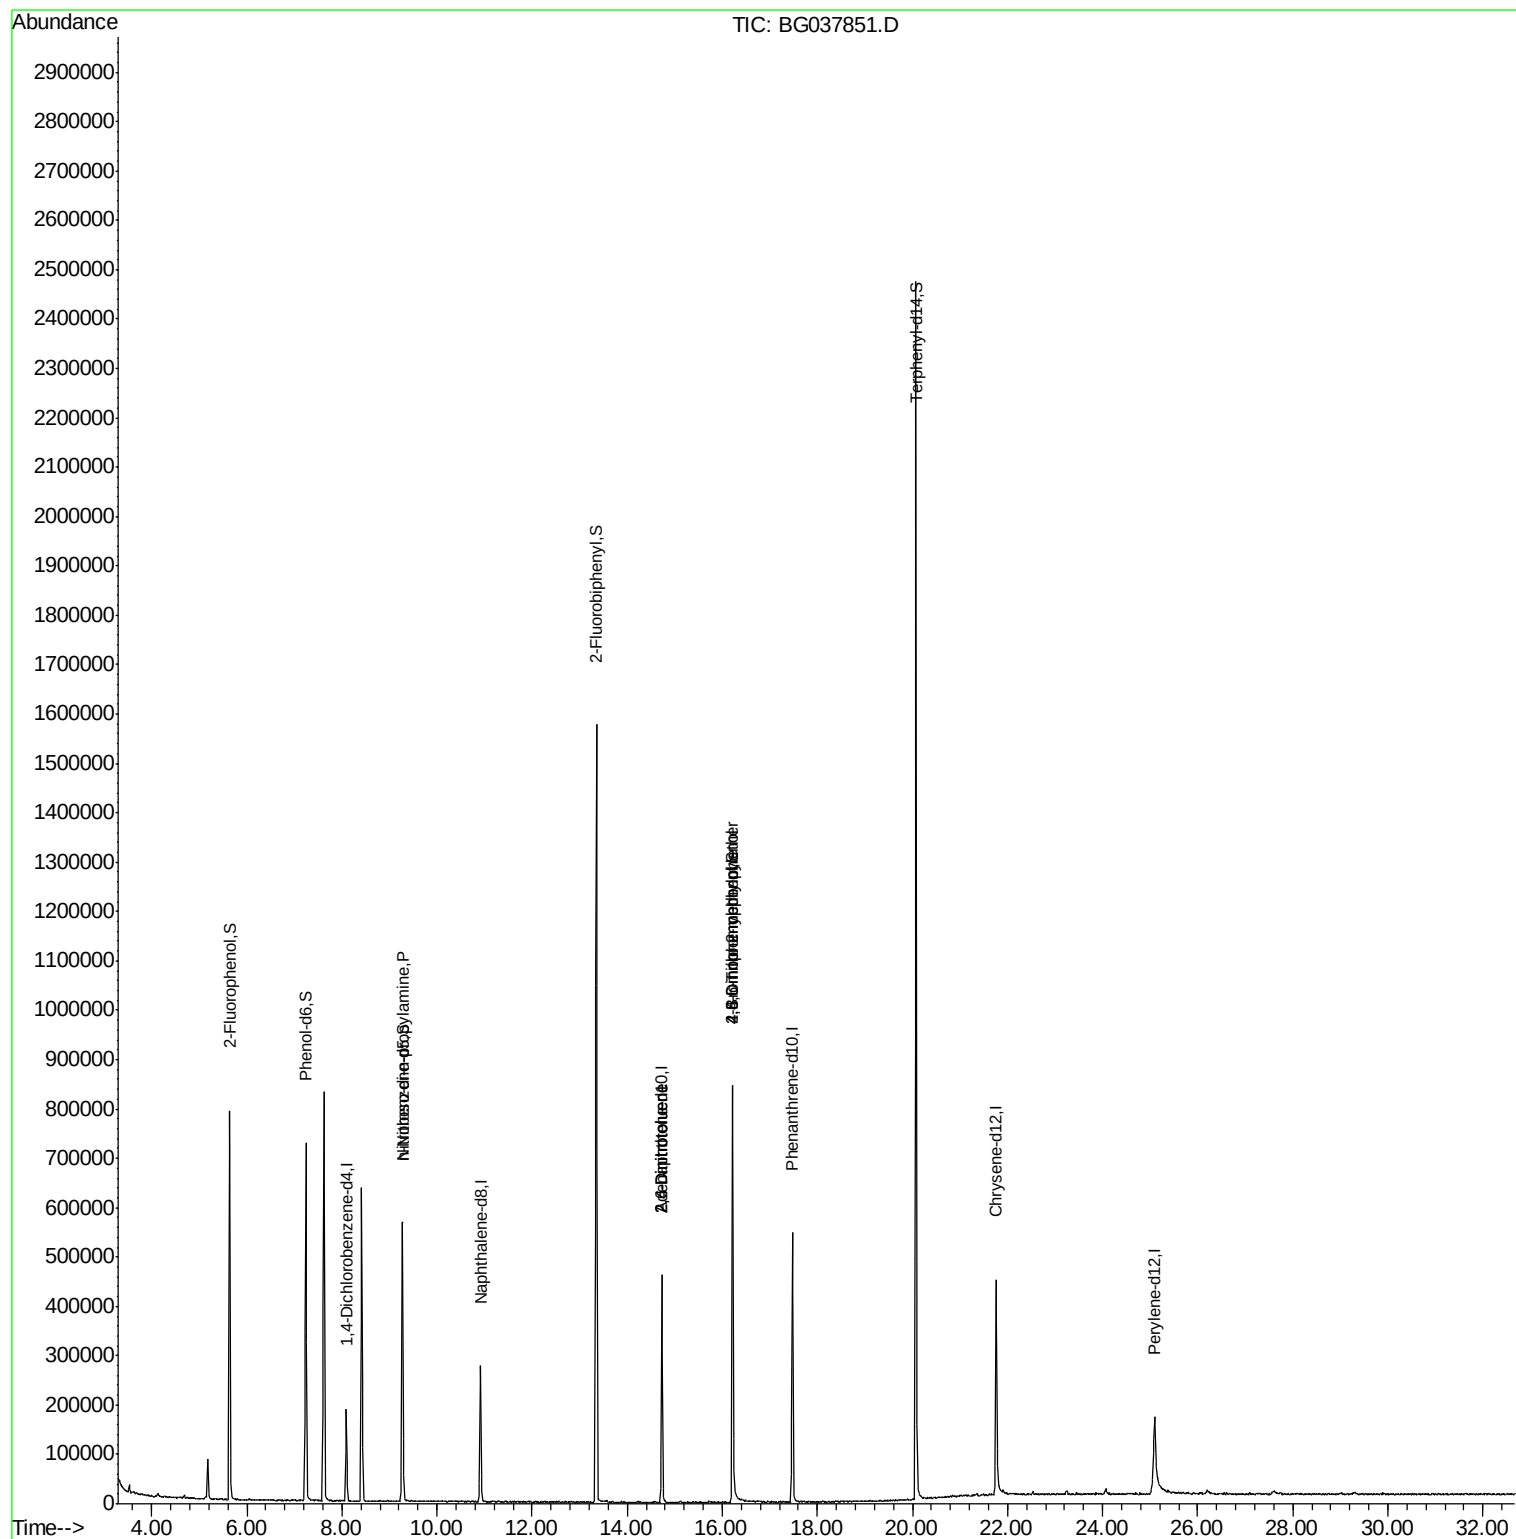

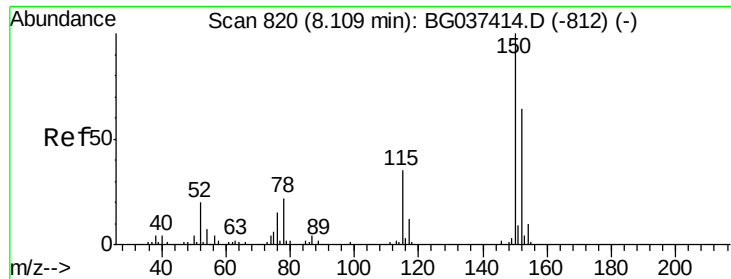


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.09 min Scan# 818
Delta R.T. -0.02 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.4	126.0	189.0
115	58.1	45.5	68.3

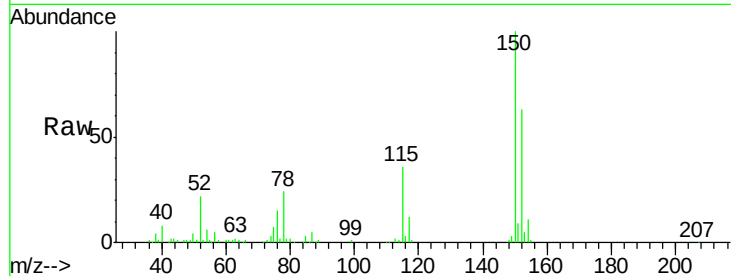


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

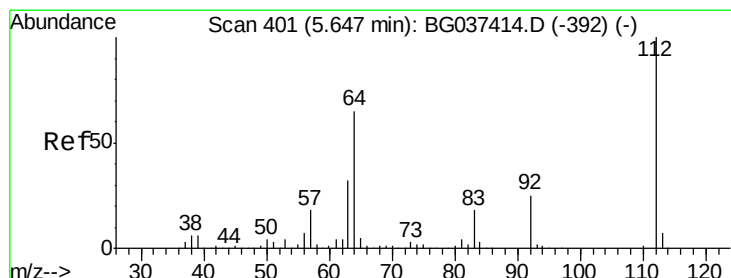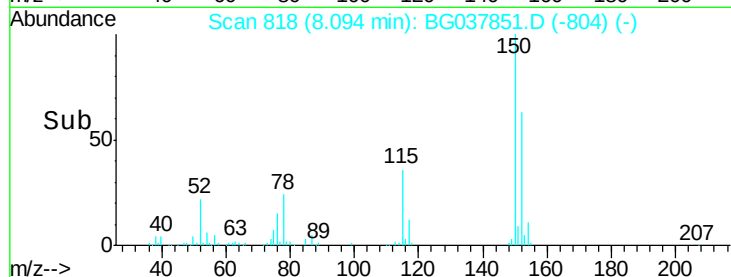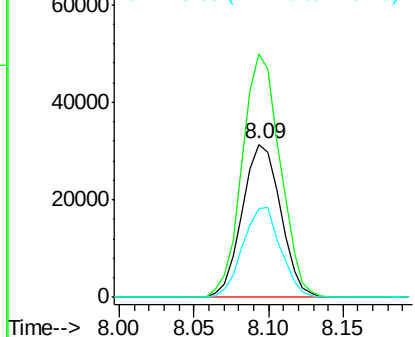



#5


2-Fluorophenol
Concen: 110.07 ng
RT: 5.64 min Scan# 400
Delta R.T. -0.01 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17

Tgt Ion	Ratio	Lower	Upper
112	100		
64	65.9	53.1	79.7
63	33.9	27.3	40.9

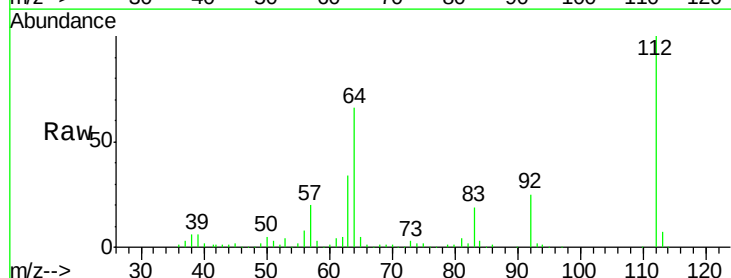

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

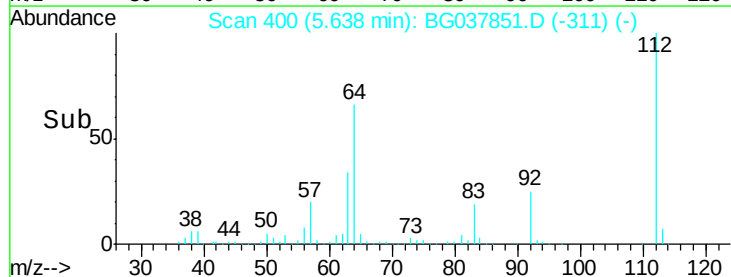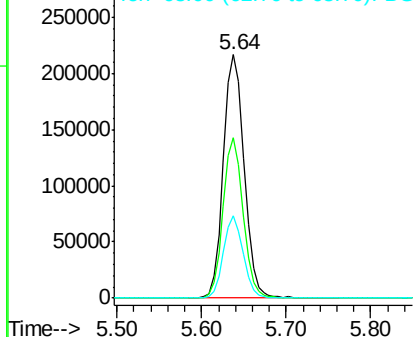

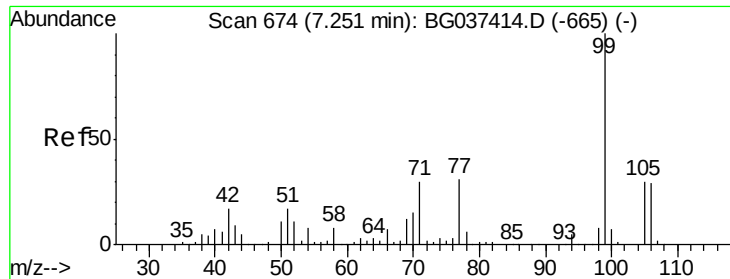

#7

Phenol-d6

Concen: 94.28 ng

RT: 7.24 min Scan# 673

Delta R.T. -0.01 min

Lab File: BG037851.D

Acq: 6 Nov 2018 23:17

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 478700

Ion Ratio Lower Upper




99 100

42 17.4 15.0 22.4

71 30.3 25.5 38.3

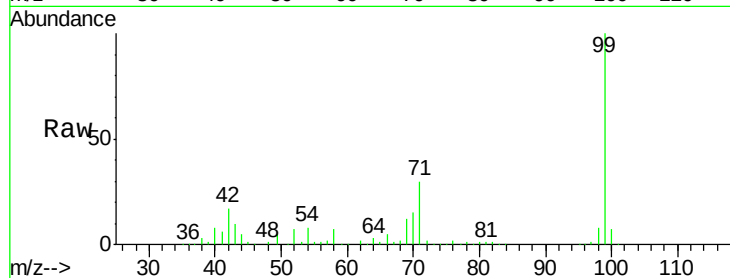

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

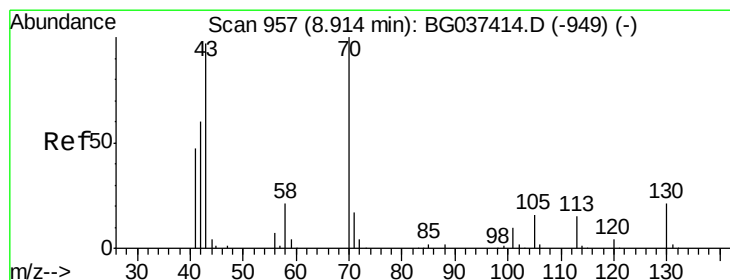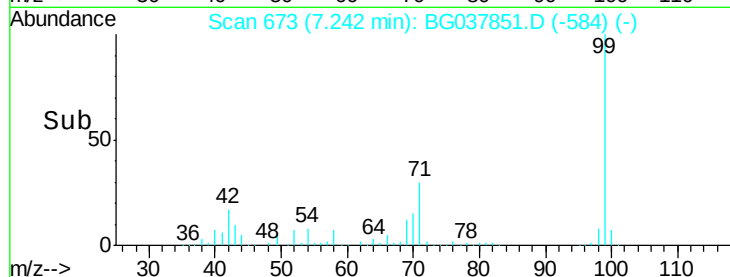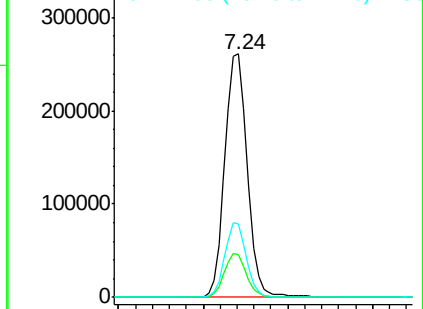

#19

n-Nitroso-di-n-propylamine

Concen: 13.02 ng

RT: 9.27 min Scan# 1019

Delta R.T. 0.36 min

Lab File: BG037851.D

Acq: 6 Nov 2018 23:17

Tgt Ion: 70 Resp: 45525


Ion Ratio Lower Upper

70 100



42 45.3 53.9 80.9#


101 0.0 8.2 12.2#

130 2.3 18.2 27.4#

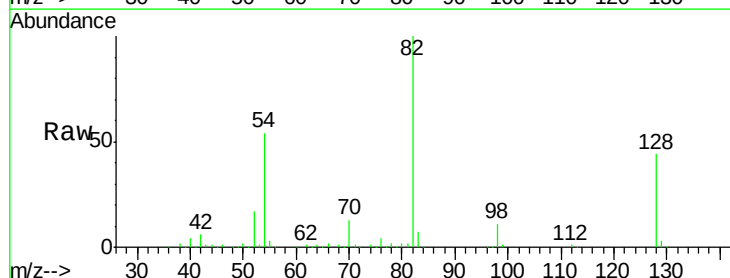

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

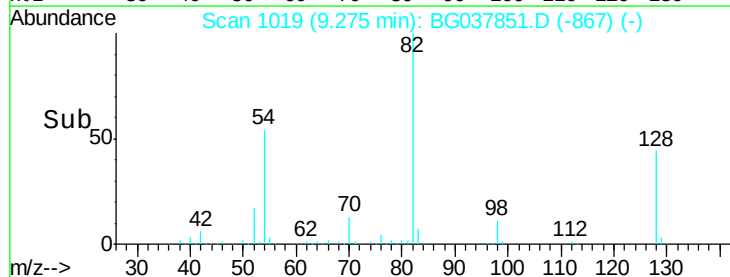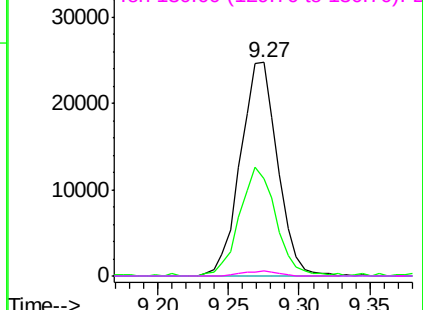


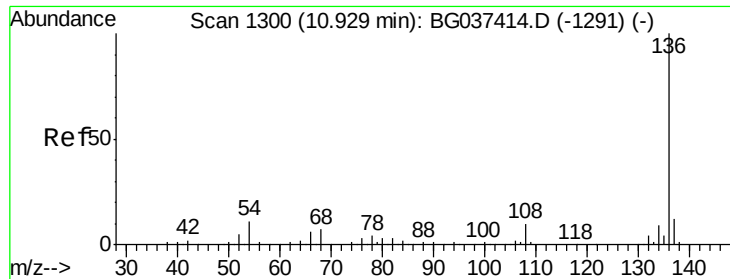




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.91 min Scan# 1298
Delta R.T. -0.02 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	250584
Ion Ratio	Lower	Upper
136	100	
137	11.7	9.6 14.4
54	11.6	7.9 11.9
68	6.9	4.8 7.2

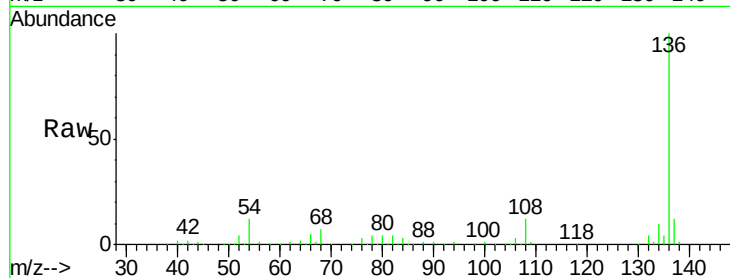


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

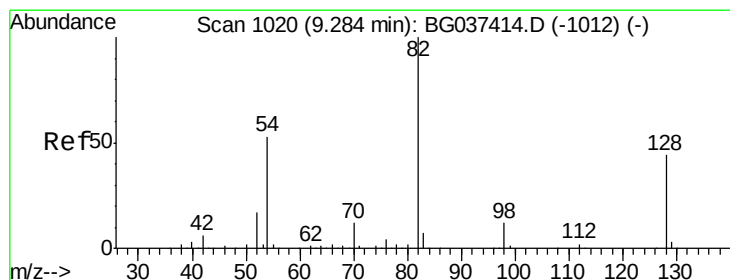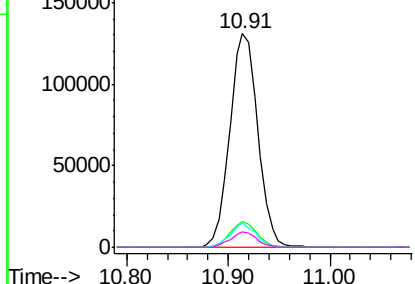
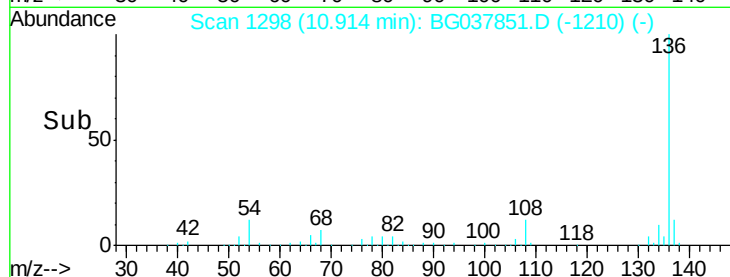



#23
Nitrobenzene-d5
Concen: 80.81 ng
RT: 9.27 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17

Tgt Ion: 82	Resp:	361471
Ion Ratio	Lower	Upper
82	100	
128	44.3	34.6 51.8
54	53.6	45.3 67.9

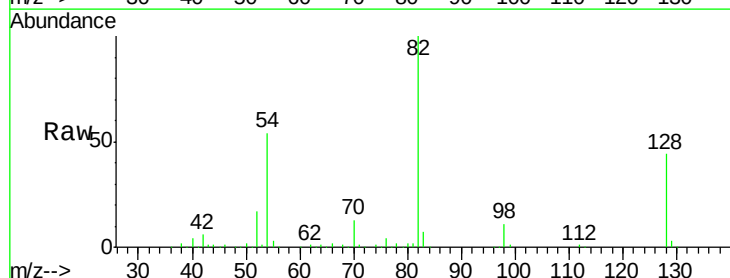

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

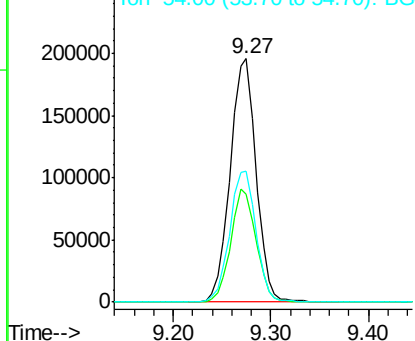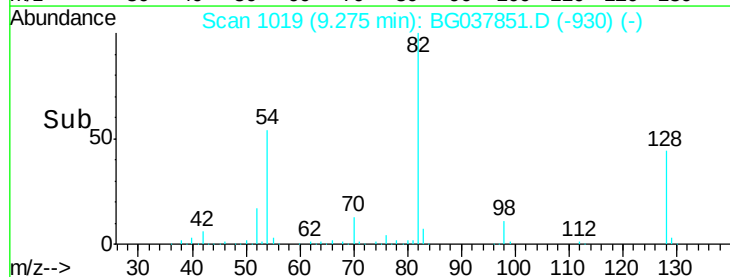

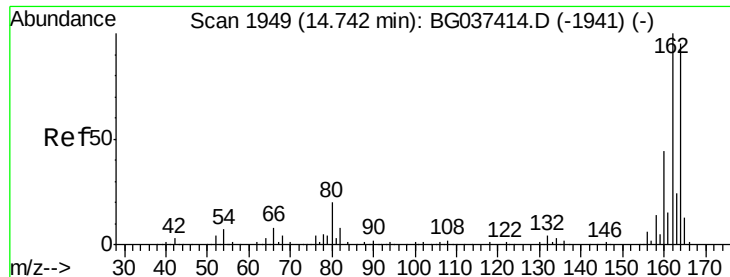

#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.73 min Scan# 1947

Delta R.T. -0.02 min

Lab File: BG037851.D

Acq: 6 Nov 2018 23:17

Instrument :

BNA_G

ClientSampled :


Tot Ion:164 Resp: 164597

Ion Ratio Lower Upper

164 100

162 104.2 81.3 121.9




160 47.3 36.3 54.5

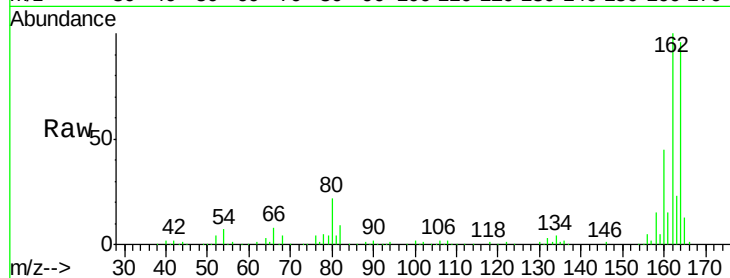

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

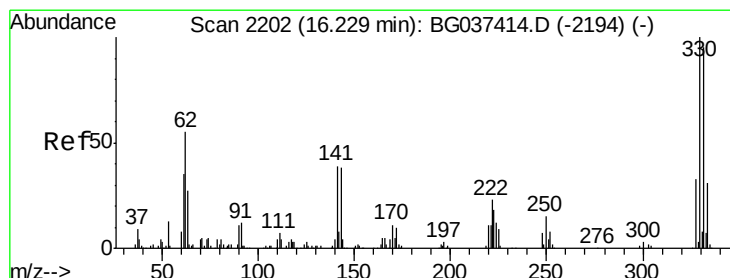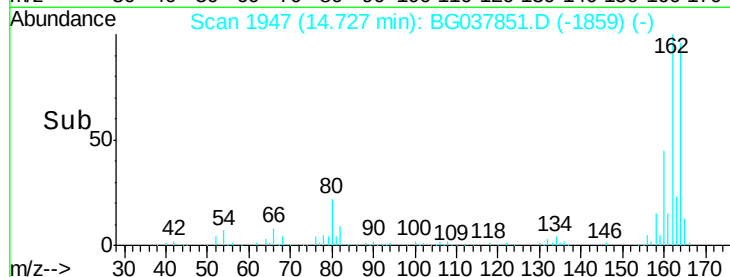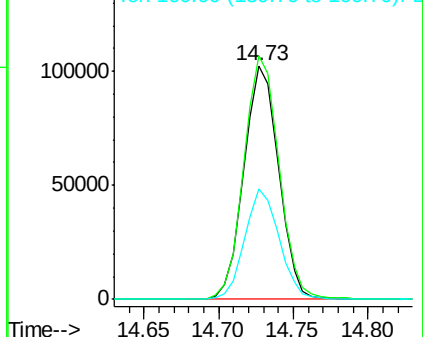

#42

2,4,6-Tribromophenol

Concen: 93.82 ng

RT: 16.21 min Scan# 2200

Delta R.T. -0.02 min

Lab File: BG037851.D

Acq: 6 Nov 2018 23:17


Tgt Ion:330 Resp: 168437

Ion Ratio Lower Upper

330 100

332 96.2 78.4 117.6



141 39.2 32.2 48.2

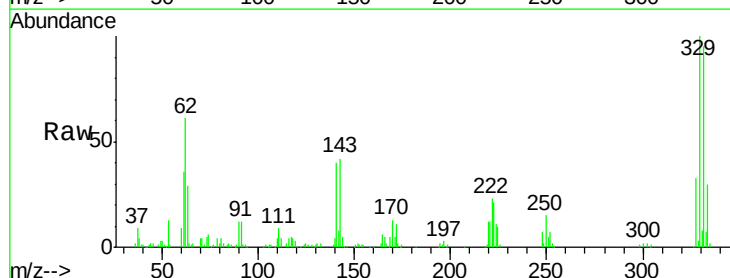


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



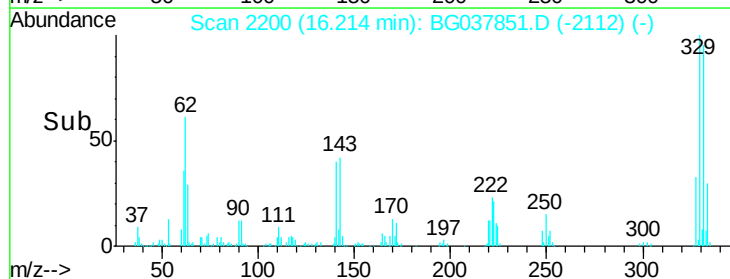
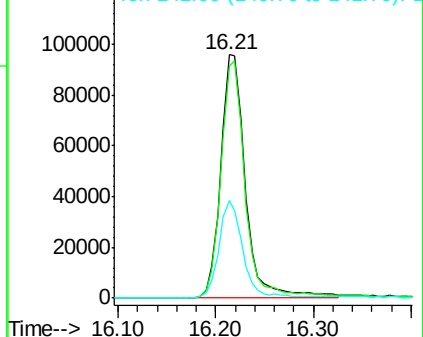


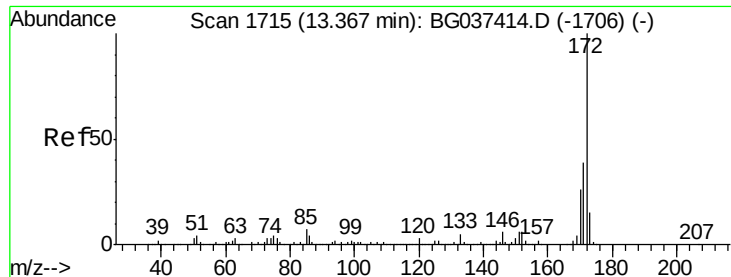

#45
2-Fluorobiphenyl
Concen: 80.42 ng
RT: 13.35 min Scan# 1713
Delta R.T. -0.02 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17




Instrument :
BNA_G
ClientSampleId :


Tot Ion:172 Resp: 877862
Ion Ratio Lower Upper
172 100
171 38.7 31.0 46.4
170 24.8 20.2 30.2

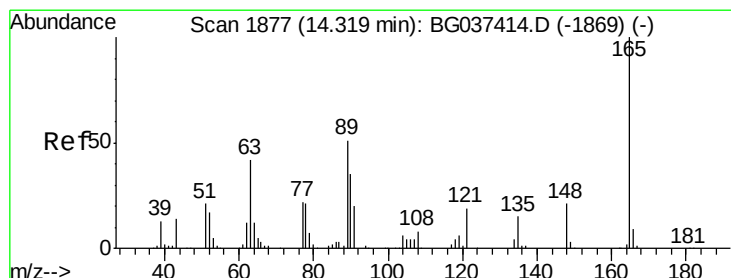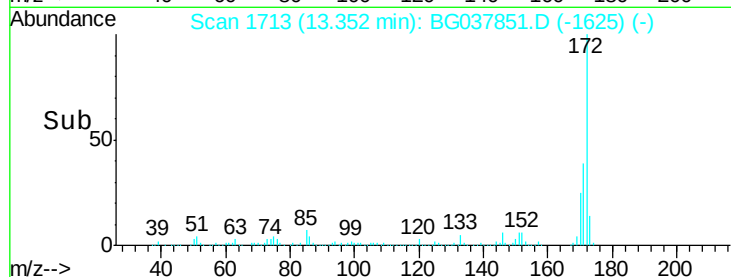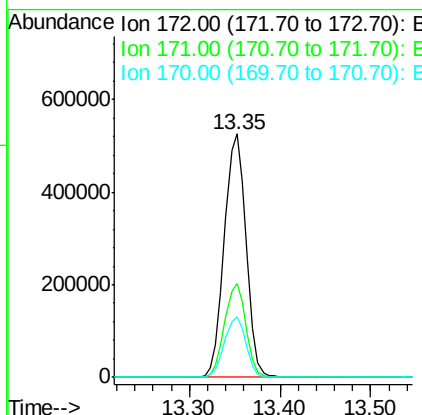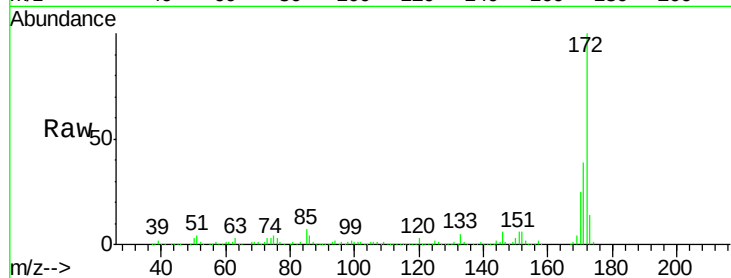

#51
2,6-Dinitrotoluene
Concen: 7.30 ng
RT: 14.73 min Scan# 1947
Delta R.T. 0.41 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17

Tgt Ion:165 Resp: 20559
Ion Ratio Lower Upper
165 100
63 0.0 43.4 65.2#
89 1.4 45.8 68.6#


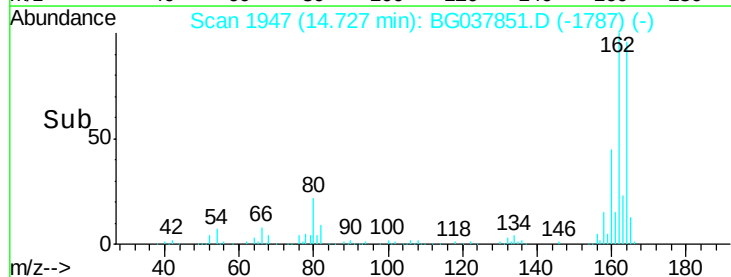
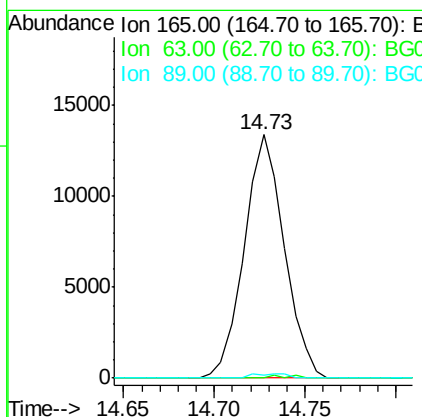
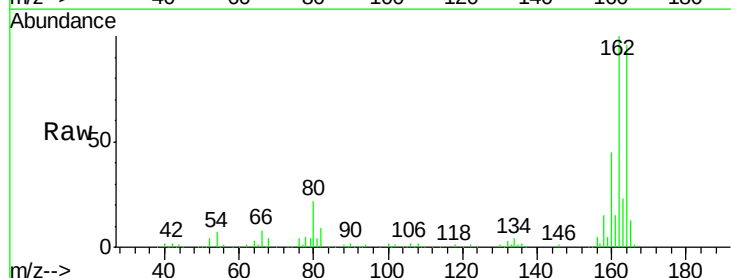


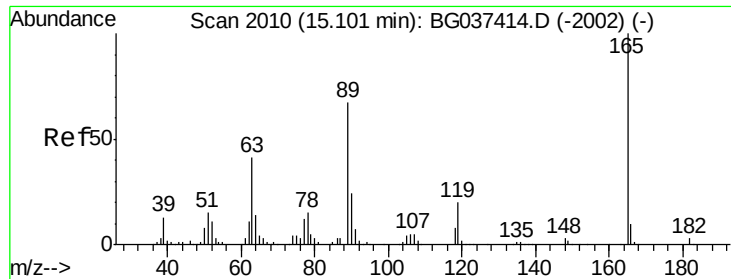

#57
 2,4-Dinitrotoluene
 Concen: 5.56 ng
 RT: 14.73 min Scan# 1947
 Delta R.T. -0.37 min
 Lab File: BG037851.D
 Acq: 6 Nov 2018 23:17




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:165	Resp:	20559
Ion Ratio	Lower	Upper
165	100	
63	0.0	33.4 50.0#
89	1.4	57.2 85.8#
182	0.0	2.6 4.0#

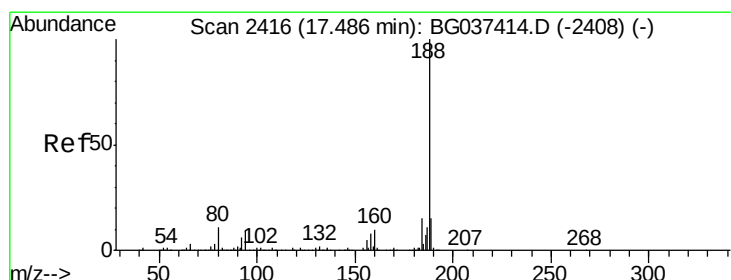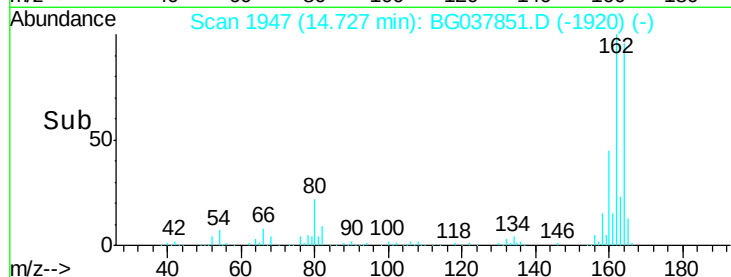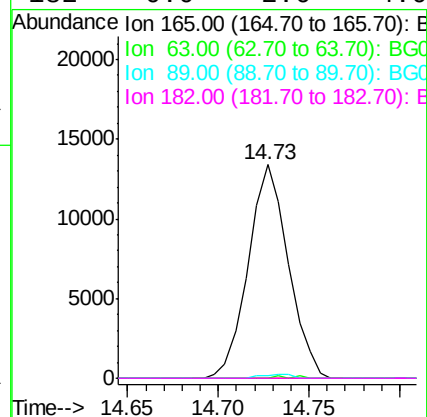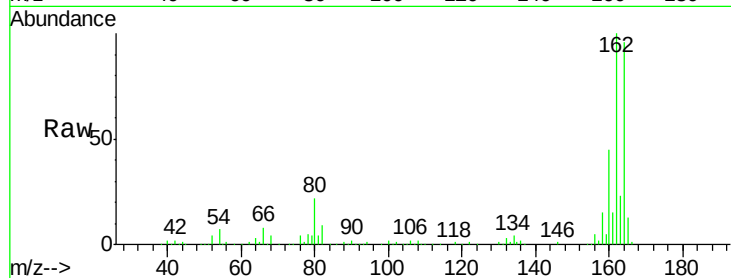

#64
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.48 min Scan# 2415
 Delta R.T. -0.01 min
 Lab File: BG037851.D
 Acq: 6 Nov 2018 23:17

Tgt Ion:188	Resp:	361436
Ion Ratio	Lower	Upper
188	100	
94	9.0	7.2 10.8
80	9.3	7.7 11.5

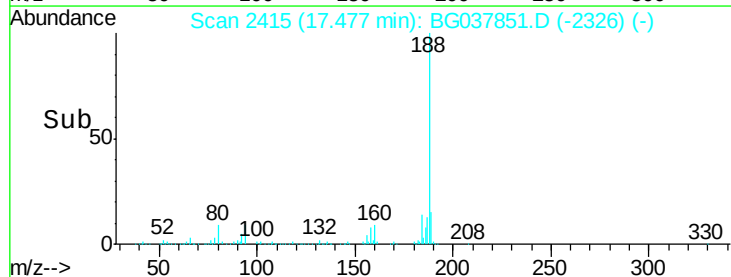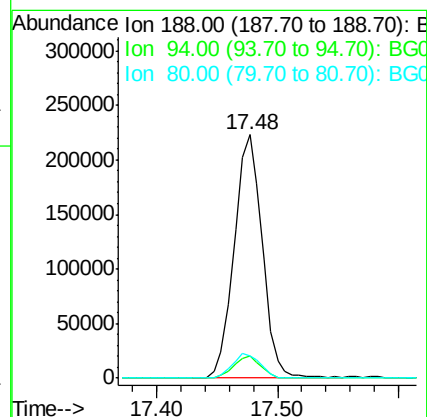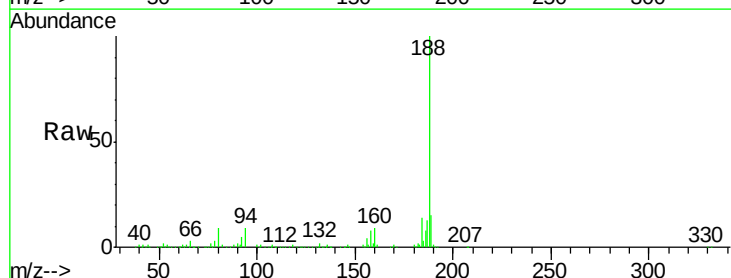


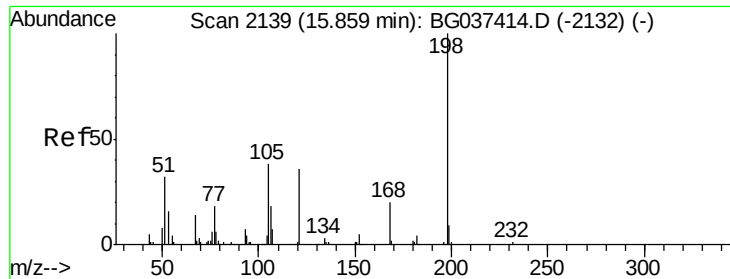




#65
 4,6-Dinitro-2-methylphenol
 Concen: 8.75 ng
 RT: 16.21 min Scan# 2199
 Delta R.T. 0.35 min
 Lab File: BG037851.D
 Acq: 6 Nov 2018 23:17

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:198 Resp: 564
 Ion Ratio Lower Upper
 198 100
 51 25.1 22.7 62.7
 105 10.2 19.7 59.7#

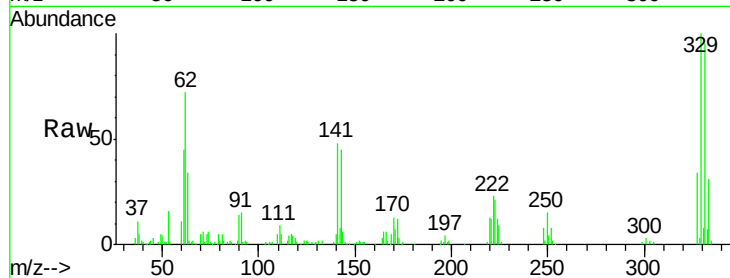


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BG
 Ion 105.00 (104.70 to 105.70): E

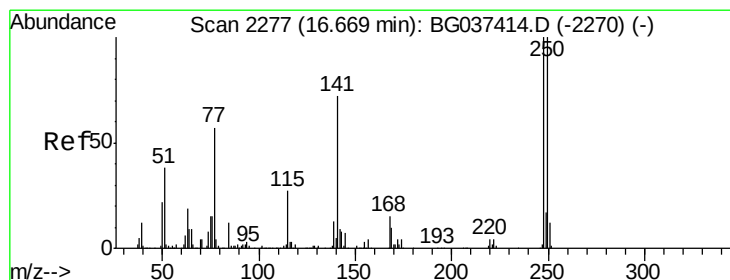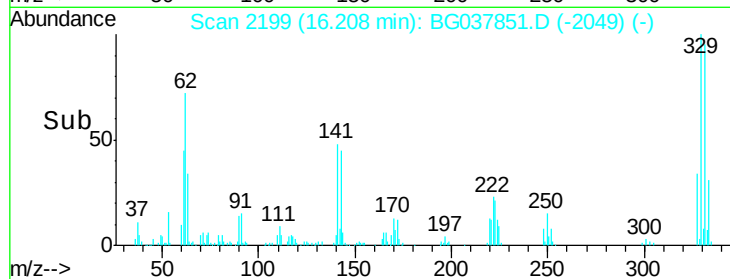
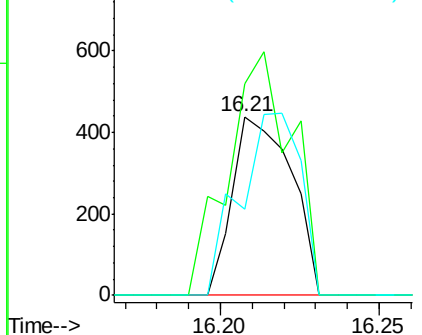



#67
 4-Bromophenyl-phenylether
 Concen: 3.00 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. -0.45 min
 Lab File: BG037851.D
 Acq: 6 Nov 2018 23:17

Tgt Ion:248 Resp: 11910
 Ion Ratio Lower Upper
 248 100
 250 181.7 77.0 115.6#
 141 346.5 55.5 83.3#

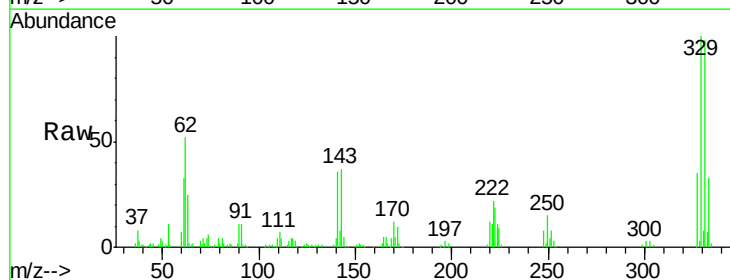

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

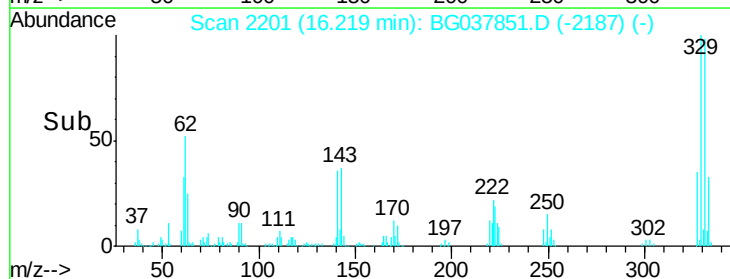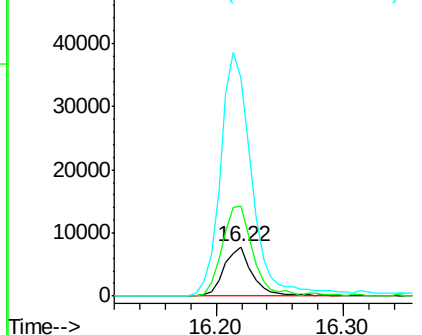

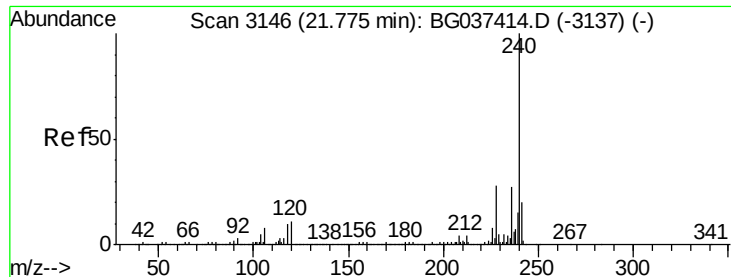

#76

Chrysene-d12

Concen: 20.00 ng

RT: 21.76 min Scan# 3144

Delta R.T. -0.02 min

Lab File: BG037851.D

Acq: 6 Nov 2018 23:17

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 319235

Ion Ratio Lower Upper

240 100

120 10.6 8.1 12.1




236 26.9 21.4 32.0

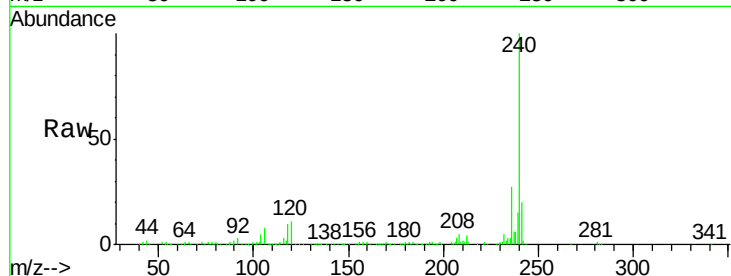

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

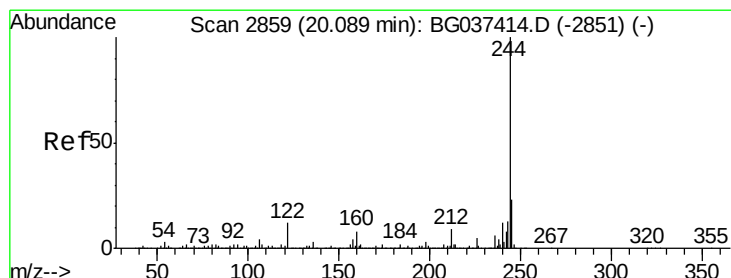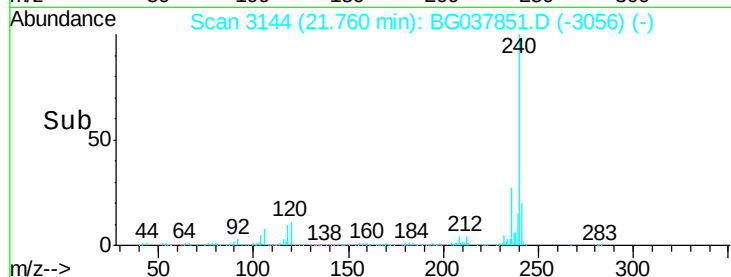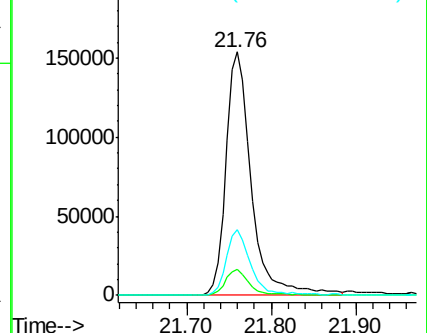

#79

Terphenyl-d14

Concen: 83.81 ng

RT: 20.07 min Scan# 2857

Delta R.T. -0.02 min

Lab File: BG037851.D

Acq: 6 Nov 2018 23:17


Tgt Ion:244 Resp: 1252097

Ion Ratio Lower Upper

244 100

212 8.4 6.5 9.7



122 11.2 9.0 13.4

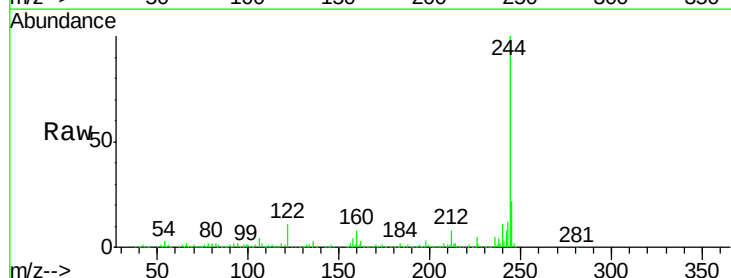


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

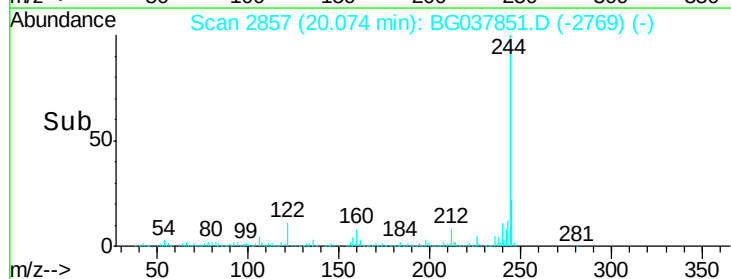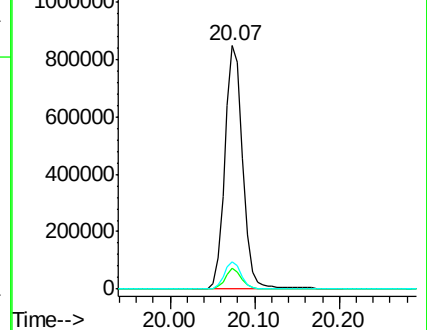


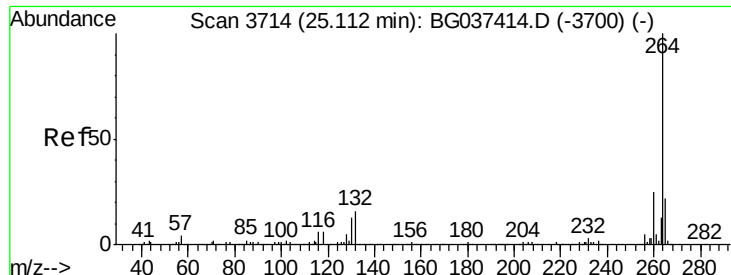

#87
Pervlene-d12
Concen: 20.00 ng
RT: 25.10 min Scan# 3712
Delta R.T. -0.02 min
Lab File: BG037851.D
Acq: 6 Nov 2018 23:17

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.6	18.2	27.4
265	20.1	17.9	26.9

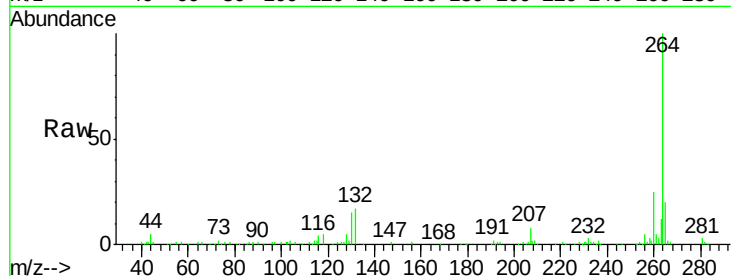

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

