
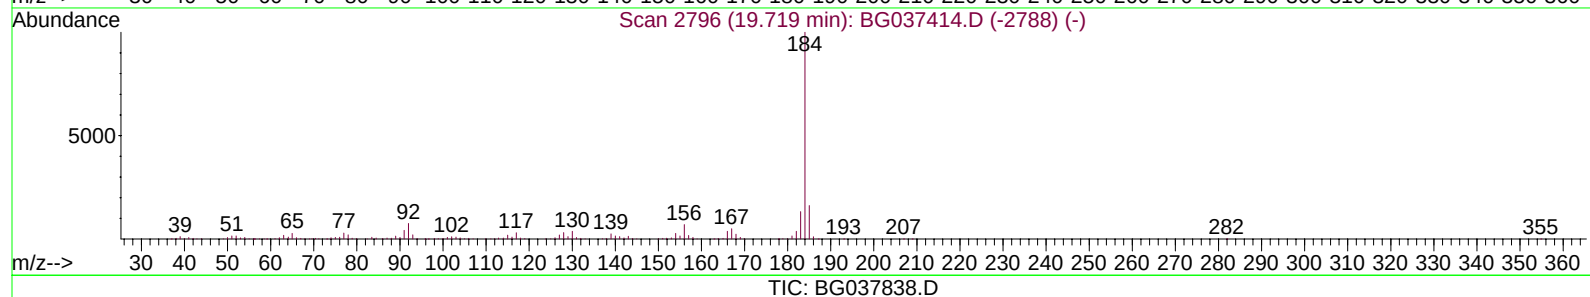
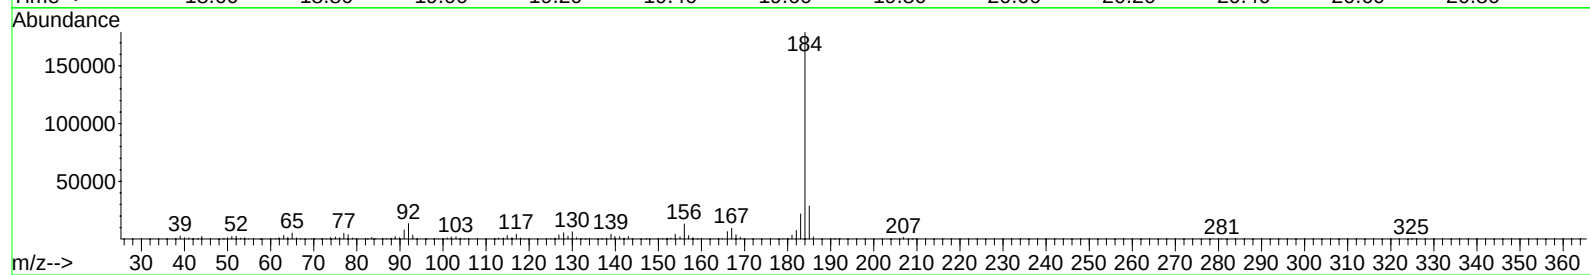


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110618\
Data File : BG037838.D
Acq On : 6 Nov 2018 14:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 17:41:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

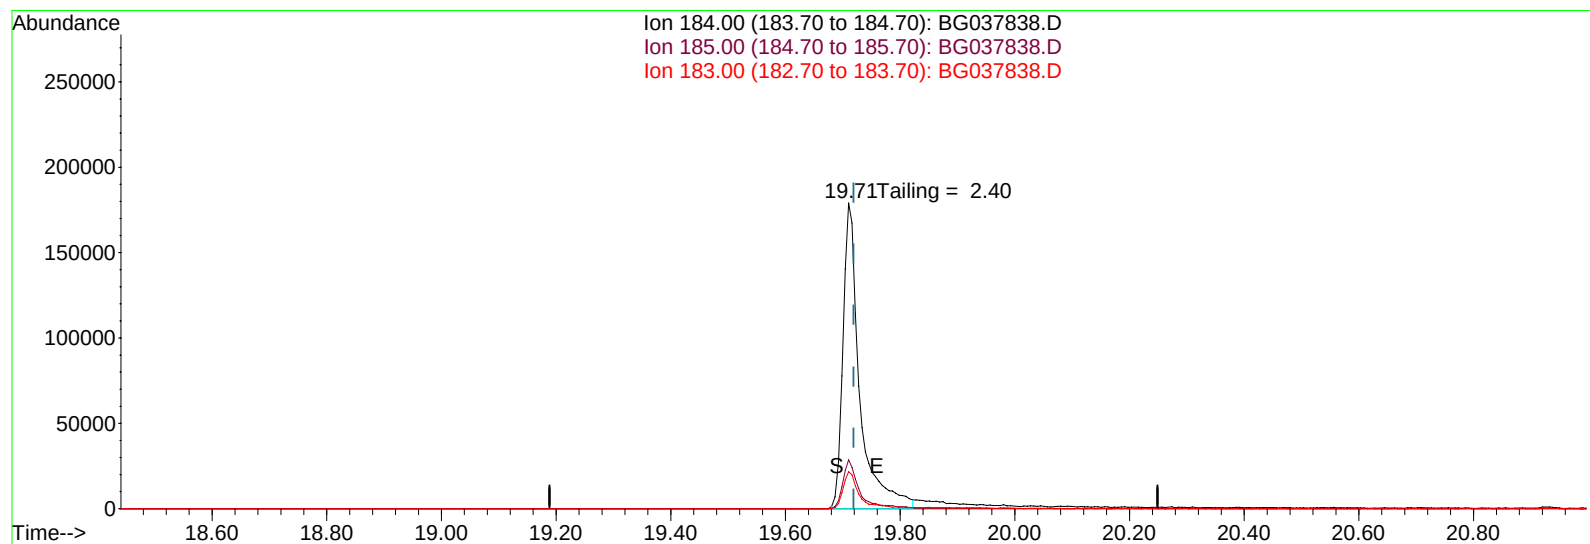

(77) Benzidine


19.710min (-0.009) 90487.06ng

response 390753

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.04
183.00	12.70	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110618\
Data File : BG037838.D
Acq On : 6 Nov 2018 14:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 17:41:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

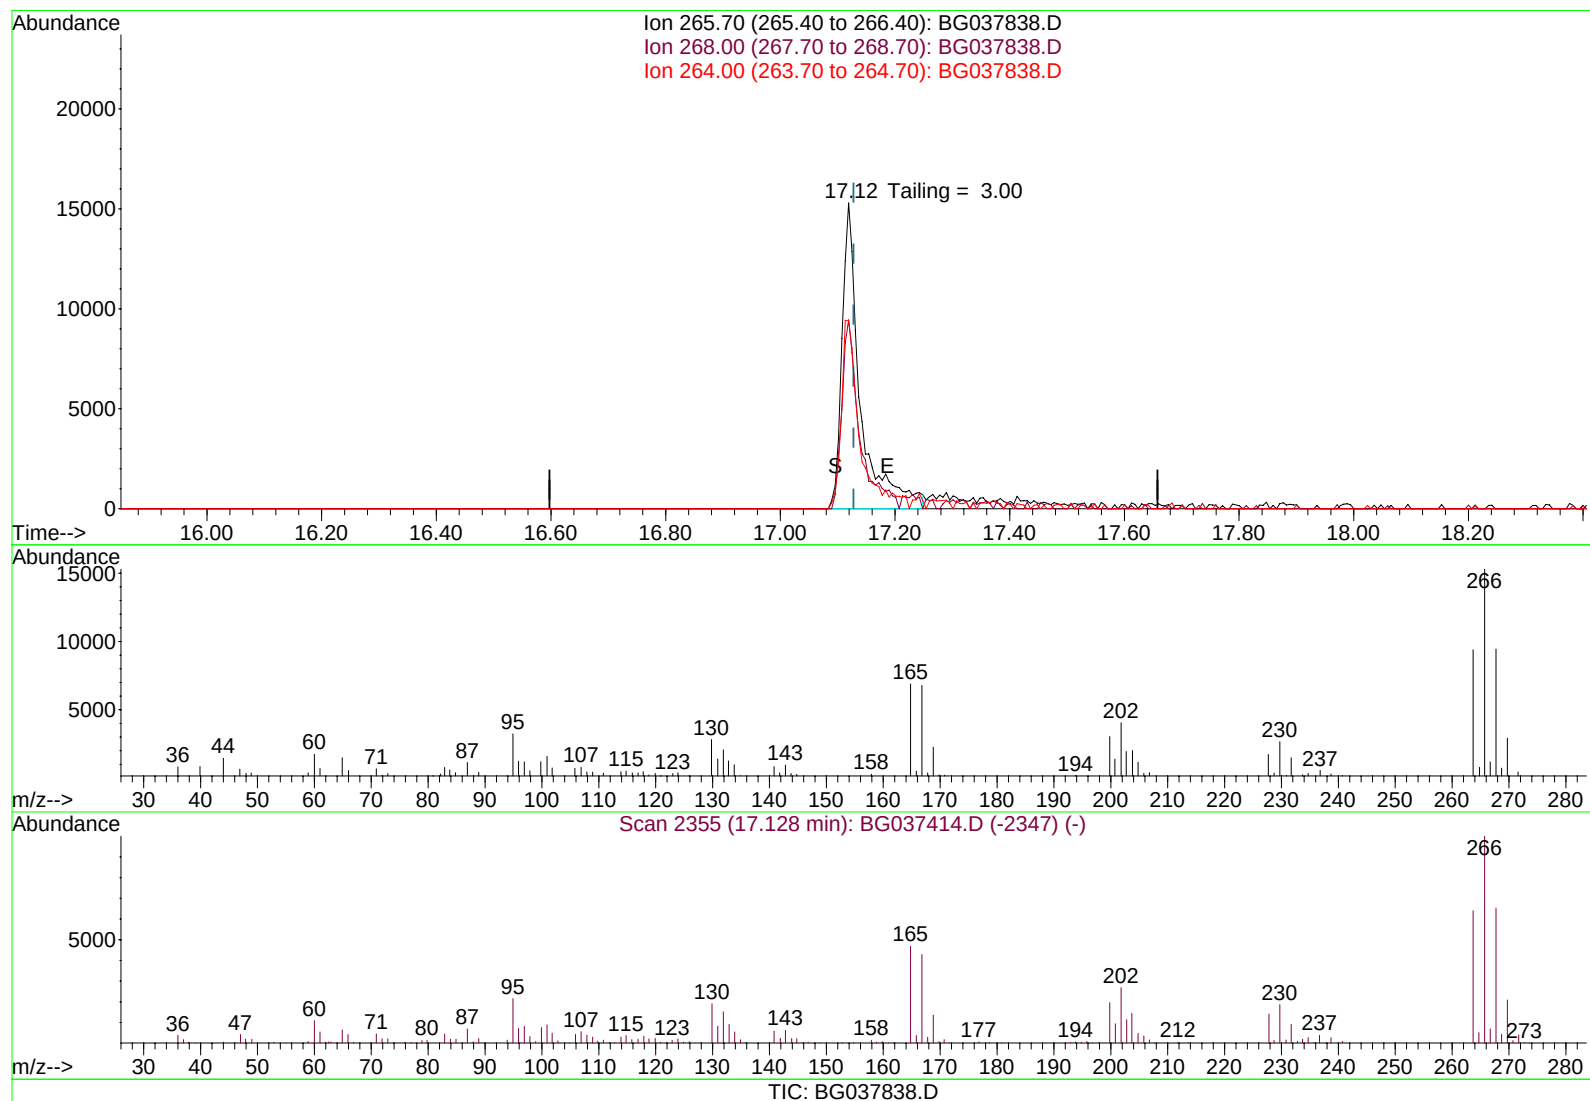

(70) Pentachlorophenol (C)

17.119min (-0.009) 11401.53ng

response 34421

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.54
264.00	73.60	61.46
0.00	0.00	0.00