

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110618\
 Data File : BG037844.D
 Acq On : 6 Nov 2018 18:44
 Operator : JU/SJ
 Sample : J5819-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BES48_SB02_3.5-4

Quant Time: Nov 07 09:35:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	53966	20.00	ng	-0.01
21) Naphthalene-d8	10.92	136	244683	20.00	ng	-0.01
39) Acenaphthene-d10	14.73	164	161381	20.00	ng	-0.01
64) Phenanthrene-d10	17.47	188	347496	20.00	ng	-0.01
76) Chrysene-d12	21.76	240	305310	20.00	ng	-0.02
87) Perylene-d12	25.09	264	270969	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	449872	139.37	ng	-0.01
7) Phenol-d6	7.24	99	681878	139.70	ng	-0.01
23) Nitrobenzene-d5	9.27	82	413717	94.72	ng	-0.01
42) 2,4,6-Tribromophenol	16.22	330	232708	132.21	ng	-0.01
45) 2-Fluorobiphenyl	13.35	172	992395	92.73	ng	-0.02
79) Terphenyl-d14	20.08	244	1314071	91.97	ng	-0.01
Target Compounds						
10) Phenol	7.27	94	54278	10.539	ng	Qvalue 97
50) Dimethylphthalate	14.17	163	136653	10.946	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110618\
Data File : BG037844.D
Acq On : 6 Nov 2018 18:44
Operator : JU/SJ
Sample : J5819-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BES48_SB02_3.5-4

Quant Time: Nov 07 09:35:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

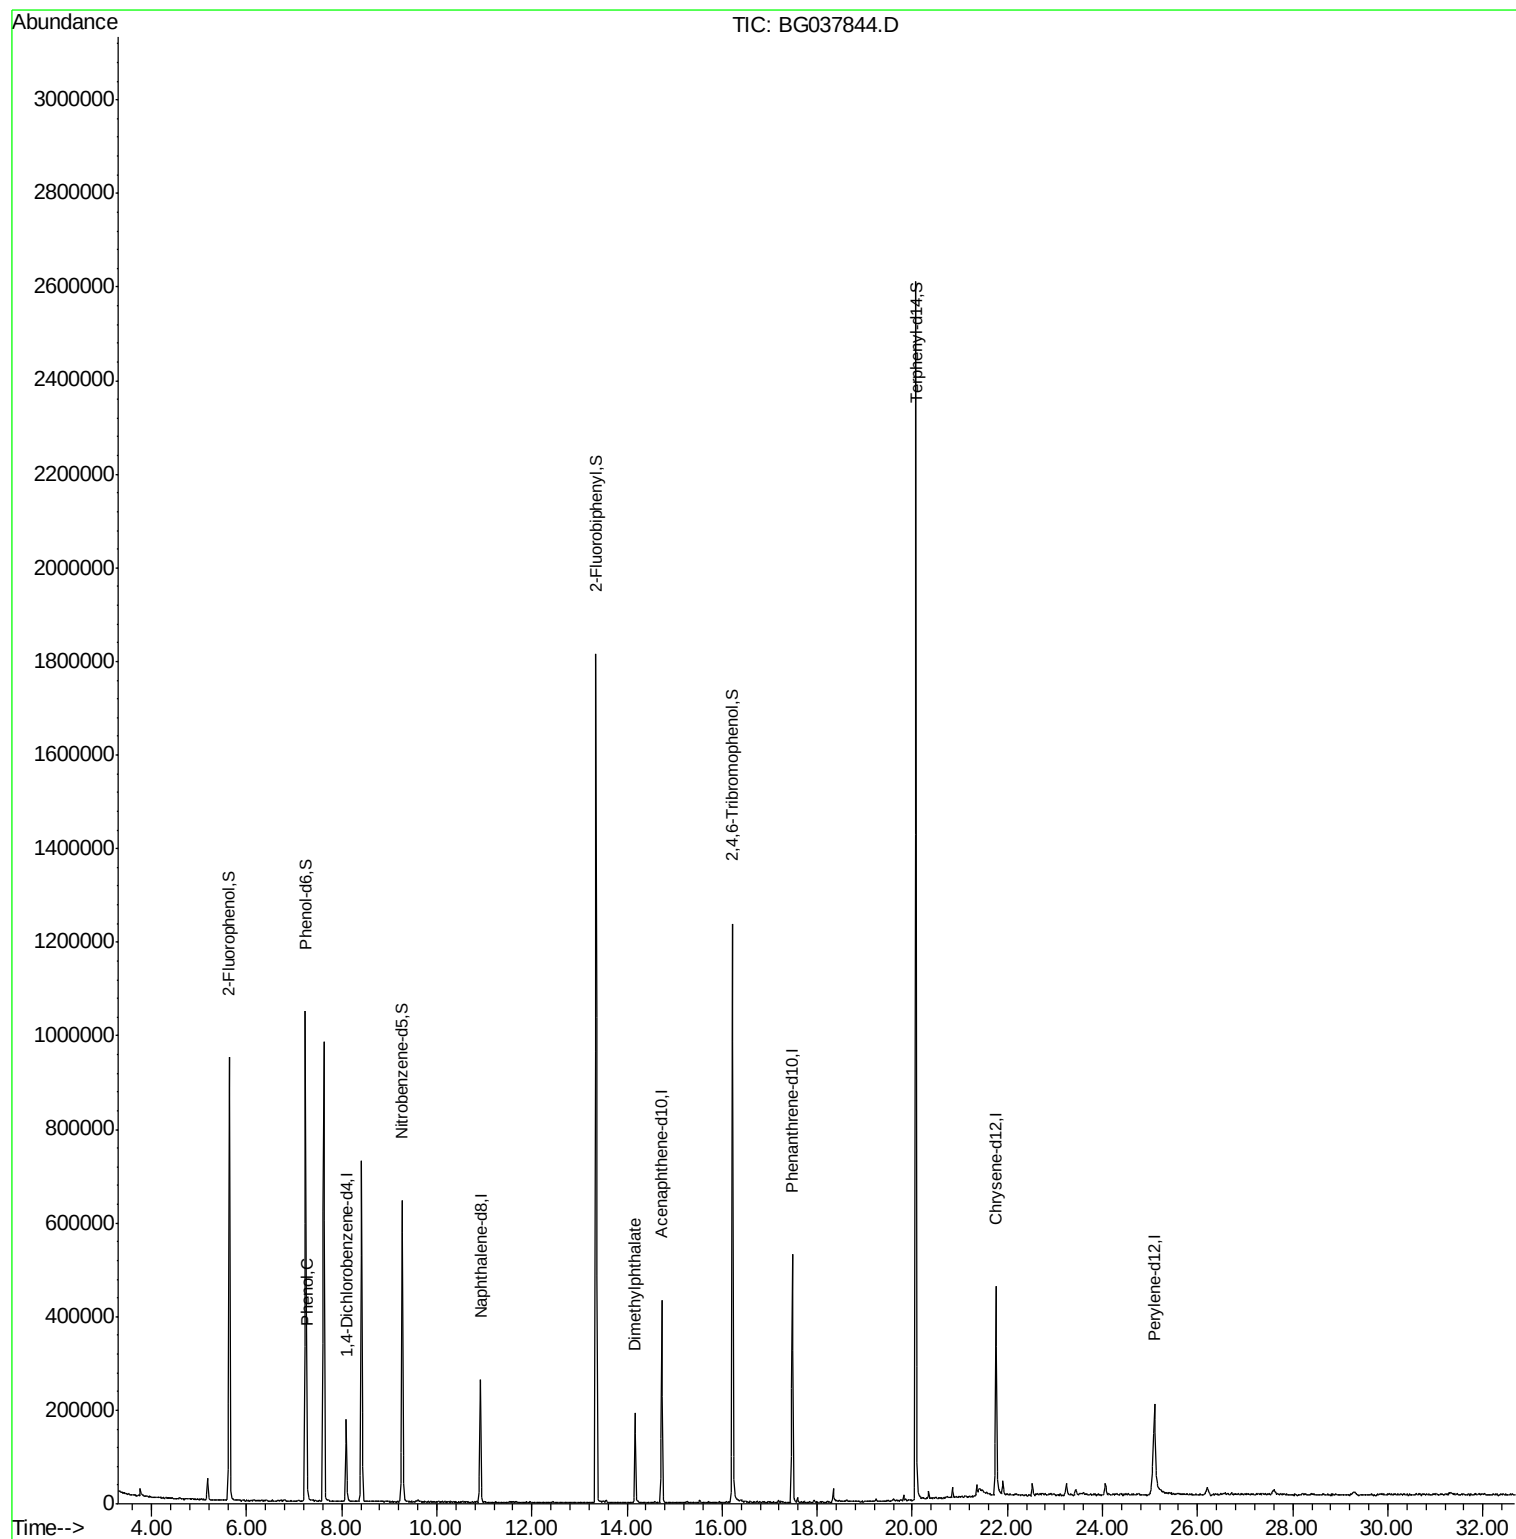

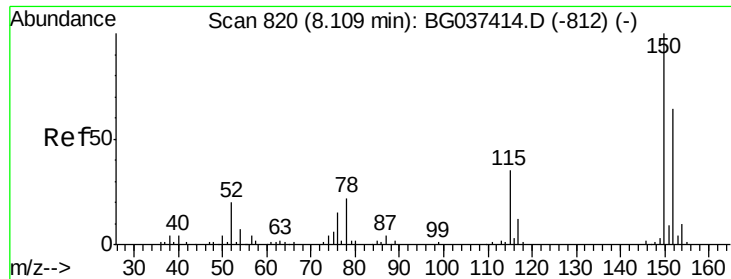


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 818
Delta R.T. -0.01 min
Lab File: BG037844.D
Acq: 6 Nov 2018 18:44

Instrument :
BNA_G
ClientSampleId :
BES48_SB02_3.5-4

Tgt Ion:152 Resp: 53966
Ion Ratio Lower Upper
152 100
150 160.1 126.0 189.0
115 60.5 45.5 68.3

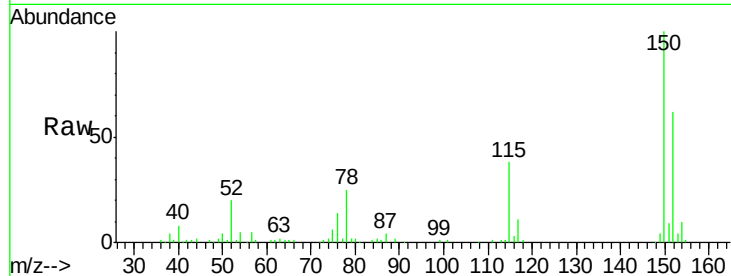


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

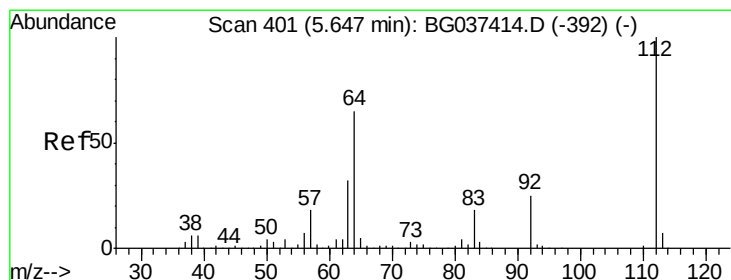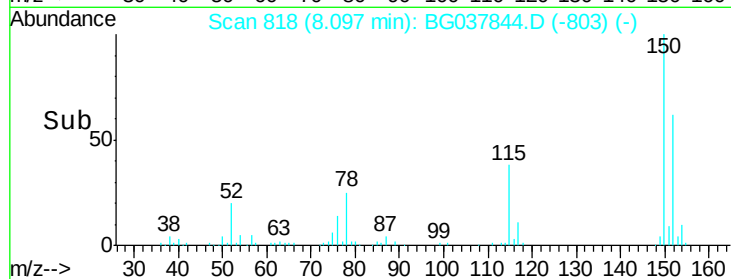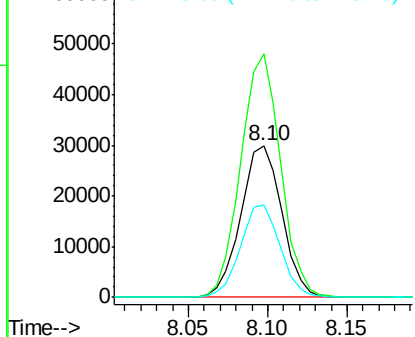



#5


2-Fluorophenol
Concen: 139.369 ng
RT: 5.64 min Scan# 399
Delta R.T. -0.01 min
Lab File: BG037844.D
Acq: 6 Nov 2018 18:44

Tgt Ion:112 Resp: 449872
Ion Ratio Lower Upper
112 100
64 66.0 53.1 79.7
63 33.7 27.3 40.9

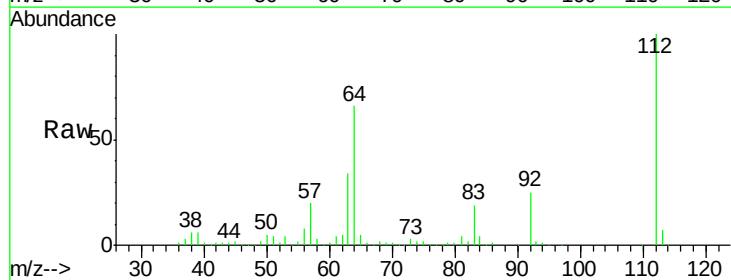

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

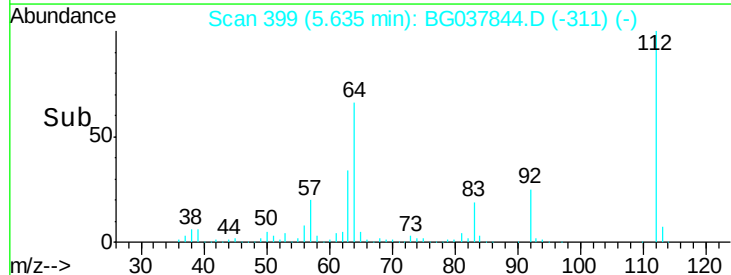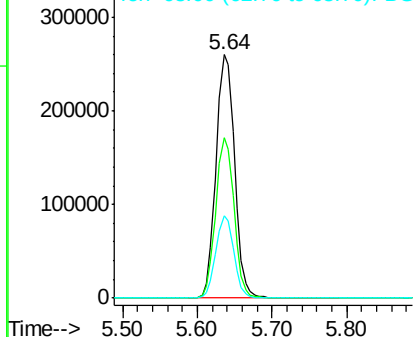

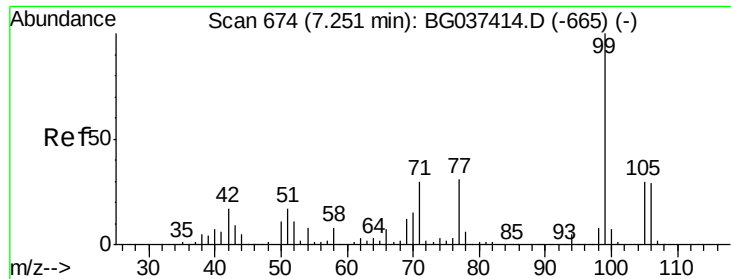

#7

Phenol-d6

Concen: 139.700 ng

RT: 7.24 min Scan# 672

Delta R.T. -0.01 min

Lab File: BG037844.D

Acq: 6 Nov 2018 18:44

Instrument :

BNA_G

ClientSampleId :

BES48_SB02_3.5-4


Tgt Ion: 99 Resp: 681878

Ion Ratio Lower Upper




99 100

42 17.7 15.0 22.4

71 31.2 25.5 38.3

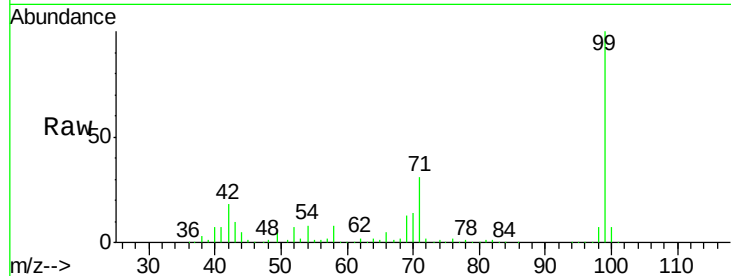

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

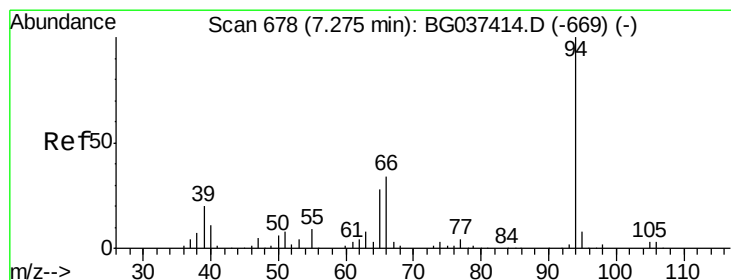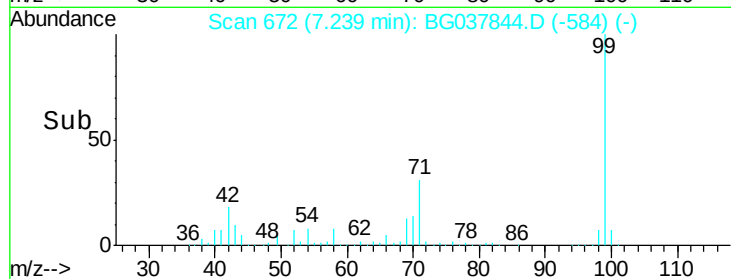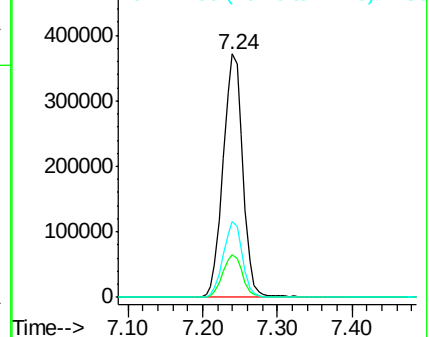

#10

Phenol

Concen: 10.539 ng

RT: 7.27 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG037844.D

Acq: 6 Nov 2018 18:44


Tgt Ion: 94 Resp: 54278

Ion Ratio Lower Upper



94 100


65 27.1 9.7 49.7

66 36.5 15.9 55.9

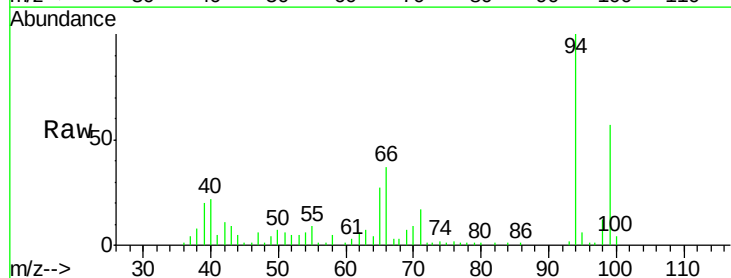

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

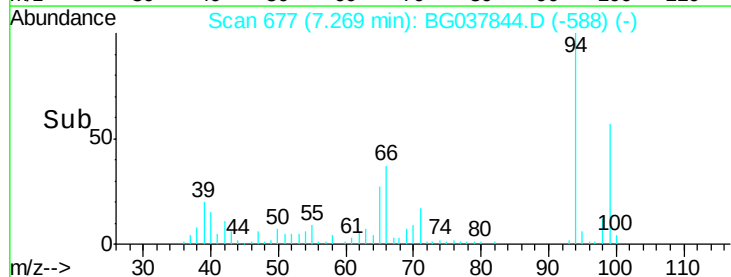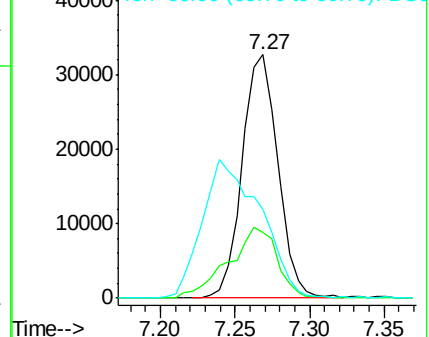


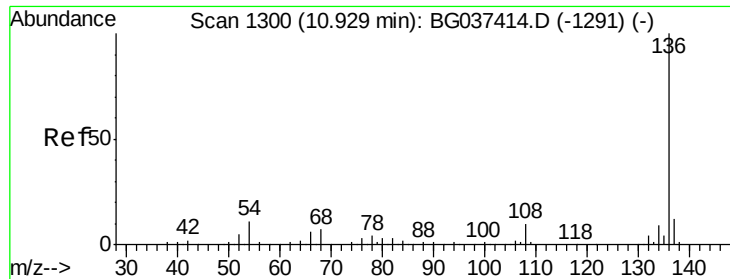




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.92 min Scan# 1298
Delta R.T. -0.01 min
Lab File: BG037844.D
Acq: 6 Nov 2018 18:44

Instrument :
BNA_G
ClientSampleId :
BES48_SB02_3.5-4

Tgt Ion:	136	Resp:	244683
Ion	Ratio	Lower	Upper
136	100		
137	10.4	9.6	14.4
54	10.0	7.9	11.9
68	6.4	4.8	7.2

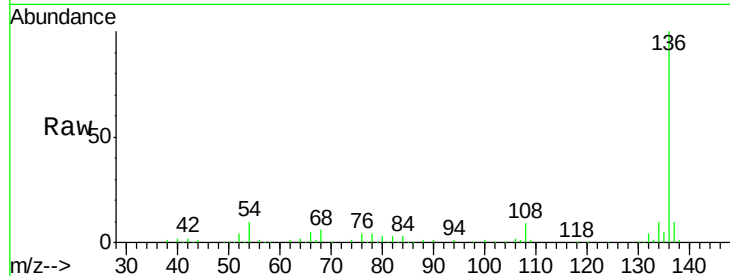


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

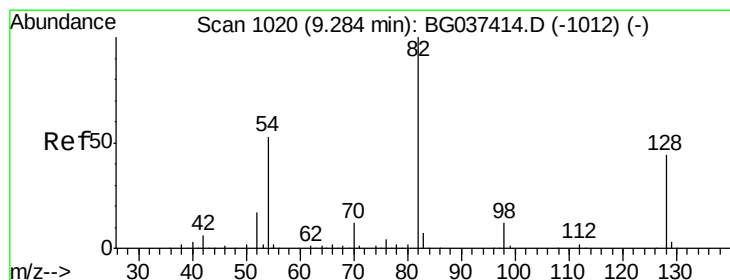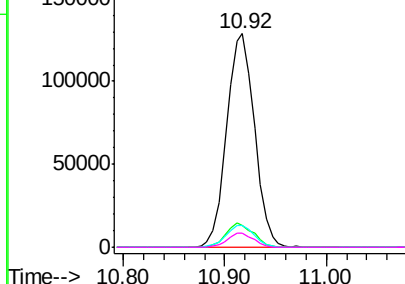
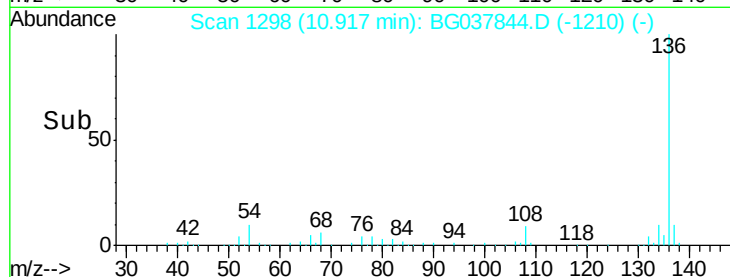



#23
Nitrobenzene-d5
Concen: 94.718 ng
RT: 9.27 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BG037844.D
Acq: 6 Nov 2018 18:44

Tgt Ion:	82	Resp:	413717
Ion	Ratio	Lower	Upper
82	100		
128	44.6	34.6	51.8
54	54.4	45.3	67.9

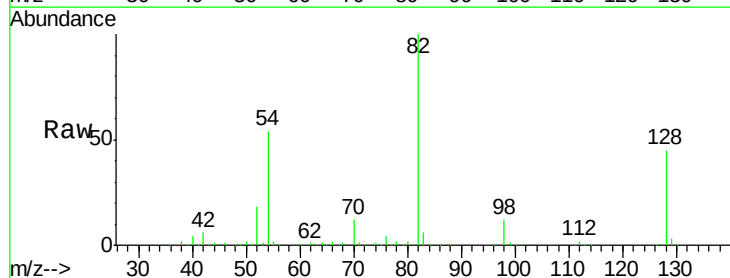

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

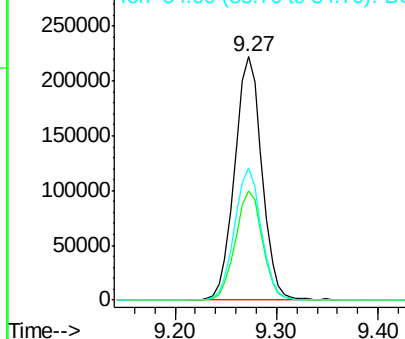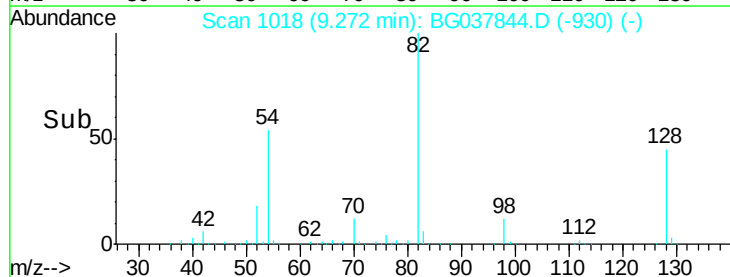

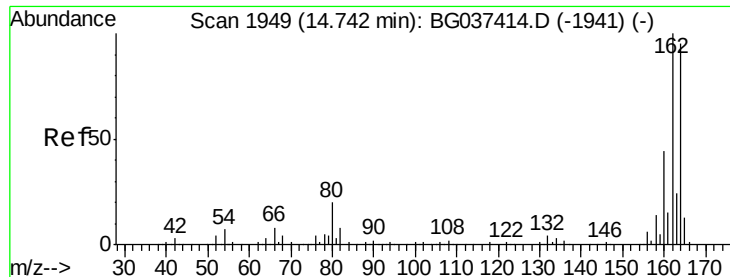

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.73 min Scan# 1947

Delta R.T. -0.01 min

Lab File: BG037844.D

Acq: 6 Nov 2018 18:44

Instrument :

BNA_G

ClientSampleId :

BES48_SB02_3.5-4


Tgt Ion:164 Resp: 161381

Ion Ratio Lower Upper

164 100

162 100.0 81.3 121.9




160 45.3 36.3 54.5

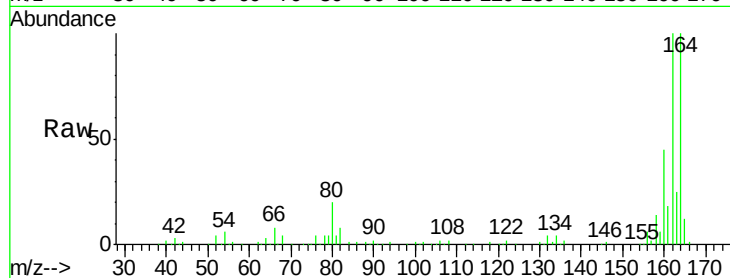

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

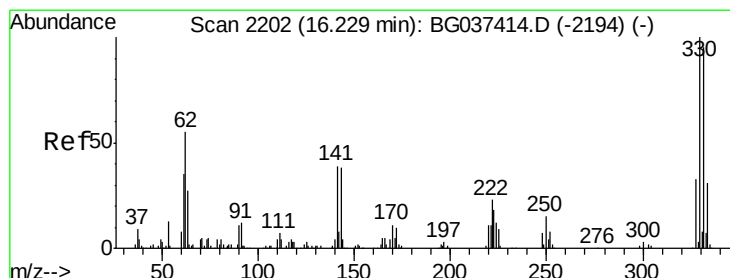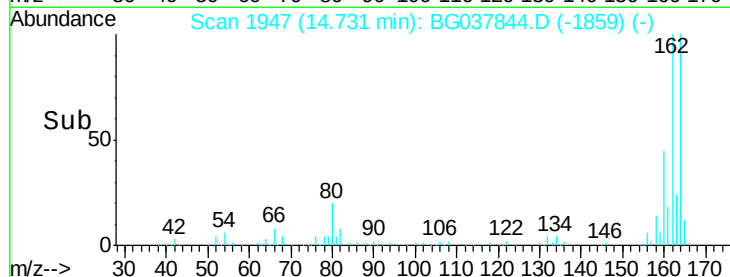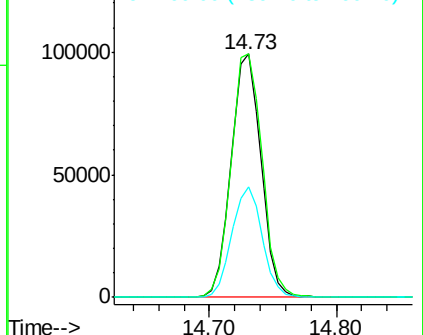

#42

2,4,6-Tribromophenol

Concen: 132.208 ng

RT: 16.22 min Scan# 2200

Delta R.T. -0.01 min

Lab File: BG037844.D

Acq: 6 Nov 2018 18:44


Tgt Ion:330 Resp: 232708

Ion Ratio Lower Upper

330 100

332 94.7 78.4 117.6



141 38.8 32.2 48.2

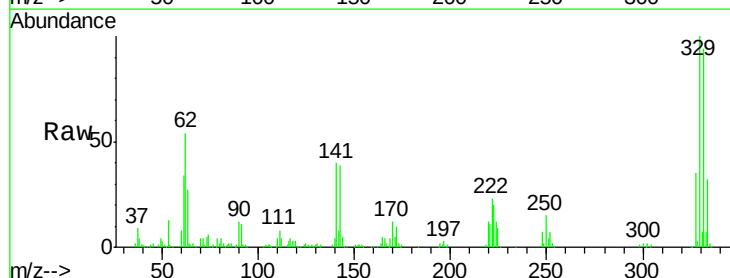


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



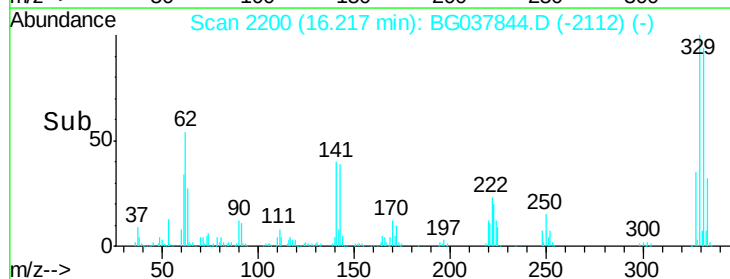
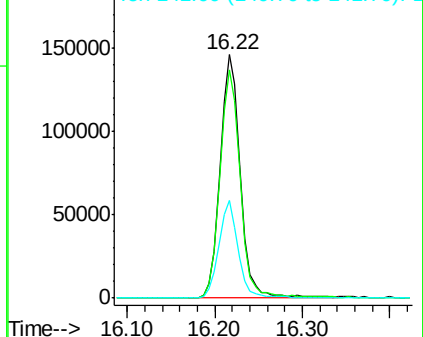


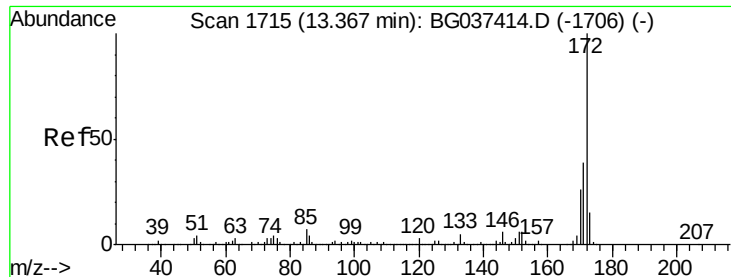

#45
 2-Fluorobiphenyl
 Concen: 92.729 ng
 RT: 13.35 min Scan# 1712
 Delta R.T. -0.02 min
 Lab File: BG037844.D
 Acq: 6 Nov 2018 18:44




Instrument :
 BNA_G
 ClientSampleId :
 BES48_SB02_3.5-4


Tgt Ion:	172	Resp:	992395
Ion	Ratio	Lower	Upper
172	100		
171	38.2	31.0	46.4
170	25.2	20.2	30.2

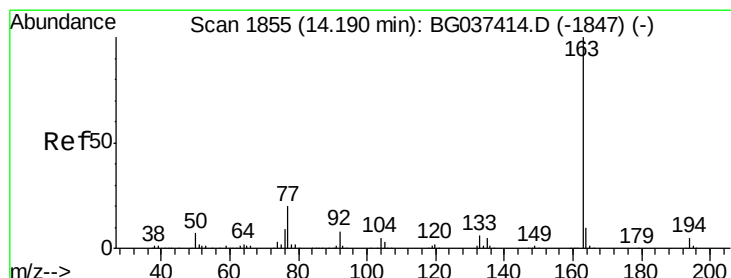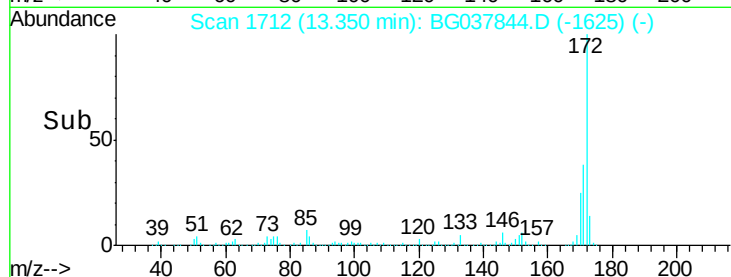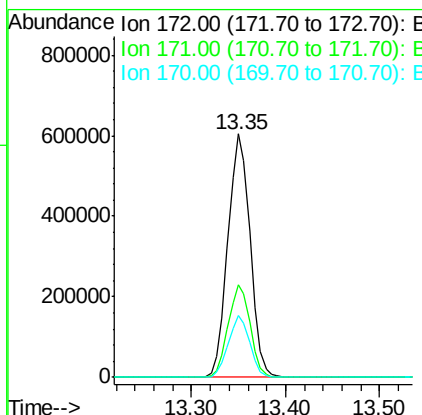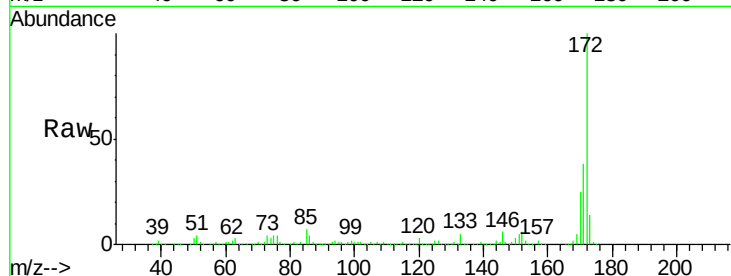

#50
 Dimethylphthalate
 Concen: 10.946 ng
 RT: 14.17 min Scan# 1852
 Delta R.T. -0.02 min
 Lab File: BG037844.D
 Acq: 6 Nov 2018 18:44

Tgt Ion:	163	Resp:	136653
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.5	5.3
164	9.8	8.5	12.7


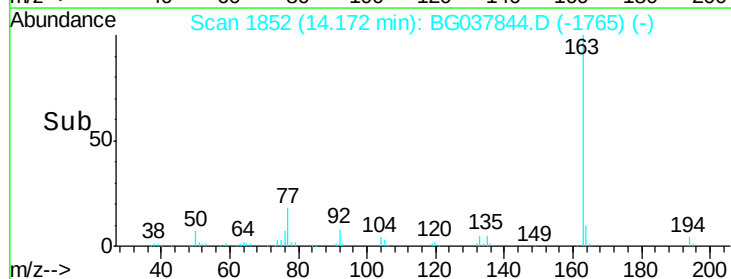
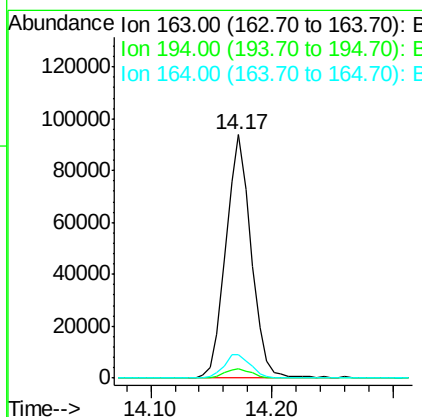
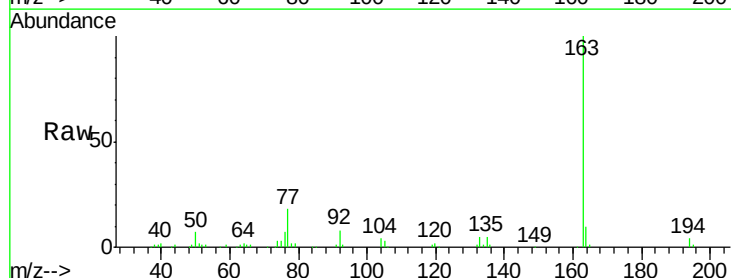


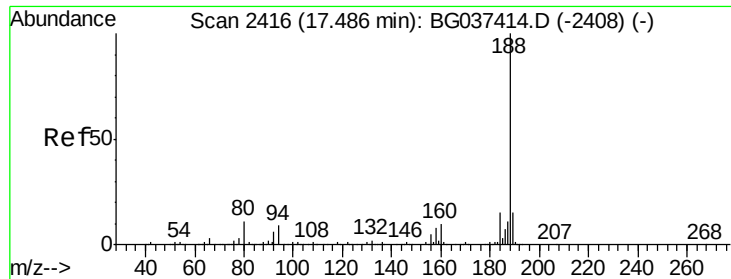

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2414
Delta R.T. -0.01 min
Lab File: BG037844.D
Acq: 6 Nov 2018 18:44




Instrument :
BNA_G
ClientSampleId :
BES48_SB02_3.5-4


Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.7	7.2	10.8
80	9.9	7.7	11.5

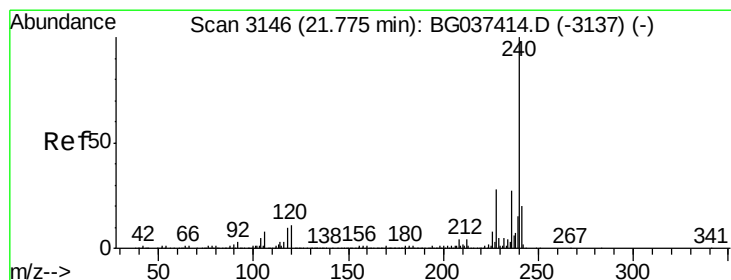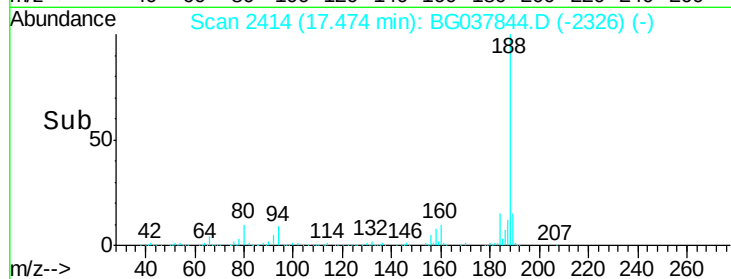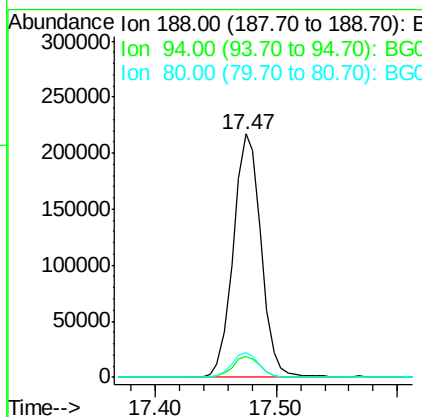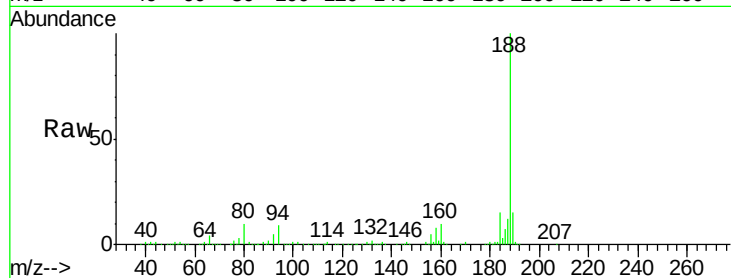

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3143
Delta R.T. -0.02 min
Lab File: BG037844.D
Acq: 6 Nov 2018 18:44

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.4	8.1	12.1
236	26.7	21.4	32.0

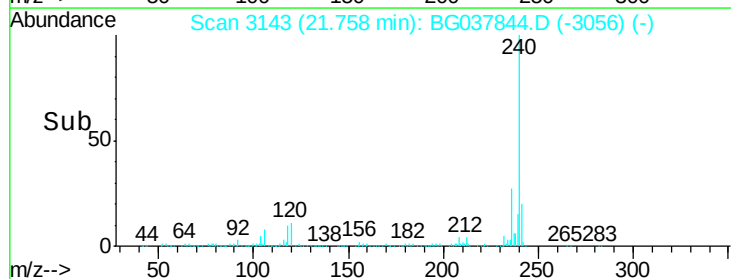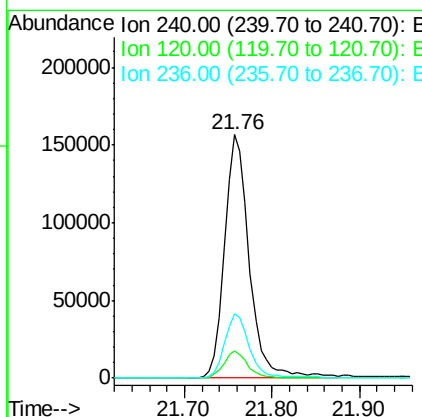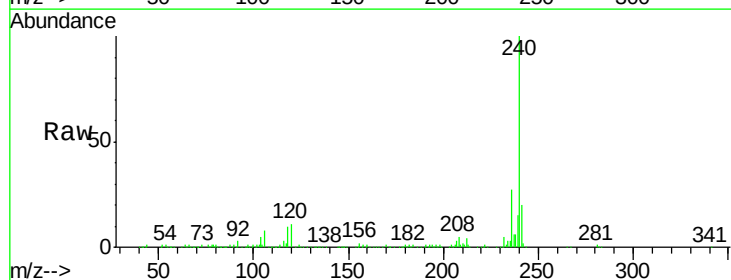

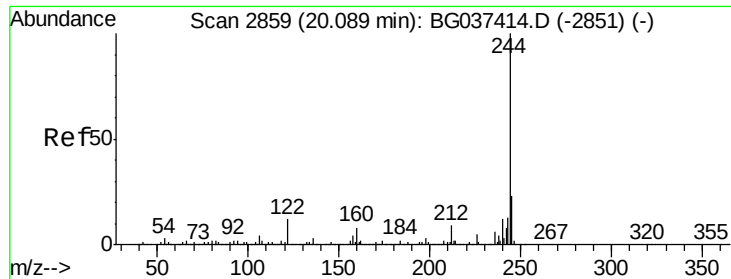

#79

Terphenyl-d14

Concen: 91.968 ng

RT: 20.08 min Scan# 2857

Delta R.T. -0.01 min

Lab File: BG037844.D

Acq: 6 Nov 2018 18:44

Instrument :

BNA_G

ClientSampleId :

BES48_SB02_3.5-4


Tgt Ion:244 Resp: 1314071

Ion Ratio Lower Upper

244 100

212 8.2 6.5 9.7




122 10.8 9.0 13.4

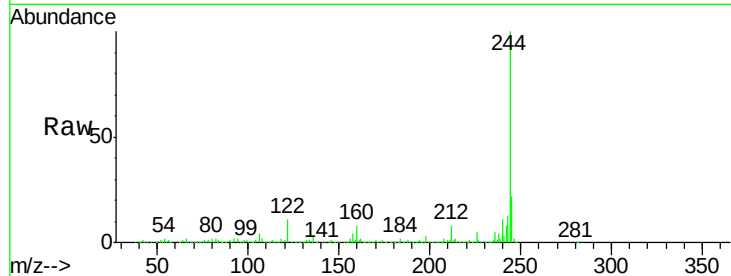

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

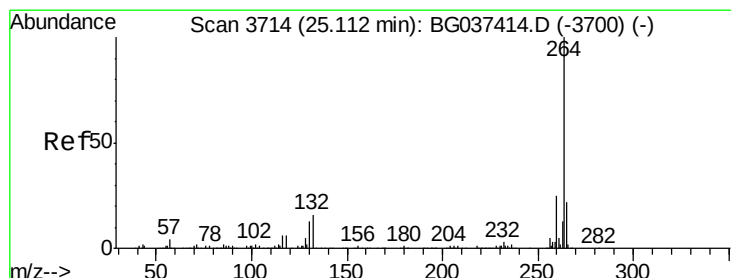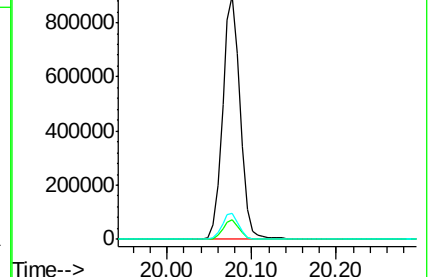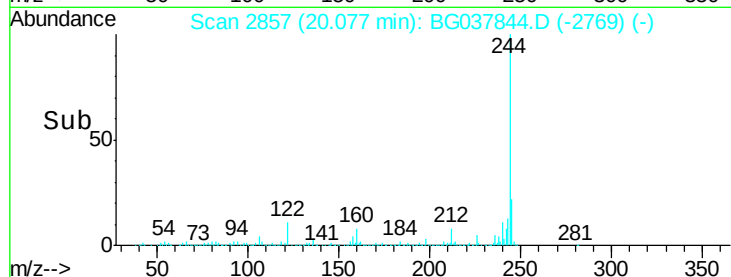

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3710

Delta R.T. -0.02 min

Lab File: BG037844.D

Acq: 6 Nov 2018 18:44


Tgt Ion:264 Resp: 270969

Ion Ratio Lower Upper

264 100

260 23.7 18.2 27.4

265 22.5 17.9 26.9

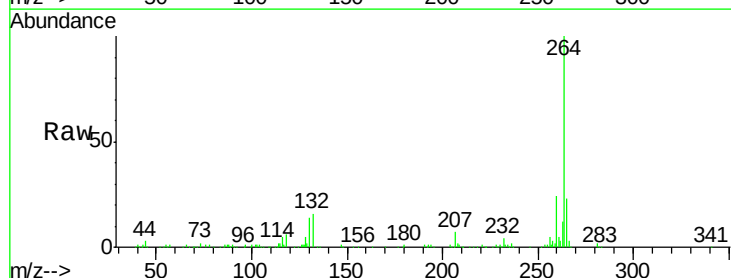

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

