

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110618\
 Data File : BG037852.D
 Acq On : 6 Nov 2018 23:56
 Operator : JU/SJ
 Sample : J5764-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-03-110218-A

Quant Time: Nov 07 09:44:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	53060	20.00	ng	-0.01
21) Naphthalene-d8	10.91	136	236985	20.00	ng	-0.01
39) Acenaphthene-d10	14.73	164	159354	20.00	ng	-0.01
64) Phenanthrene-d10	17.48	188	352645	20.00	ng	0.00
76) Chrysene-d12	21.76	240	309403	20.00	ng	-0.01
87) Perylene-d12	25.09	264	226991	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	372525	117.38	ng	0.00
7) Phenol-d6	7.24	99	492055	102.53	ng	-0.01
23) Nitrobenzene-d5	9.27	82	369851	87.43	ng	-0.01
42) 2,4,6-Tribromophenol	16.21	330	179529	103.29	ng	-0.01
45) 2-Fluorobiphenyl	13.35	172	909544	86.07	ng	-0.01
79) Terphenyl-d14	20.07	244	1290980	89.16	ng	-0.01


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110618\
Data File : BG037852.D
Acq On : 6 Nov 2018 23:56
Operator : JU/SJ
Sample : J5764-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-03-110218-A

Quant Time: Nov 07 09:44:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration




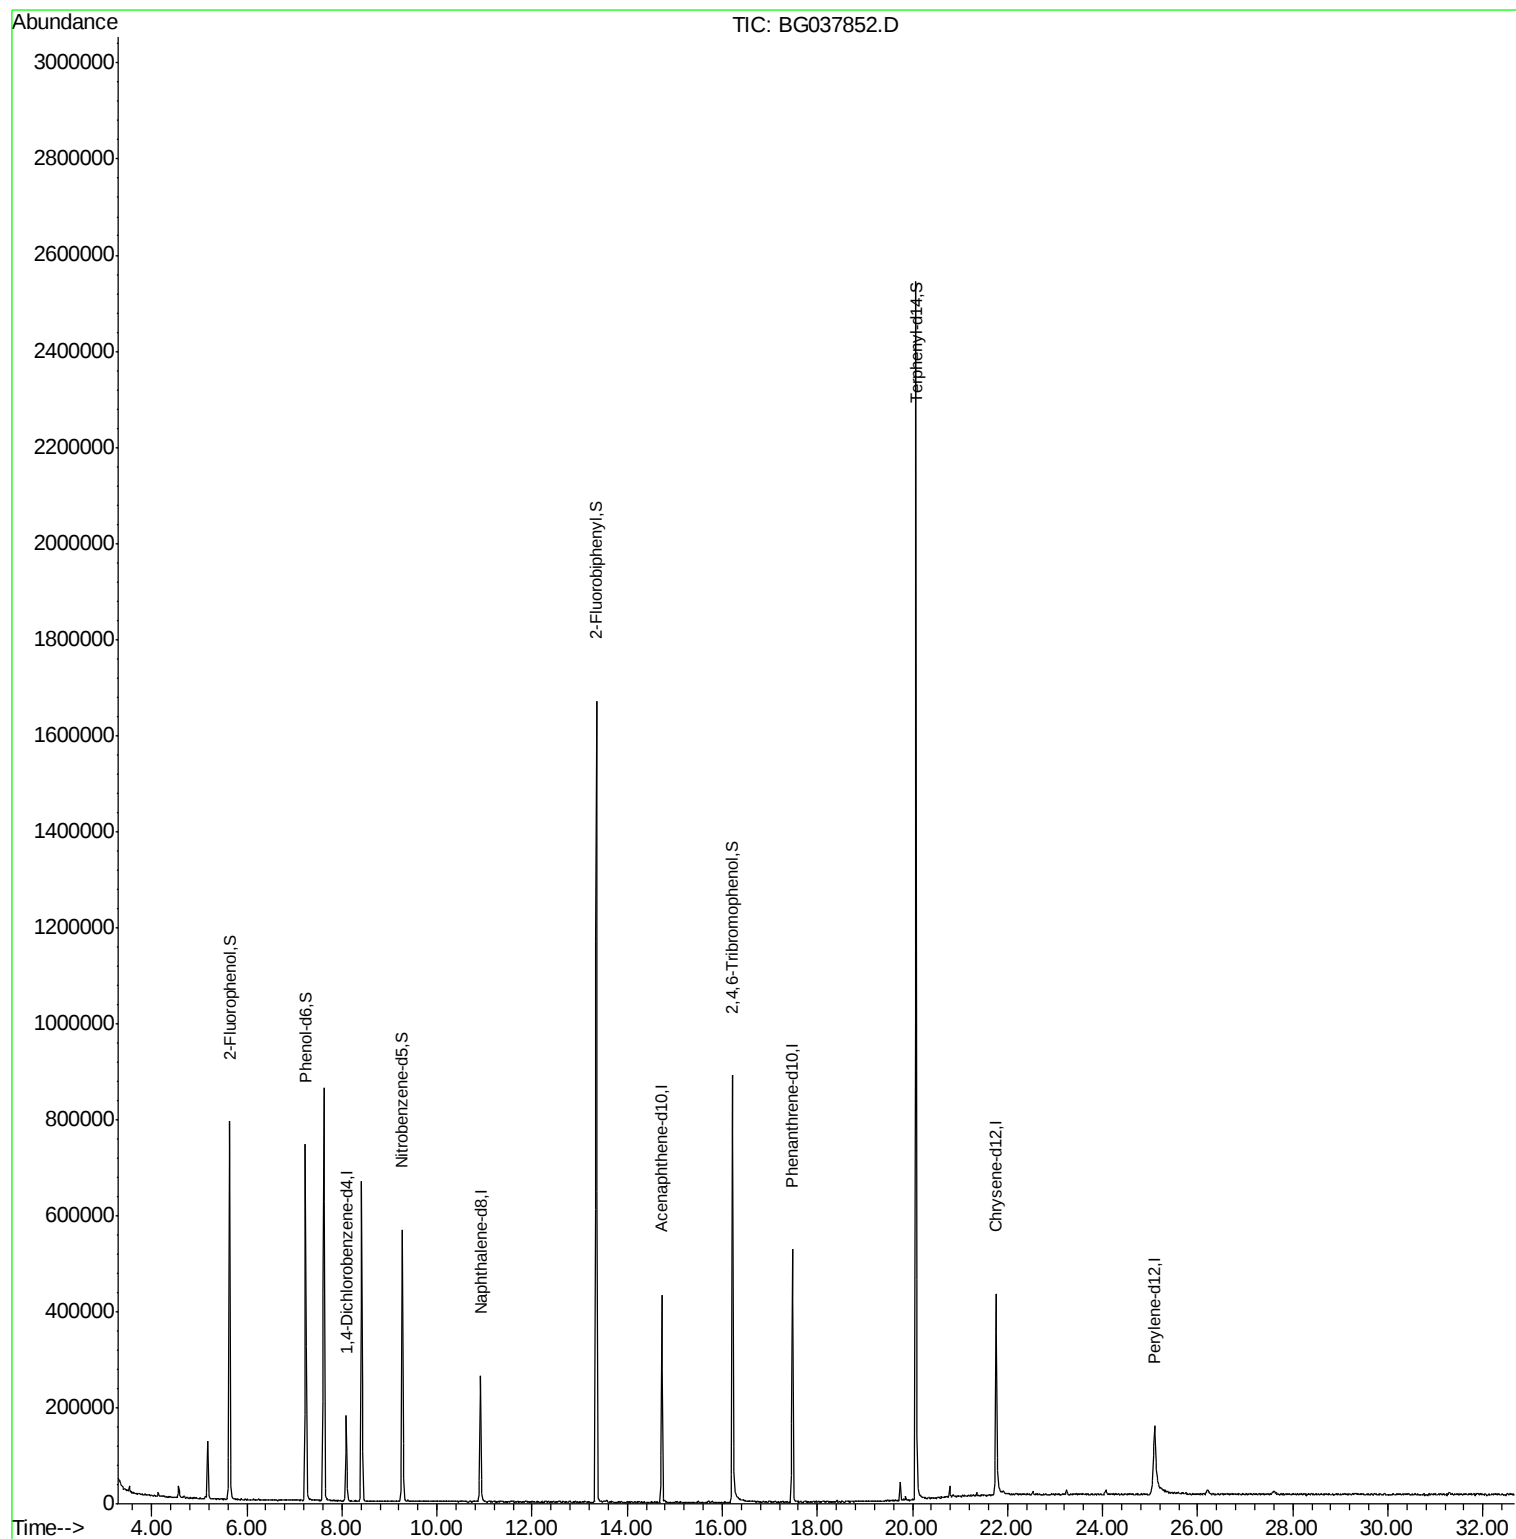




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.09 min Scan# 818
 Delta R.T. -0.01 min
 Lab File: BG037852.D
 Acq: 6 Nov 2018 23:56




Instrument :
 BNA_G
 ClientSampleId :
 JC-03-110218-A

Tgt Ion:152 Resp: 53060
 Ion Ratio Lower Upper
 152 100
 150 157.7 126.0 189.0
 115 52.6 45.5 68.3

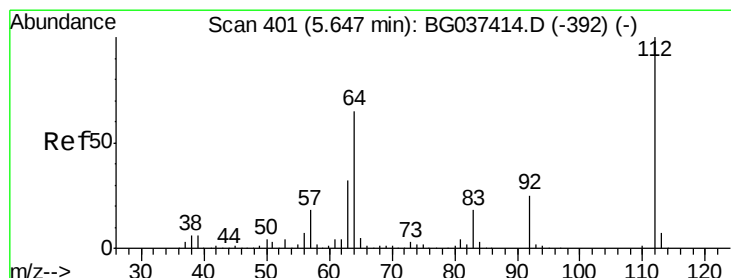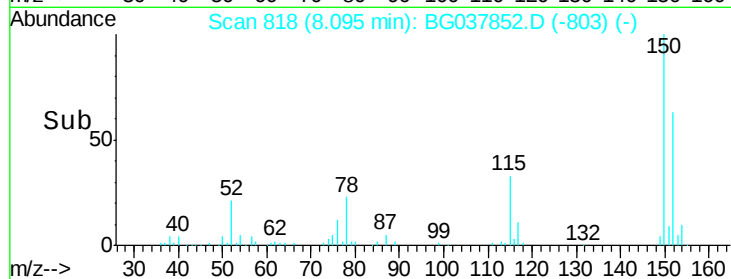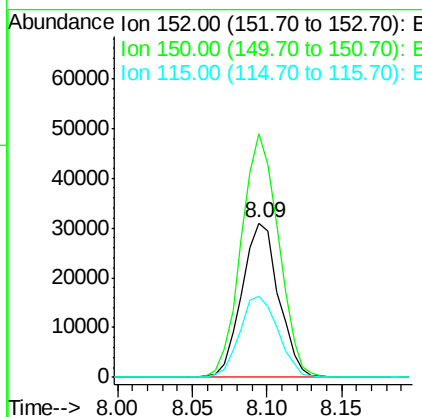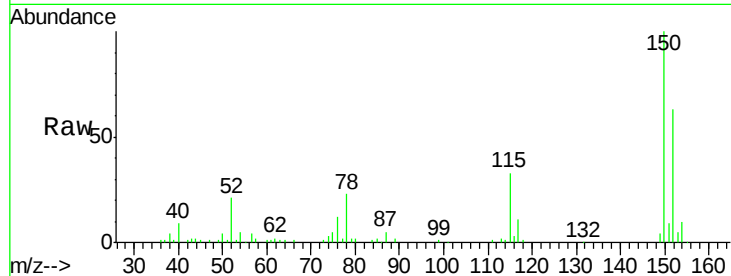

#5
 2-Fluorophenol
 Concen: 117.378 ng
 RT: 5.64 min Scan# 400
 Delta R.T. -0.01 min
 Lab File: BG037852.D
 Acq: 6 Nov 2018 23:56

Tgt Ion:112 Resp: 372525
 Ion Ratio Lower Upper
 112 100
 64 63.6 53.1 79.7
 63 32.4 27.3 40.9

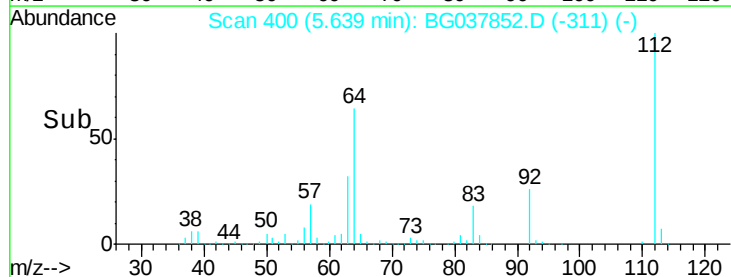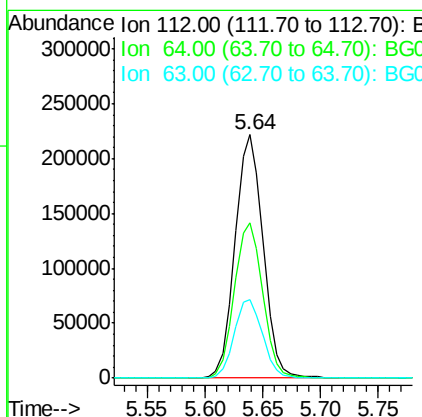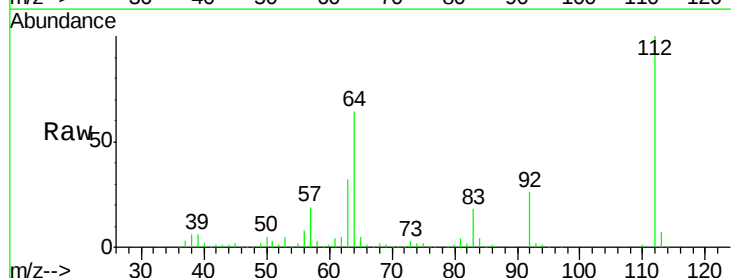



#7

Phenol-d6

Concen: 102.531 ng

RT: 7.24 min Scan# 672

Delta R.T. -0.01 min

Lab File: BG037852.D

Acq: 6 Nov 2018 23:56

Instrument :

BNA_G

ClientSampleId :

JC-03-110218-A


Tgt Ion: 99 Resp: 492055

Ion Ratio Lower Upper




99 100

42 17.6 15.0 22.4

71 30.6 25.5 38.3

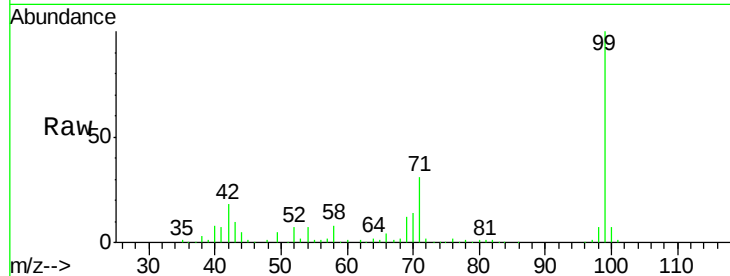

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

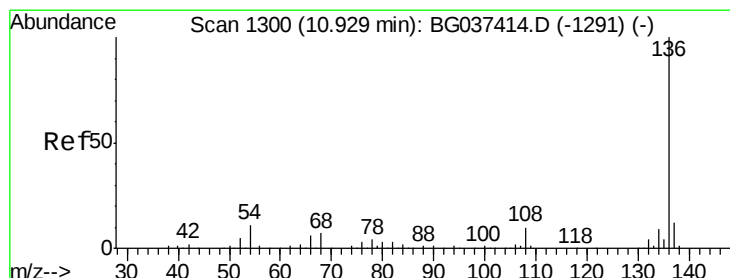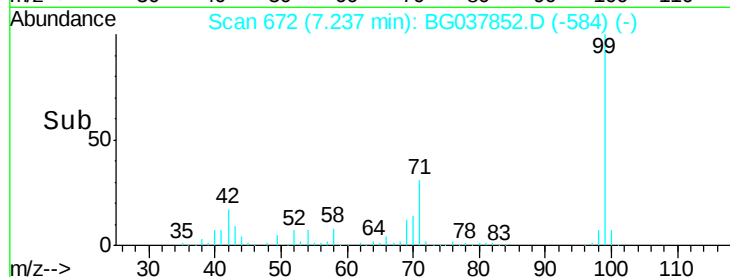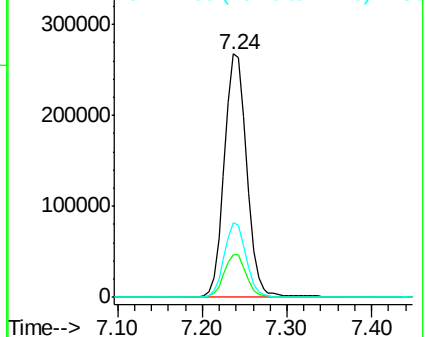

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.91 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BG037852.D

Acq: 6 Nov 2018 23:56

Tgt Ion: 136 Resp: 236985


Ion Ratio Lower Upper

136 100



137 12.2 9.6 14.4


54 11.0 7.9 11.9

68 6.5 4.8 7.2

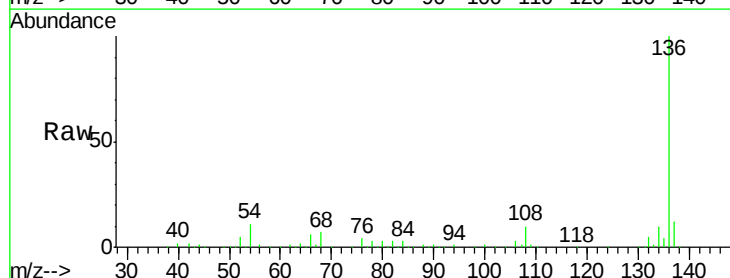

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

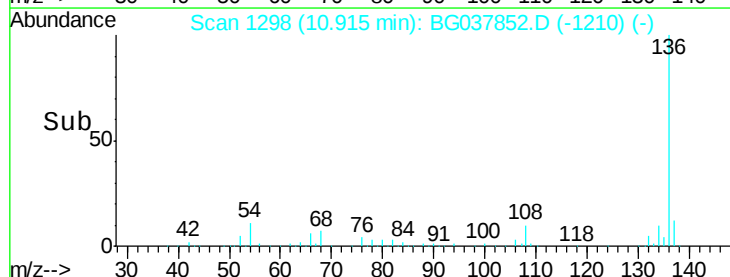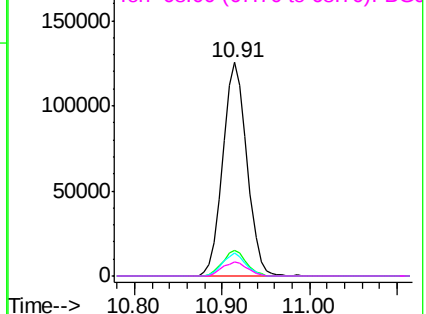


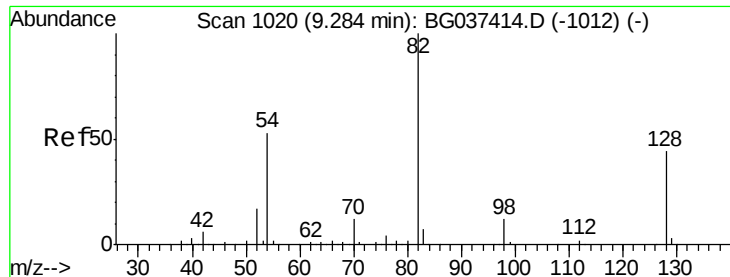




#23
Nitrobenzene-d5
Concen: 87.426 ng
RT: 9.27 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BG037852.D
Acq: 6 Nov 2018 23:56

Instrument :
BNA_G
ClientSampleId :
JC-03-110218-A

Tgt Ion: 82 Resp: 369851
Ion Ratio Lower Upper
82 100
128 45.9 34.6 51.8
54 54.0 45.3 67.9

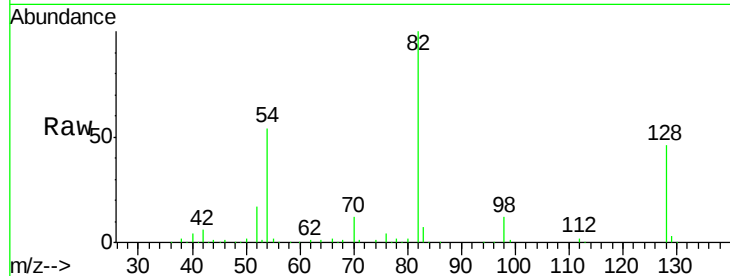


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

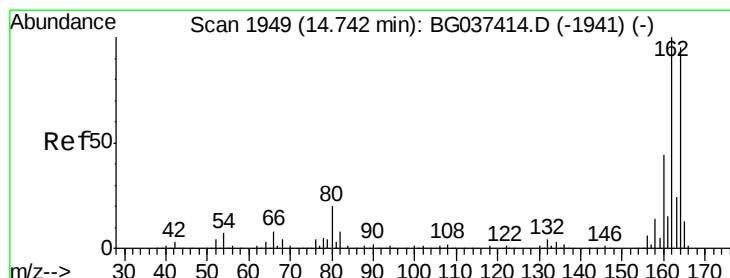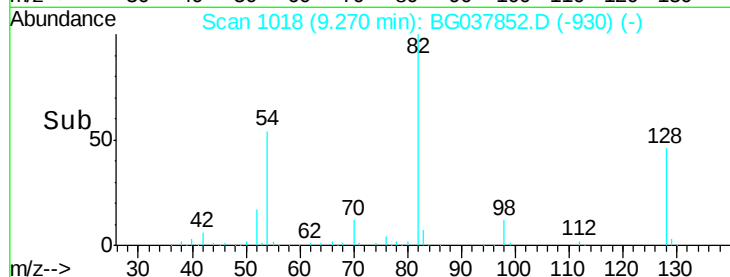
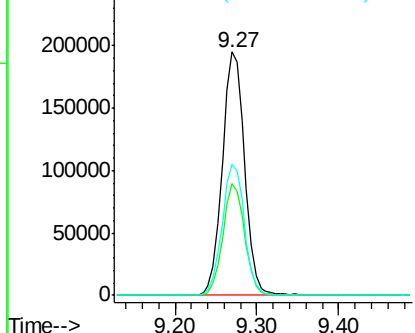



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1947
Delta R.T. -0.01 min
Lab File: BG037852.D
Acq: 6 Nov 2018 23:56

Tgt Ion: 164 Resp: 159354
Ion Ratio Lower Upper
164 100
162 101.1 81.3 121.9
160 43.1 36.3 54.5

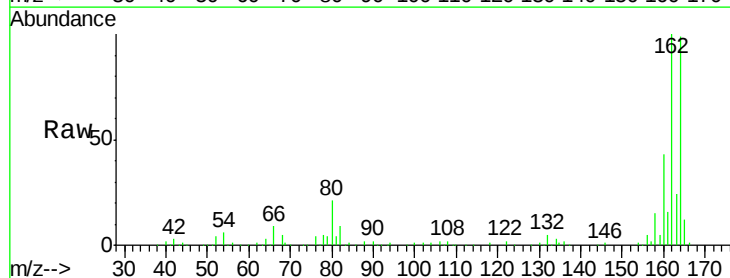

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

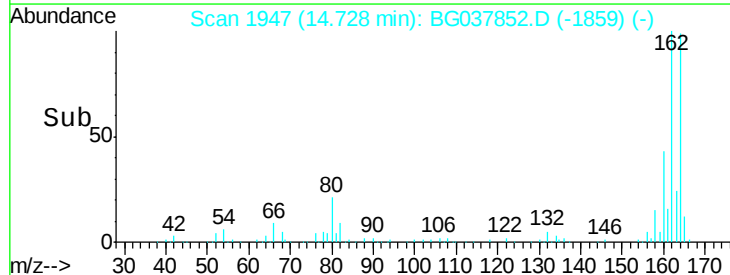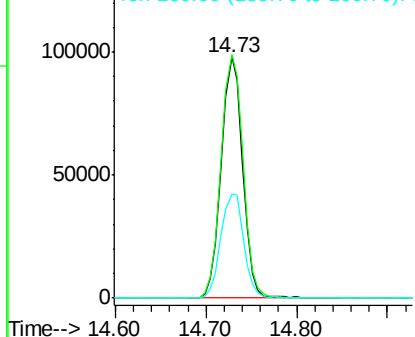


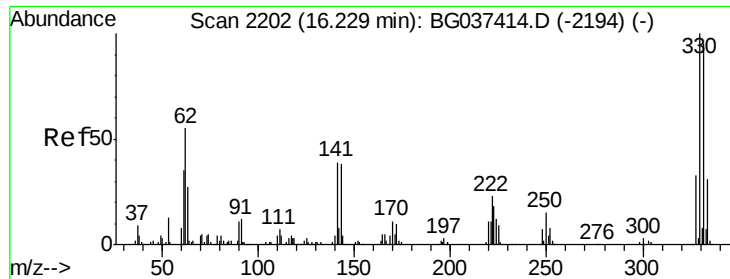




#42
 2,4,6-Tribromophenol
 Concen: 103.293 ng
 RT: 16.21 min Scan# 2200
 Delta R.T. -0.01 min
 Lab File: BG037852.D
 Acq: 6 Nov 2018 23:56

Instrument :
 BNA_G
 ClientSampleId :
 JC-03-110218-A

Tgt Ion:330 Resp: 179529
 Ion Ratio Lower Upper
 330 100
 332 95.8 78.4 117.6
 141 39.2 32.2 48.2

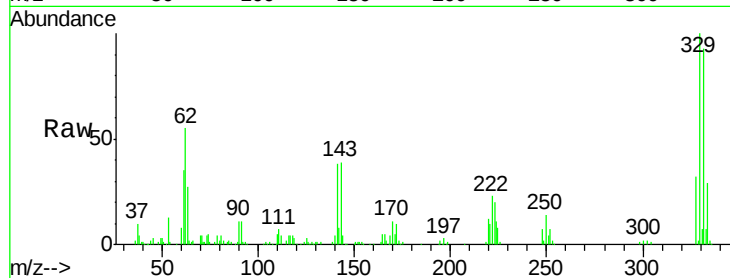


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

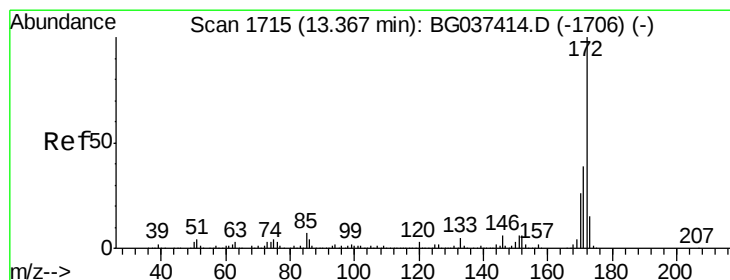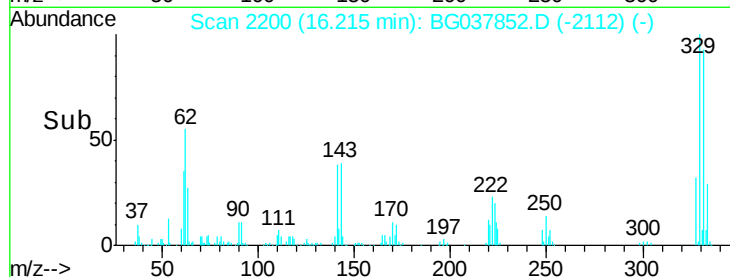
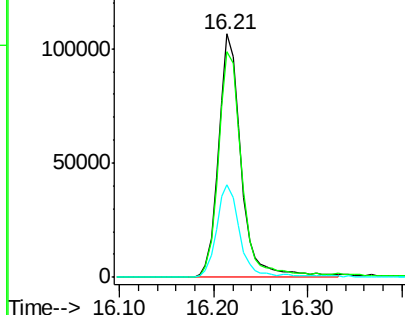



#45
 2-Fluorobiphenyl
 Concen: 86.069 ng
 RT: 13.35 min Scan# 1713
 Delta R.T. -0.01 min
 Lab File: BG037852.D
 Acq: 6 Nov 2018 23:56

Tgt Ion:172 Resp: 909544
 Ion Ratio Lower Upper
 172 100
 171 38.2 31.0 46.4
 170 25.4 20.2 30.2

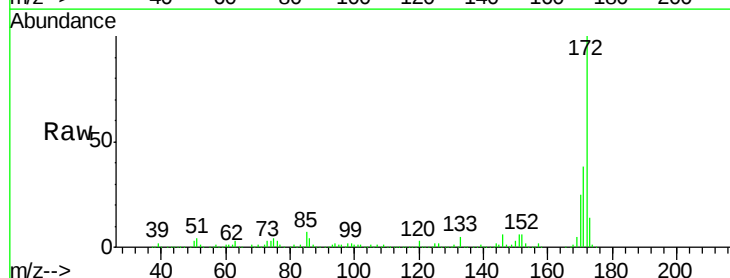

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



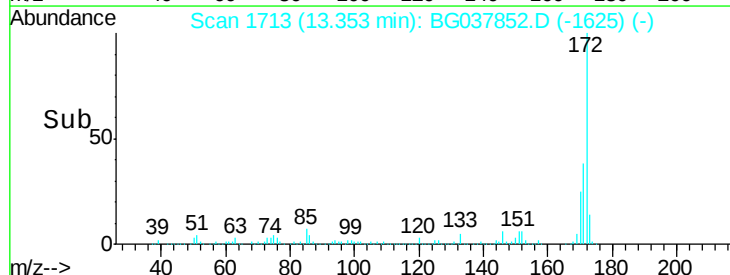
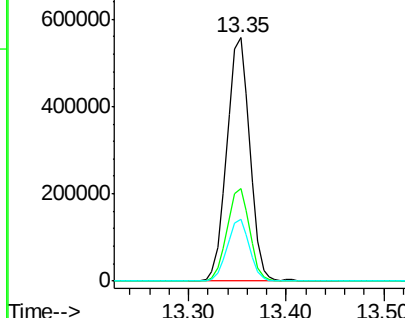


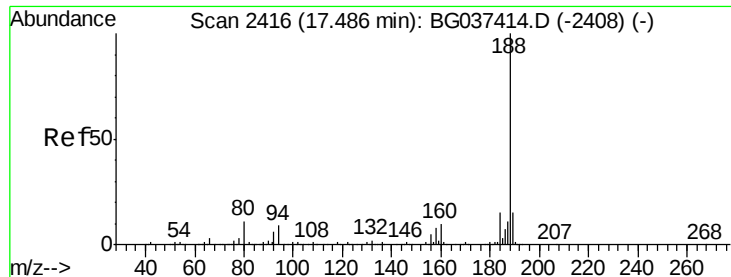

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.48 min Scan# 2415
Delta R.T. -0.01 min
Lab File: BG037852.D
Acq: 6 Nov 2018 23:56




Instrument :
BNA_G
ClientSampleId :
JC-03-110218-A


Tgt Ion:188 Resp: 352645
Ion Ratio Lower Upper
188 100
94 8.8 7.2 10.8
80 9.3 7.7 11.5

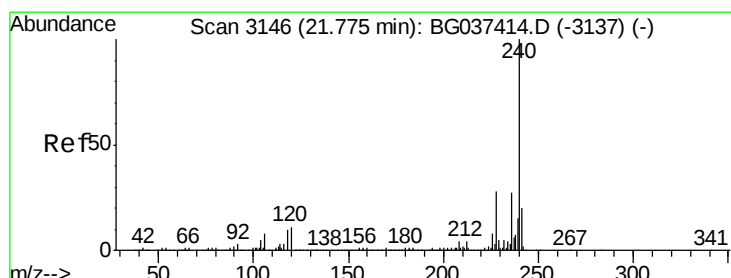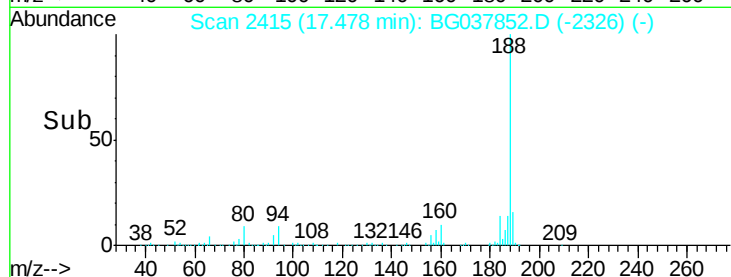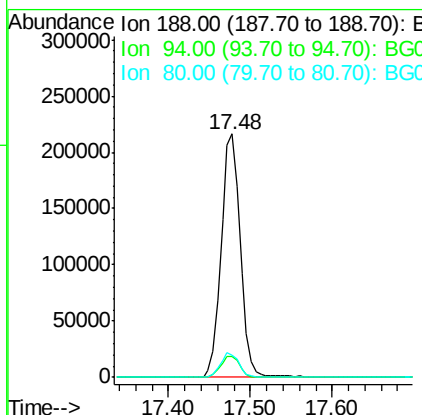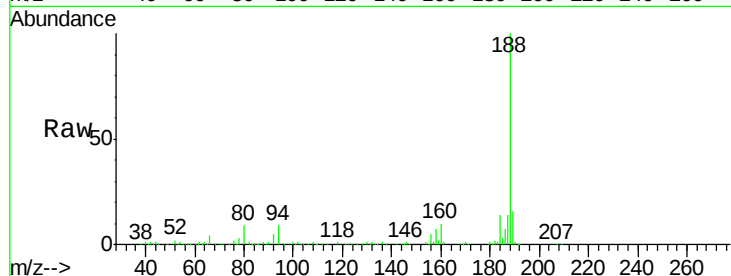

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3144
Delta R.T. -0.01 min
Lab File: BG037852.D
Acq: 6 Nov 2018 23:56

Tgt Ion:240 Resp: 309403
Ion Ratio Lower Upper
240 100
120 10.3 8.1 12.1
236 26.9 21.4 32.0

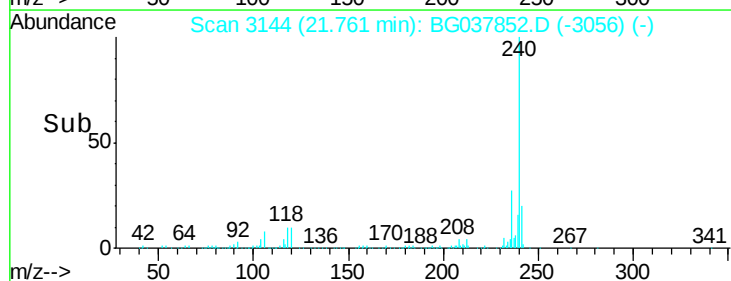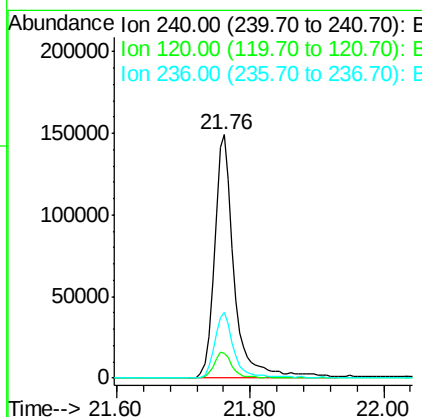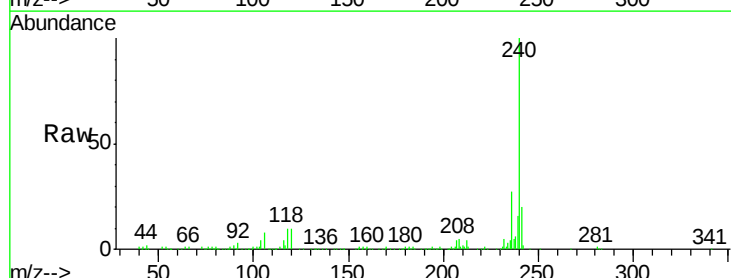

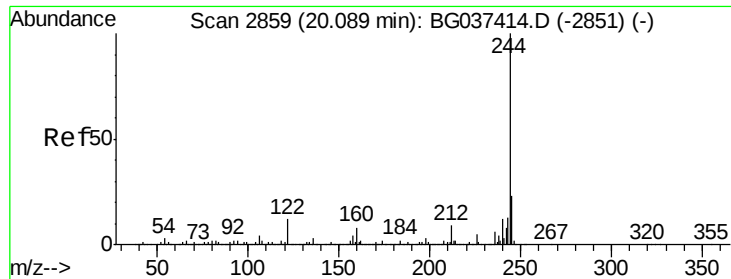

#79

Terphenyl-d14

Concen: 89.156 ng

RT: 20.07 min Scan# 2857

Delta R.T. -0.01 min

Lab File: BG037852.D

Acq: 6 Nov 2018 23:56

Instrument :

BNA_G

ClientSampleId :

JC-03-110218-A


Tgt Ion:244 Resp: 1290980

Ion Ratio Lower Upper

244 100

212 8.1 6.5 9.7




122 11.3 9.0 13.4

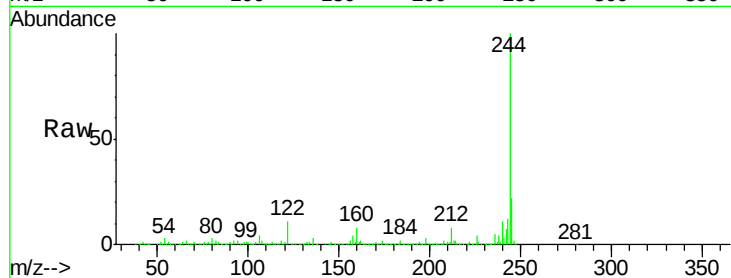

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

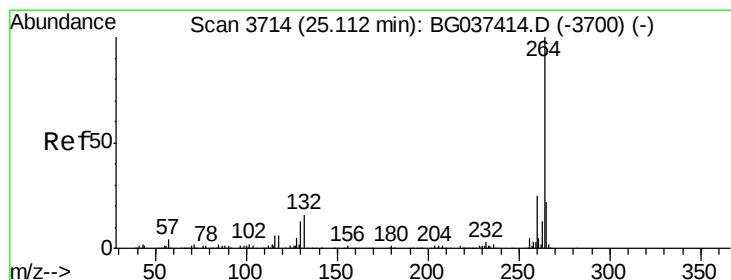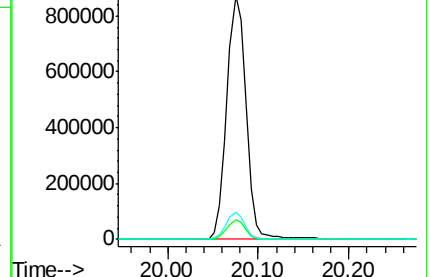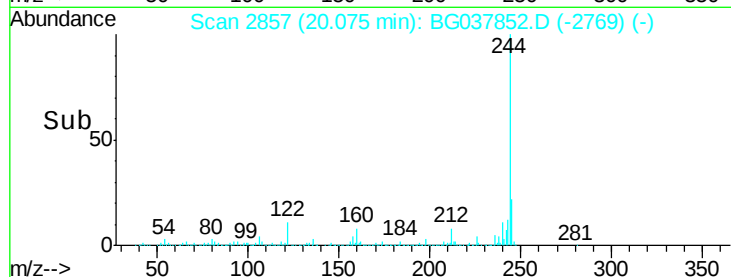

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3711

Delta R.T. -0.02 min

Lab File: BG037852.D

Acq: 6 Nov 2018 23:56


Tgt Ion:264 Resp: 226991

Ion Ratio Lower Upper

264 100

260 21.7 18.2 27.4

265 20.5 17.9 26.9

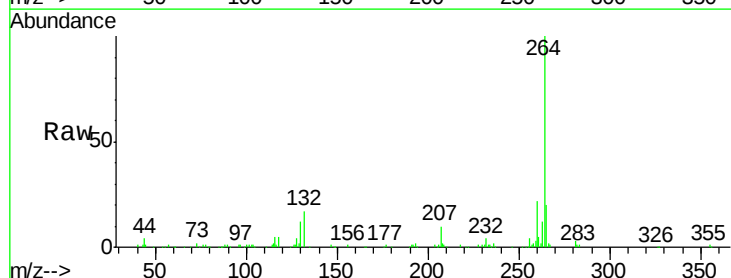

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

