


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110618\
 Data File : BG037838.D
 Acq On : 6 Nov 2018 14:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

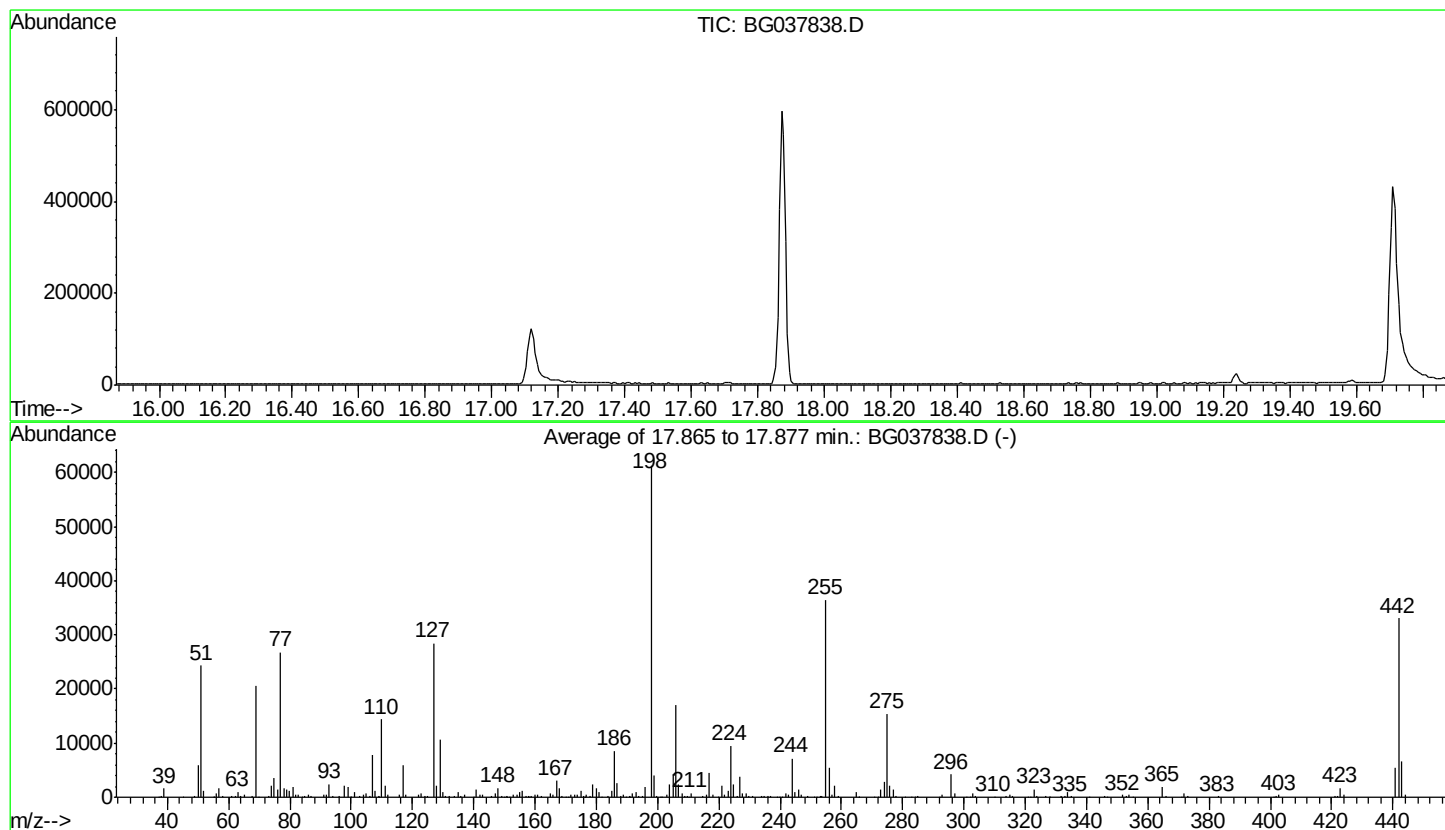

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	24242	PASS
68	69	0.00	2	1.4	280	PASS
69	198	0.00	100	33.5	20541	PASS
70	69	0.00	2	0.2	50	PASS
127	198	10	80	46.5	28464	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61242	PASS
199	198	5	9	6.6	4040	PASS
275	198	10	60	25.2	15431	PASS
365	198	1	100	3.1	1924	PASS
441	198	0.01	100	8.7	5341	PASS
442	198	50	100	54.0	33082	PASS
443	442	15	24	20.0	6600	PASS