
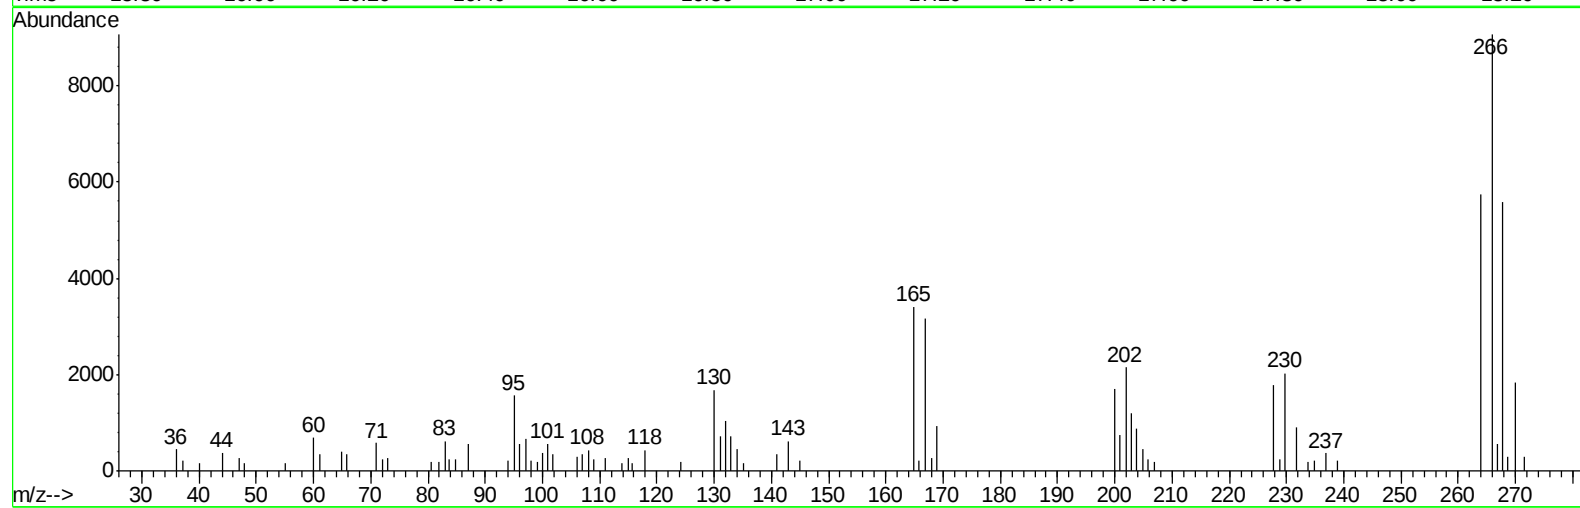


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110619\
Data File : BG043519.D
Acq On : 6 Nov 2019 13:40
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 03:40:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

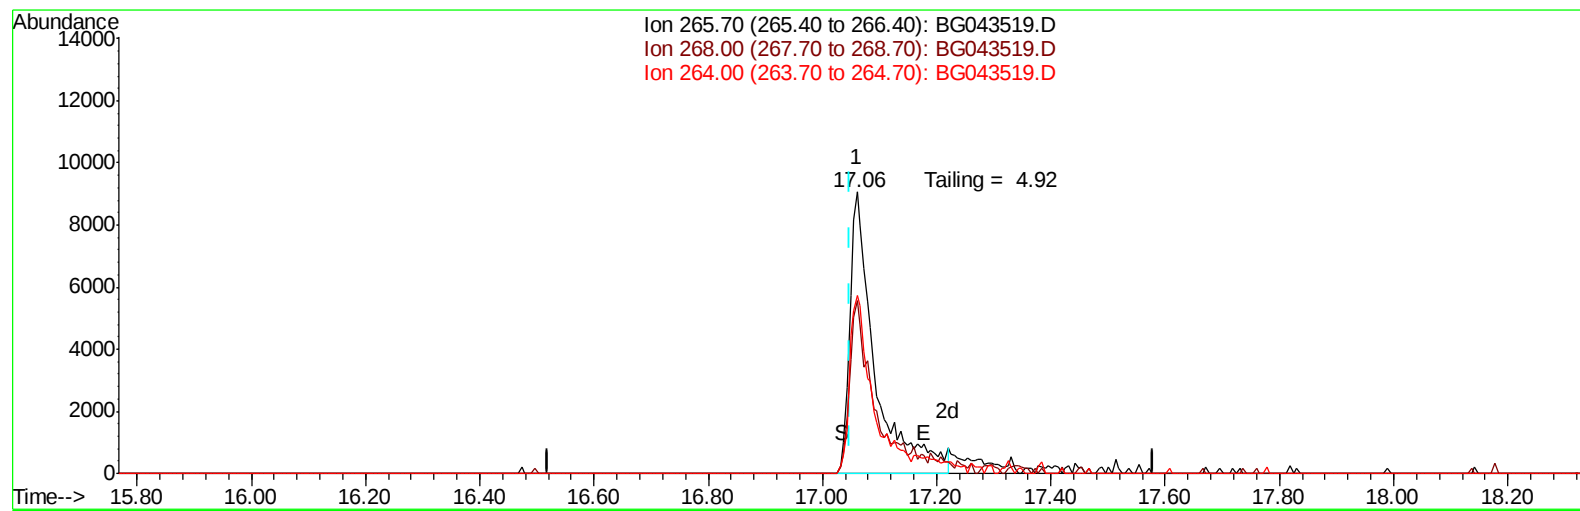

TIC: BG043519.D

(70) Pentachlorophenol (C)



17.061min (+0.011) 53923.52ng

response 25431

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	64.79
264.00	61.10	63.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110619\
Data File : BG043519.D
Acq On : 6 Nov 2019 13:40
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 03:40:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

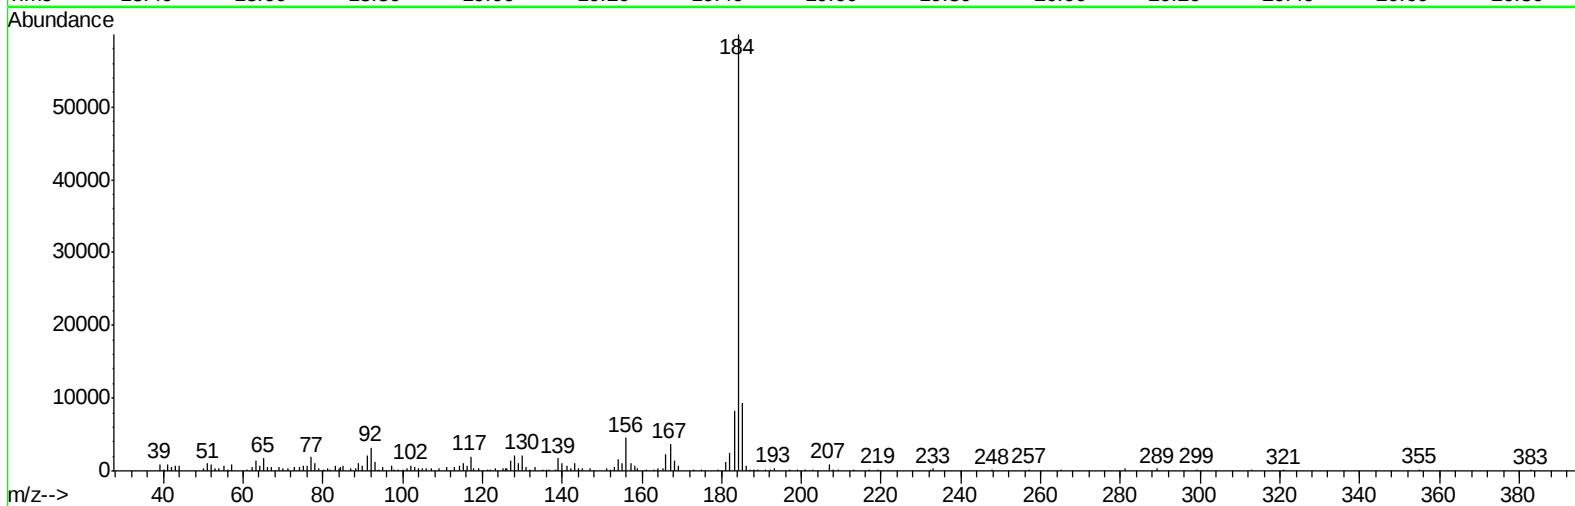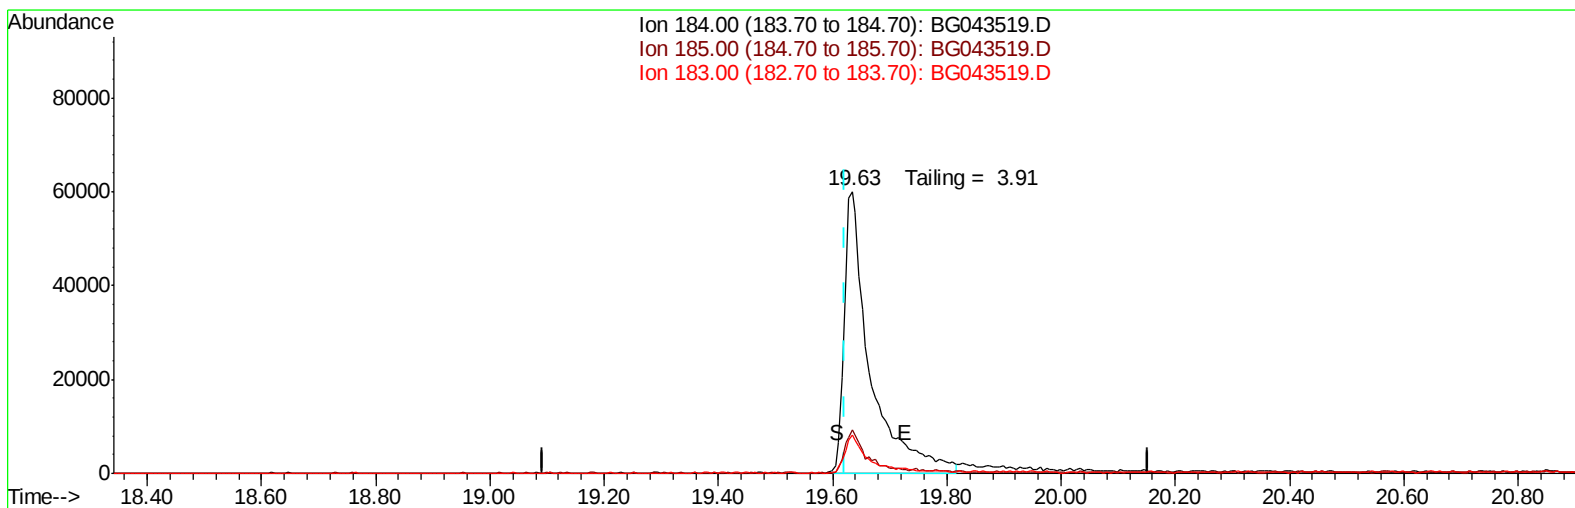

TIC: BG043519.D

(77) Benzidine

19.634min (+0.011) 24867.36ng

response 191177

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	15.48
183.00	12.50	13.72
0.00	0.00	0.00