


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110619\
Data File : BG043519.D
Acq On : 6 Nov 2019 13:40
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 04 15:22:15 2019

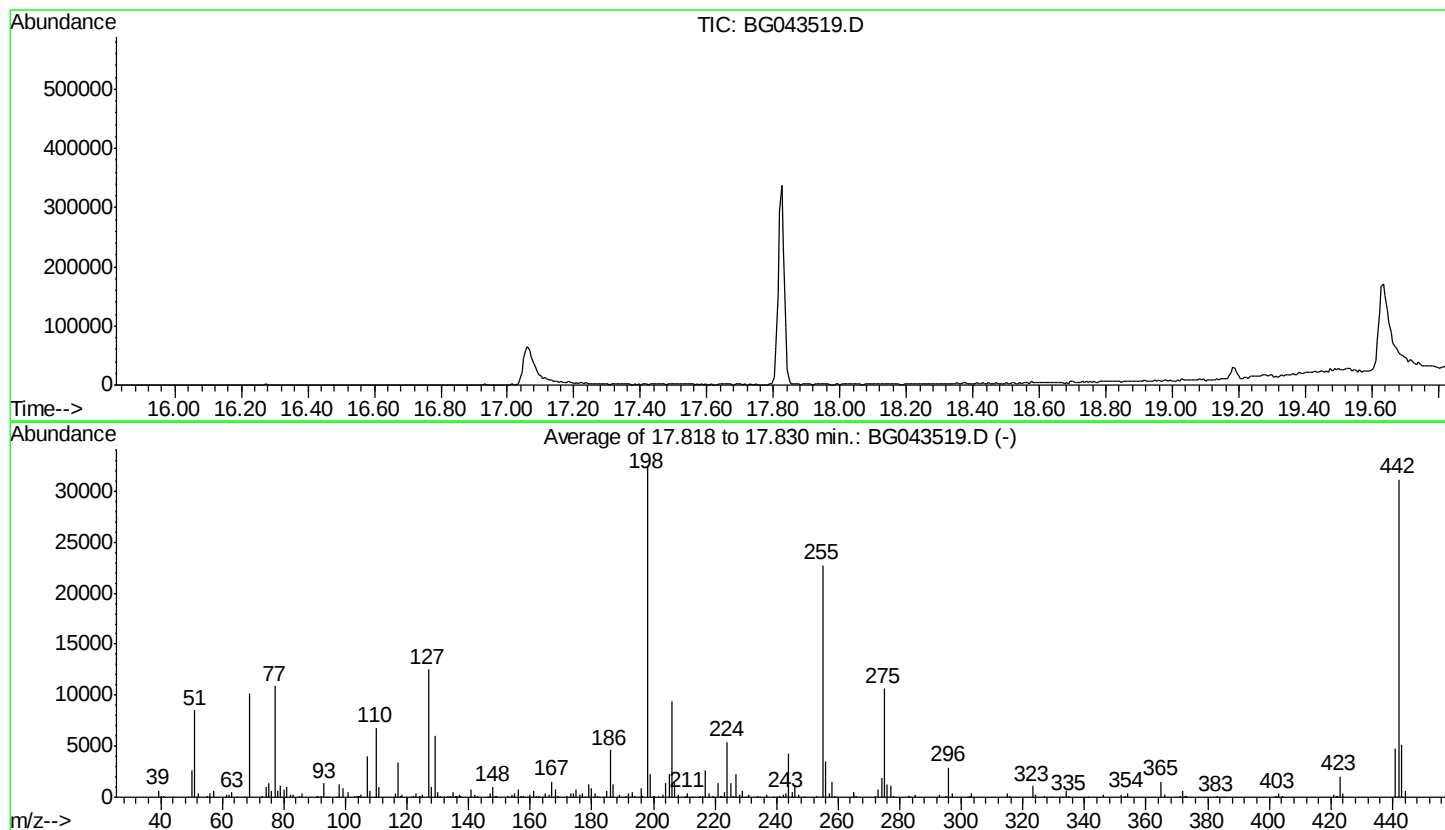

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	8481	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.1	10119	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.5	12513	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32493	PASS
199	198	5	9	7.0	2279	PASS
275	198	10	60	32.7	10629	PASS
365	198	1	100	4.8	1561	PASS
441	198	0.01	100	14.8	4822	PASS
442	198	50	100	95.8	31114	PASS
443	442	15	24	16.7	5199	PASS