
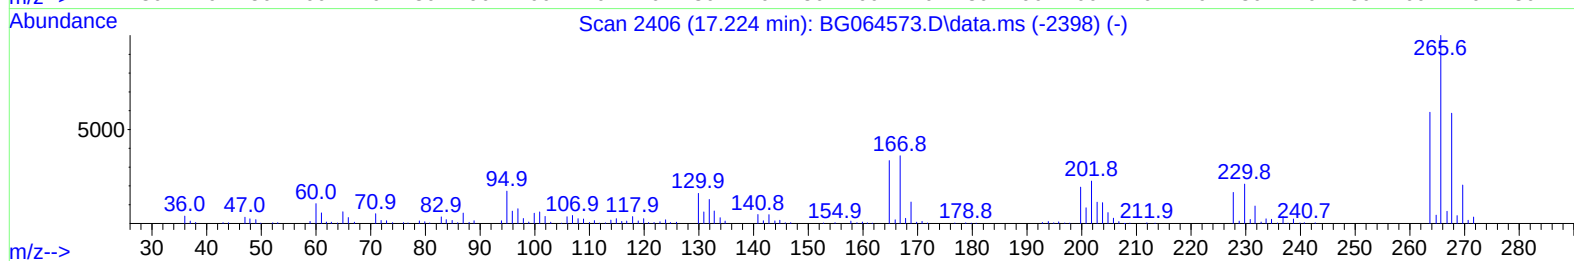
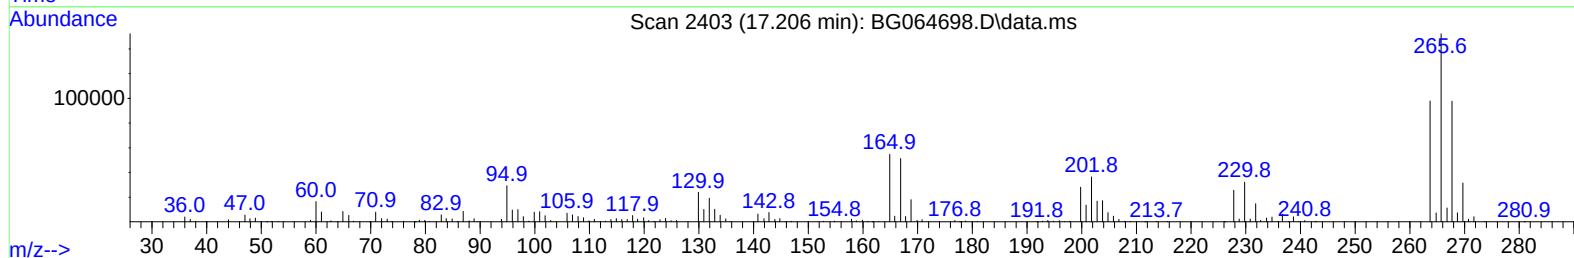


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110625\
Data File : BG064698.D
Acq On : 6 Nov 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 12:08:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

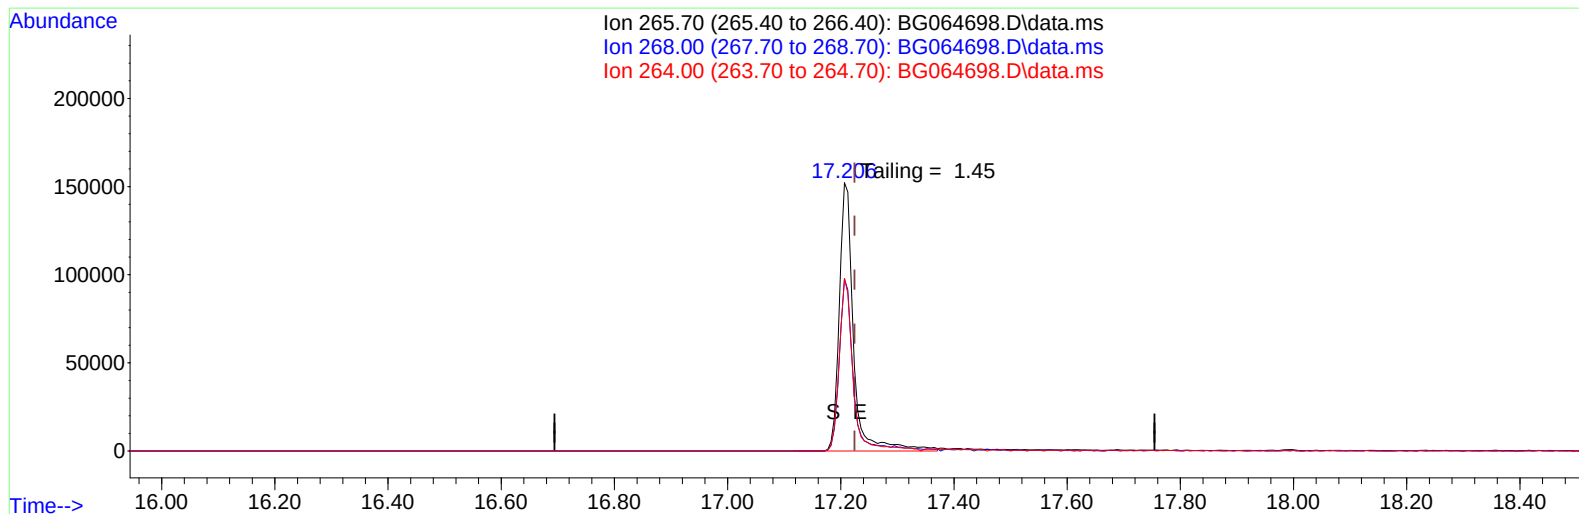

TIC: BG064698.D\data.ms

(70) Pentachlorophenol (C)




17.206min (-0.018) 138576.30 ng

response 268700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	69.06
264.00	59.10	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110625\
Data File : BG064698.D
Acq On : 6 Nov 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 12:08:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

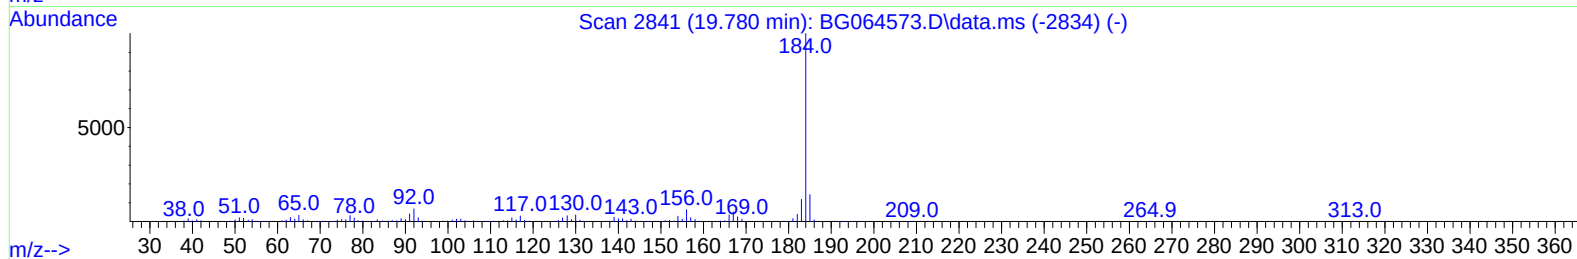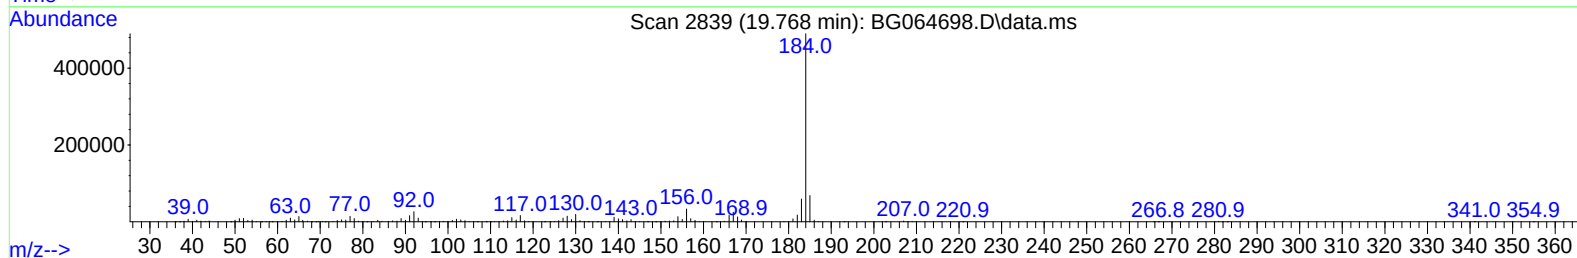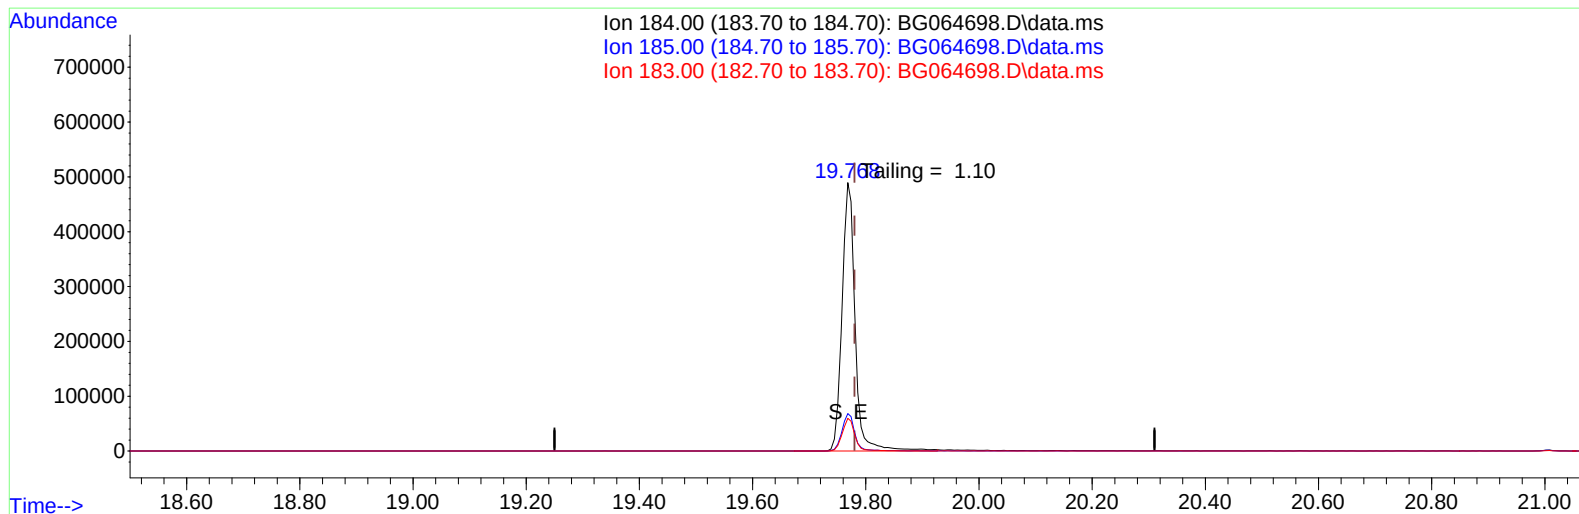

TIC: BG064698.D\data.ms

(77) Benzidine**19.768min (-0.012) 39040.29 ng****response 778451**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.96
183.00	11.80	12.16
0.00	0.00	0.00