
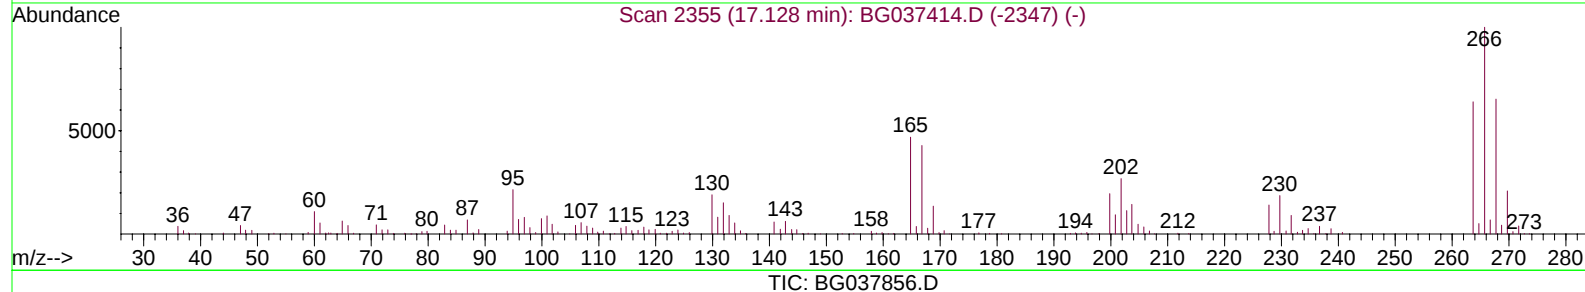
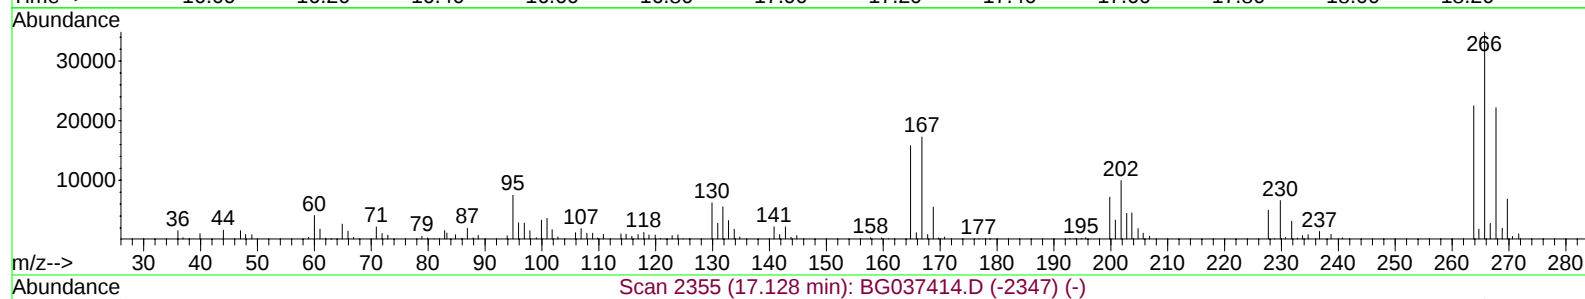


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110718\
Data File : BG037856.D
Acq On : 7 Nov 2018 8:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 15:49:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

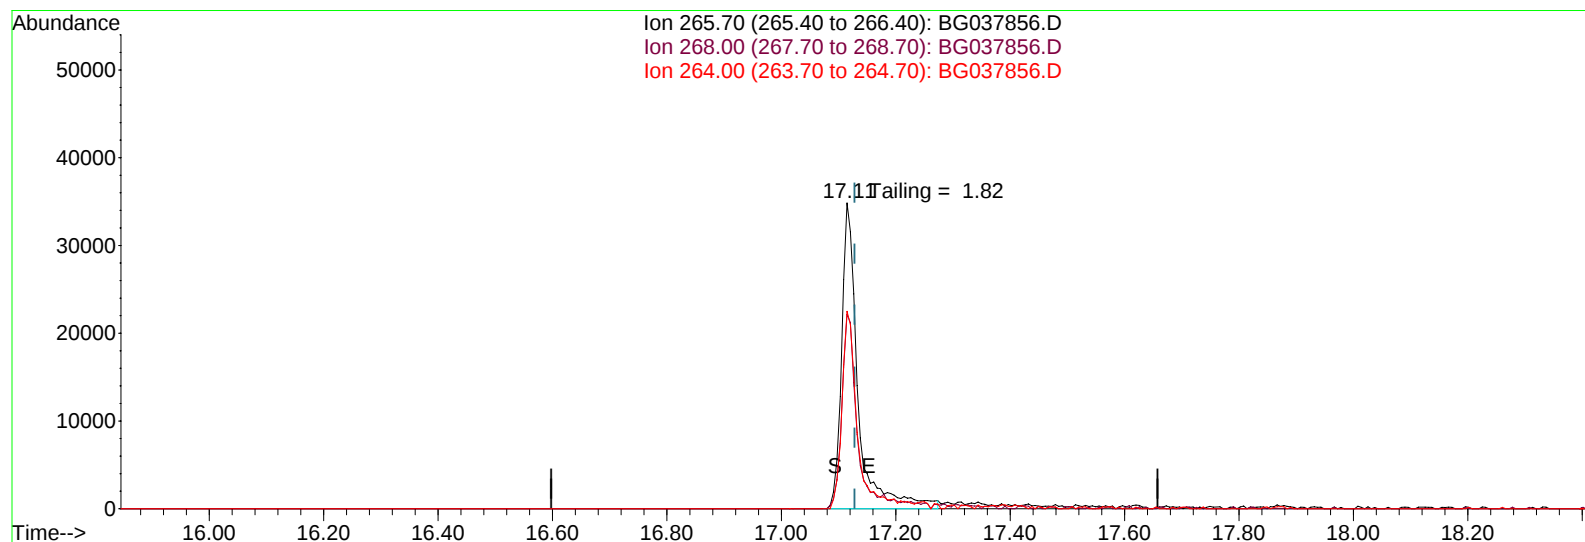

(70) Pentachlorophenol (C)




17.115min (-0.013) 19549.95ng

response 66324

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	63.63
264.00	73.60	69.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110718\
Data File : BG037856.D
Acq On : 7 Nov 2018 8:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 15:49:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

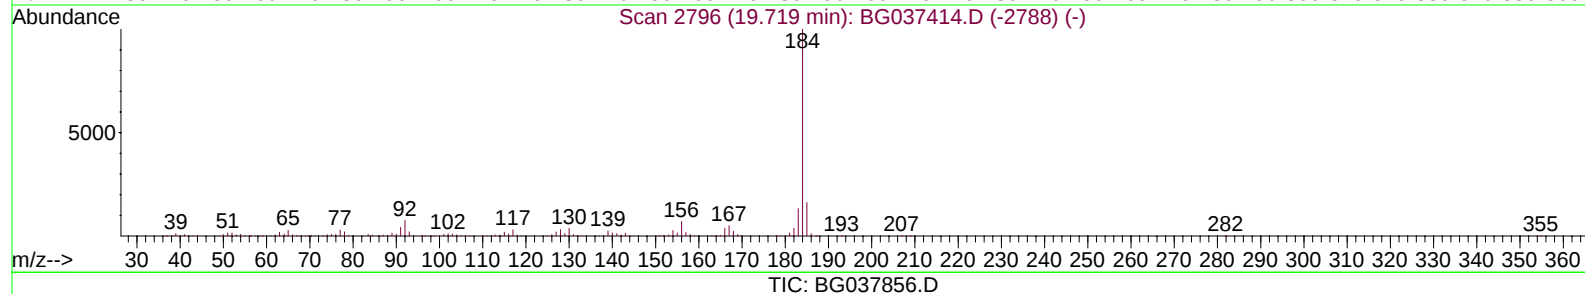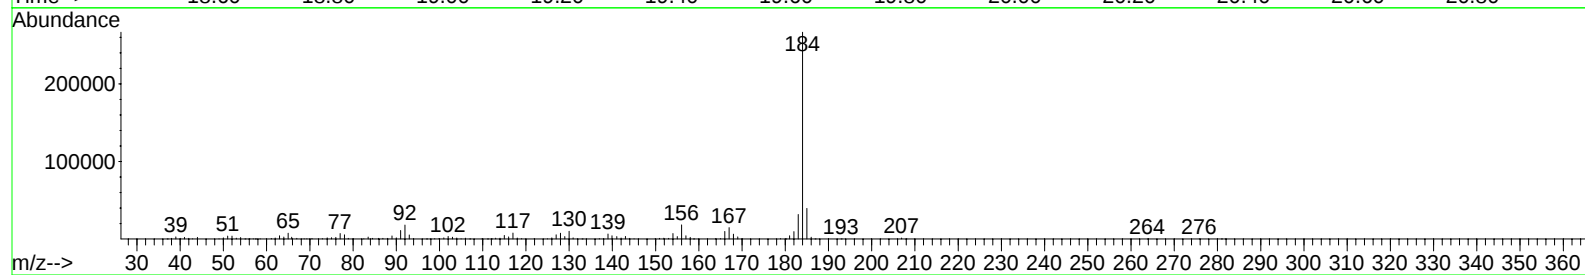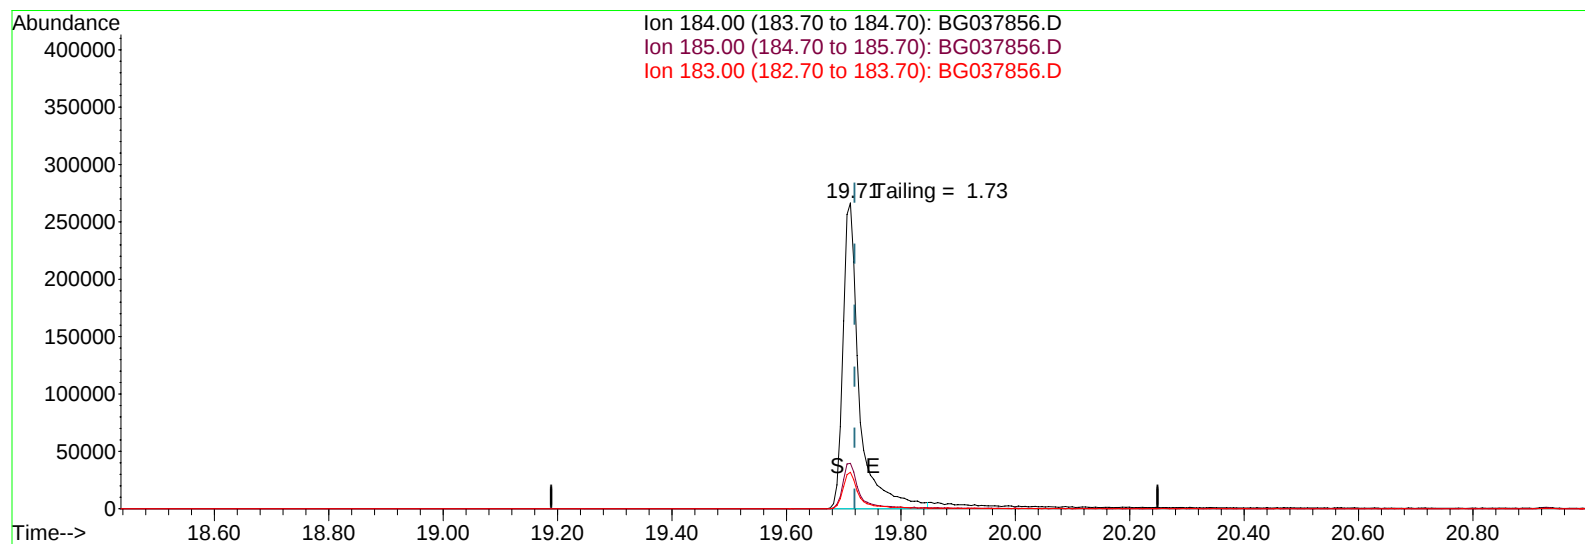

TIC: BG037856.D

(77) Benzidine

19.712min (-0.007) 237536.66ng

response 533073

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.85
183.00	12.70	11.92
0.00	0.00	0.00