

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110718\
Data File : BG037869.D
Acq On : 7 Nov 2018 17:25
Operator : JU/SJ
Sample : J5822-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.637	393	400	409	rBV	425656	725758	17.81%	3.735%
2	7.236	664	672	681	rBV	286219	511880	12.56%	2.634%
3	7.617	730	737	749	rBV	818818	1484745	36.44%	7.642%
4	8.093	811	818	829	rBV	222776	388826	9.54%	2.001%
5	8.417	863	873	883	rBV	770819	1389015	34.09%	7.149%
6	9.274	1010	1019	1030	rBV	663888	1249385	30.66%	6.430%
7	10.914	1290	1298	1308	rVB	320608	600441	14.74%	3.090%
8	13.352	1705	1713	1727	rBV	1868929	3067698	75.29%	15.788%
9	14.727	1940	1947	1957	rBV2	530488	890858	21.86%	4.585%
10	16.213	2193	2200	2219	rBV	1279858	2050031	50.31%	10.551%
11	17.476	2407	2415	2425	rBV2	643175	1031715	25.32%	5.310%
12	20.073	2851	2857	2874	rBV	2911825	4074453	100.00%	20.970%
13	21.754	3136	3143	3158	rBV	532084	1055881	25.91%	5.434%
14	25.091	3696	3711	3738	rBV3	224115	909282	22.32%	4.680%


Sum of corrected areas: 19429968

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110718\
Data File : BG037869.D
Acq On : 7 Nov 2018 17:25
Operator : JU/SJ
Sample : J5822-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

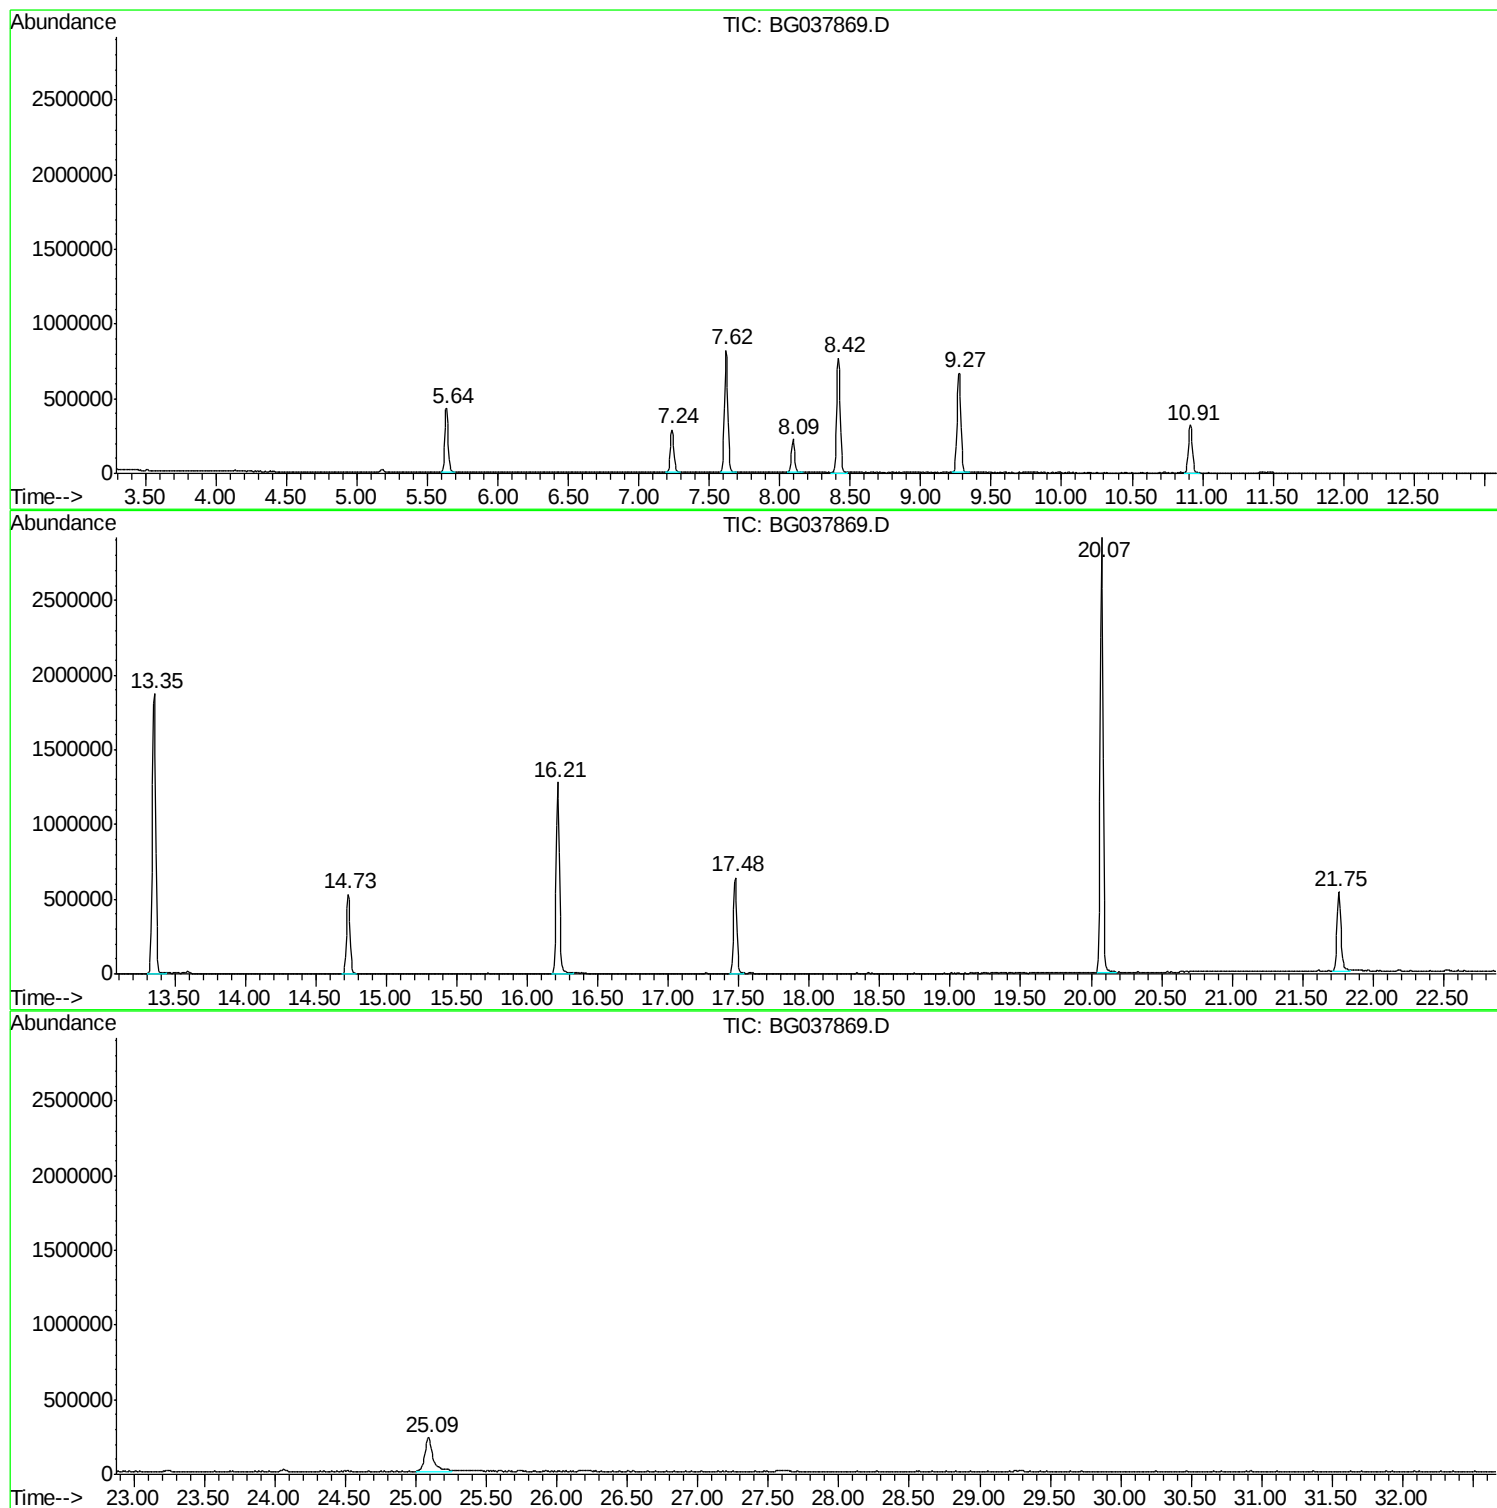

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110718\
Data File : BG037869.D
Acq On : 7 Nov 2018 17:25
Operator : JU/SJ
Sample : J5822-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-01










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.62	76.37 ng	1484750	1,4-Dichlorobenzene-d4	8.09

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

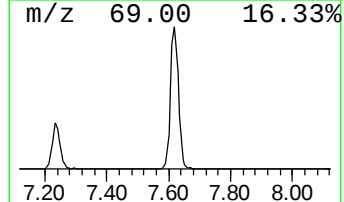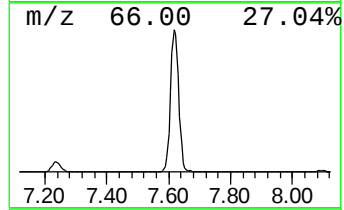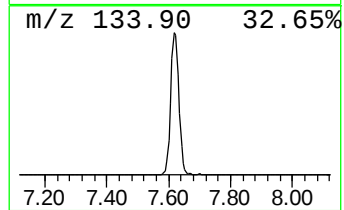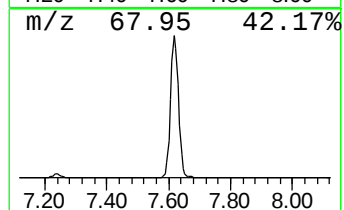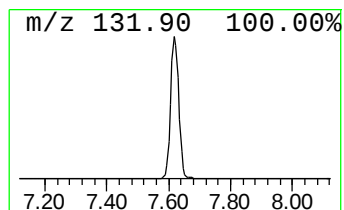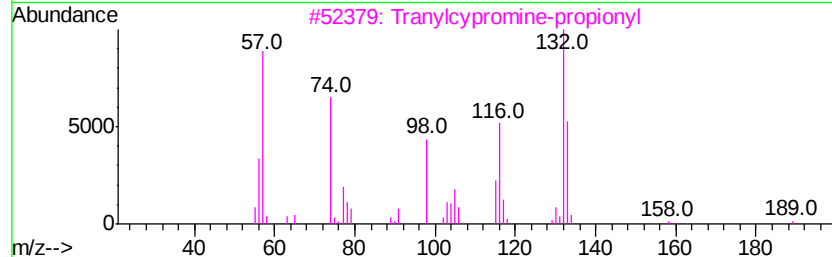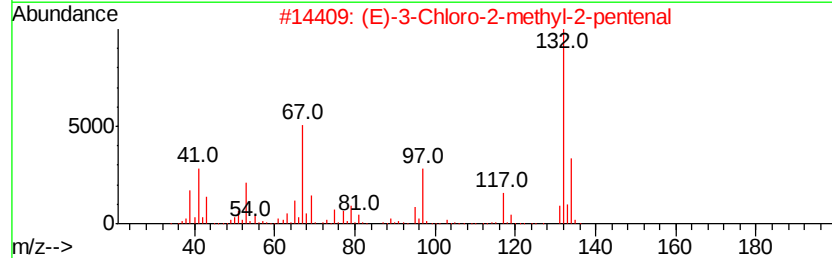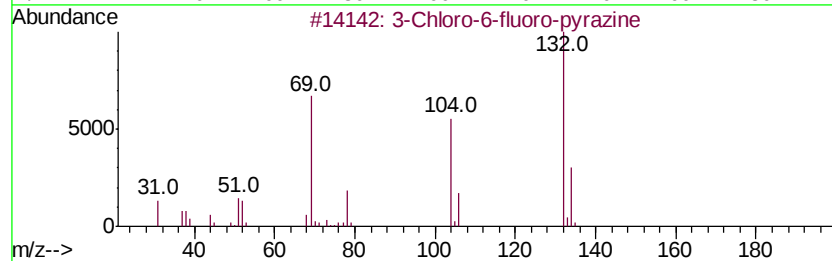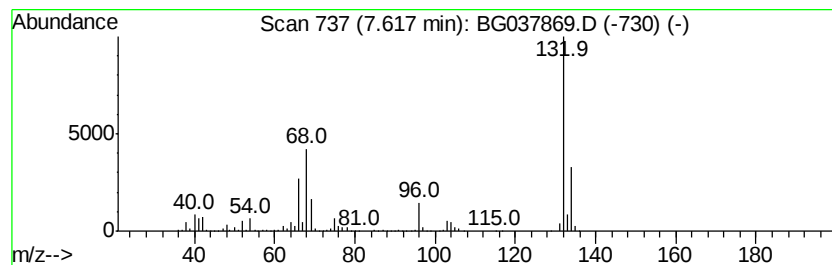

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110718\
Data File : BG037869.D
Acq On : 7 Nov 2018 17:25
Operator : JU/SJ
Sample : J5822-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.62	7.62	76.4	ng	1484750	1	8.09	388826	20.0