


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110718\
 Data File : BG037856.D
 Acq On : 7 Nov 2018 8:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

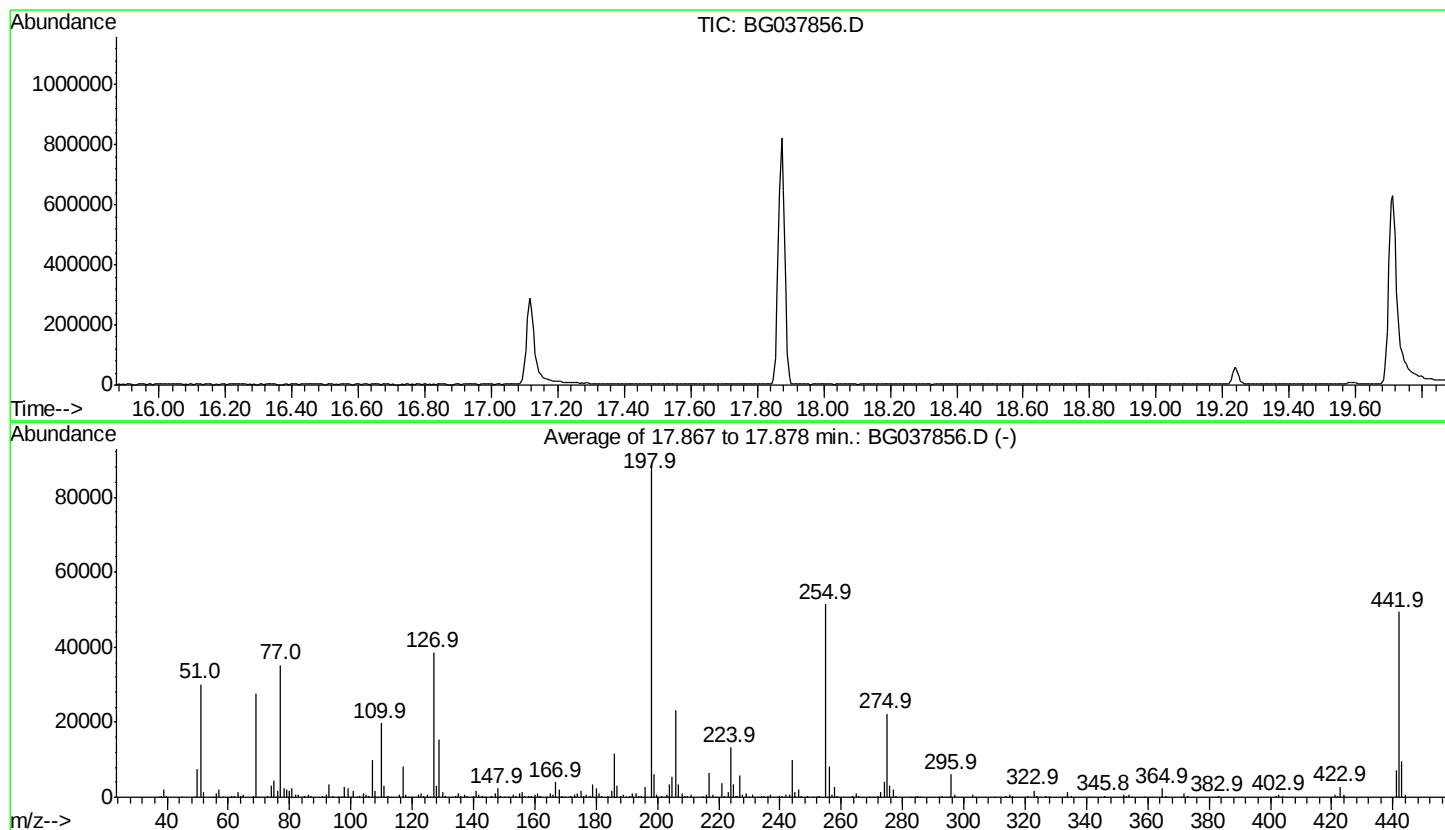

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	30160	PASS
68	69	0.00	2	0.7	198	PASS
69	198	0.00	100	31.4	27722	PASS
70	69	0.00	2	0.2	59	PASS
127	198	10	80	43.6	38490	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88378	PASS
199	198	5	9	6.9	6111	PASS
275	198	10	60	25.1	22221	PASS
365	198	1	100	2.7	2382	PASS
441	198	0.01	100	8.1	7144	PASS
442	198	50	100	55.8	49357	PASS
443	442	15	24	19.6	9651	PASS