


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110718\
 Data File : BG037873.D
 Acq On : 7 Nov 2018 20:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

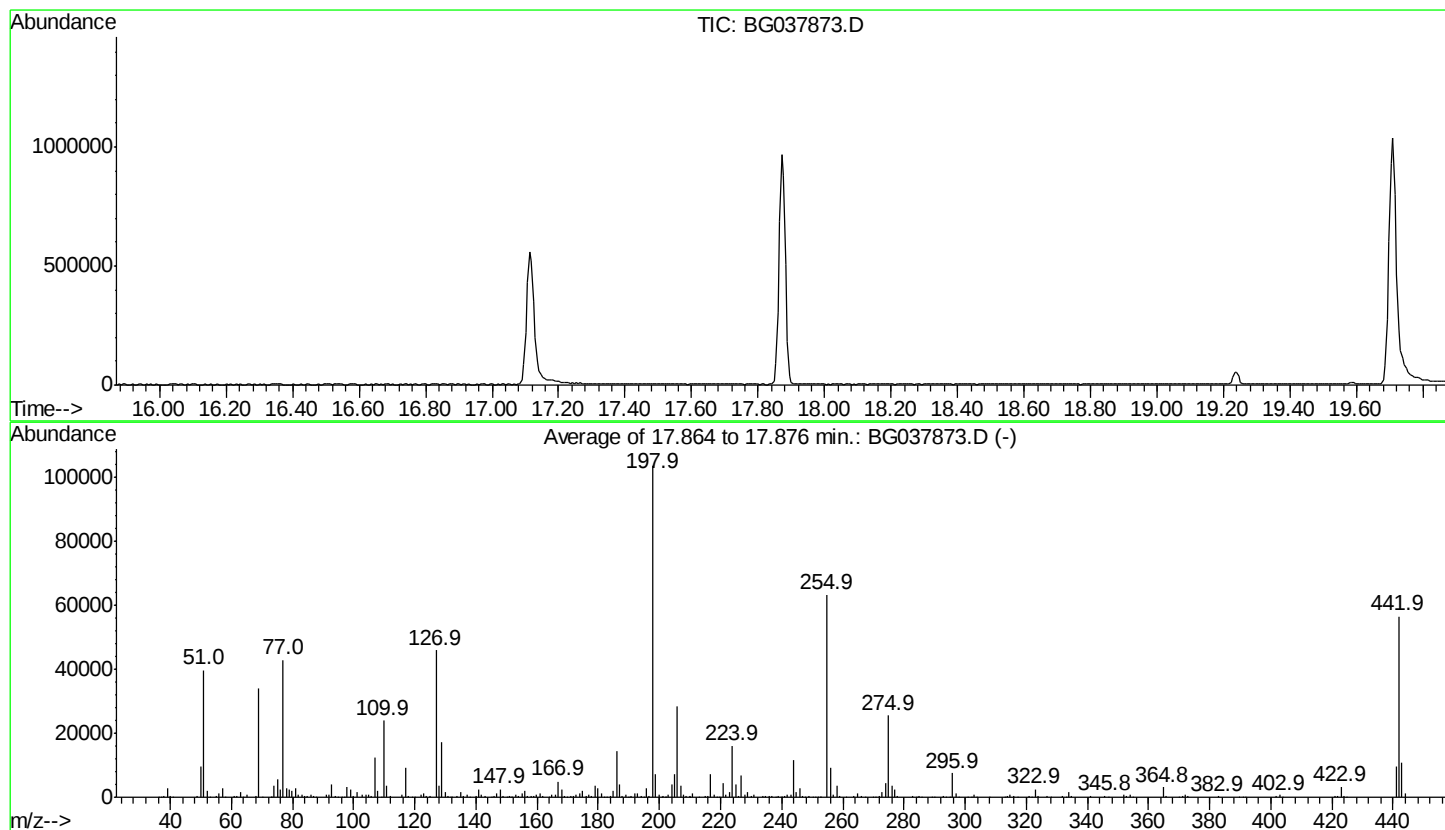

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	39656	PASS
68	69	0.00	2	1.6	540	PASS
69	198	0.00	100	32.7	33904	PASS
70	69	0.00	2	0.5	172	PASS
127	198	10	80	44.4	45984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103632	PASS
199	198	5	9	6.9	7120	PASS
275	198	10	60	24.7	25602	PASS
365	198	1	100	2.9	3052	PASS
441	198	0.01	100	9.1	9445	PASS
442	198	50	100	54.5	56466	PASS
443	442	15	24	19.0	10735	PASS