


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110719\
 Data File : BG043537.D
 Acq On : 7 Nov 2019 13:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

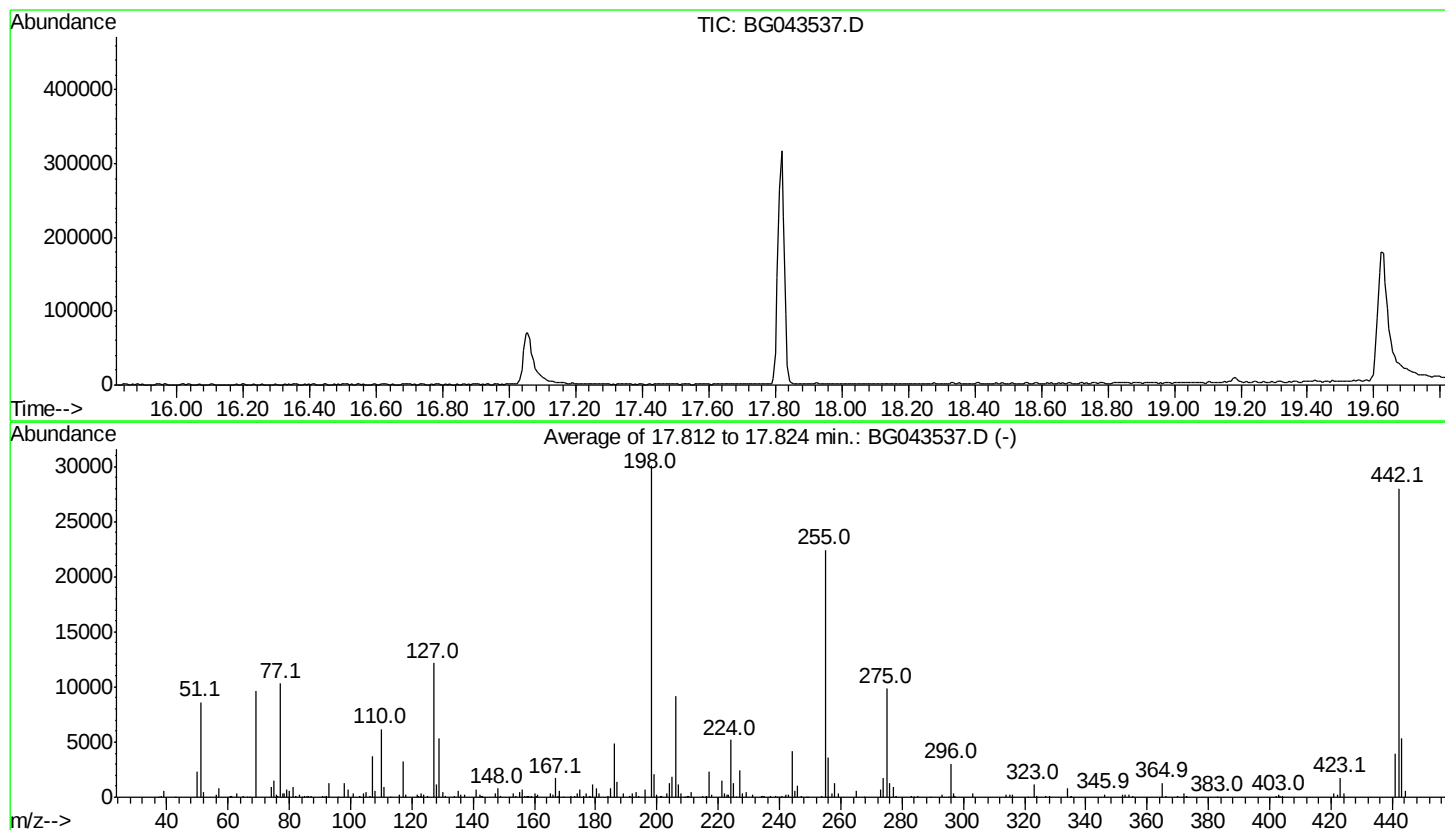

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	8603	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.9	9586	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.5	12185	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30069	PASS
199	198	5	9	6.8	2037	PASS
275	198	10	60	32.6	9812	PASS
365	198	1	100	4.4	1310	PASS
441	198	0.01	100	13.0	3915	PASS
442	198	50	100	93.2	28021	PASS
443	442	15	24	19.0	5317	PASS