


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110719\
 Data File : BG043555.D
 Acq On : 8 Nov 2019 1:57
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

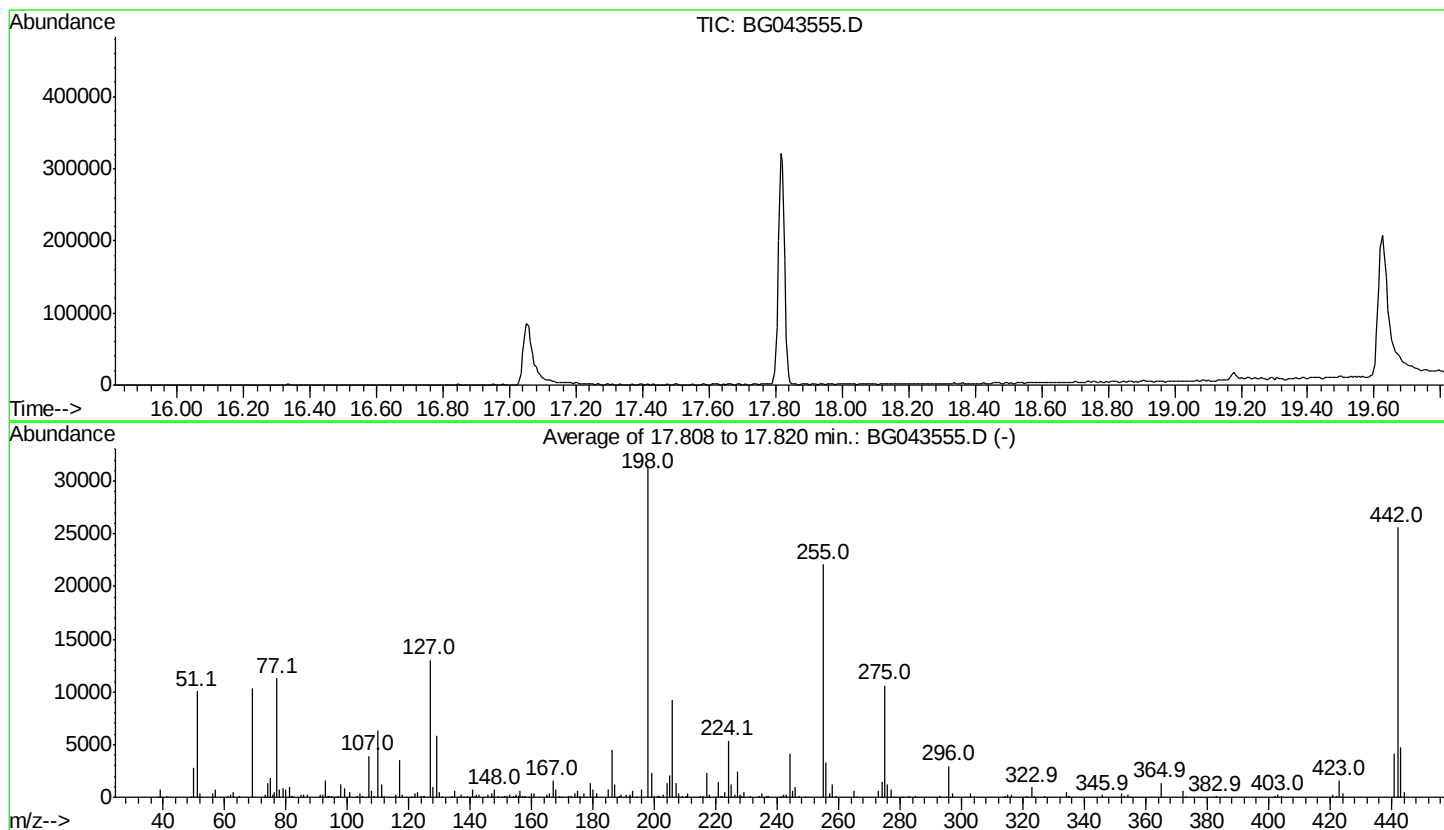

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	10056	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	10286	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.3	13002	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31477	PASS
199	198	5	9	7.5	2355	PASS
275	198	10	60	33.6	10578	PASS
365	198	1	100	4.3	1341	PASS
441	198	0.01	100	13.0	4106	PASS
442	198	50	100	81.4	25613	PASS
443	442	15	24	18.3	4684	PASS