
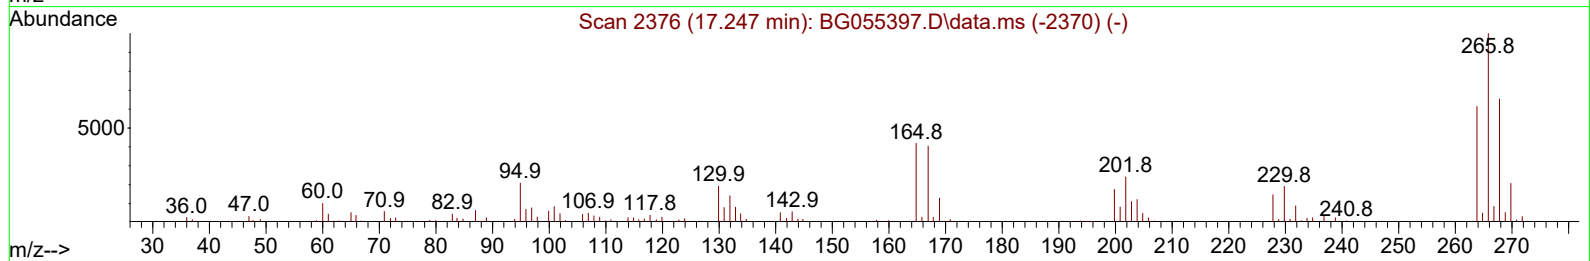
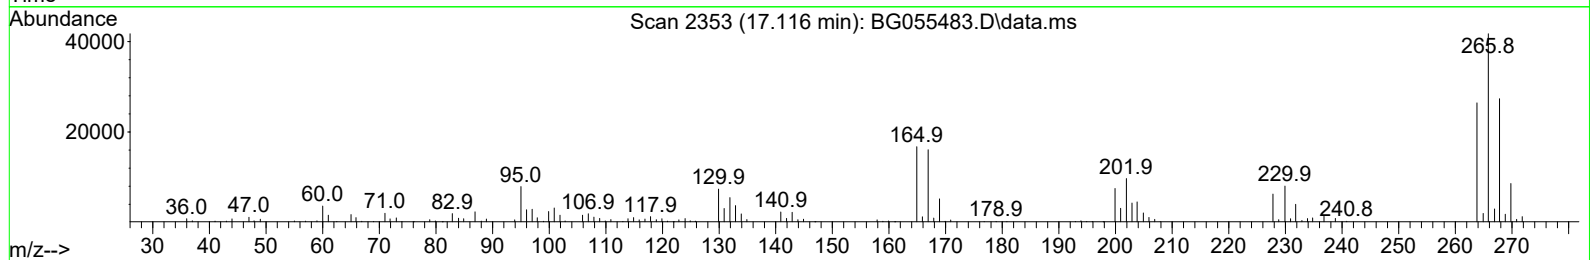


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110722\
Data File : BG055483.D
Acq On : 7 Nov 2022 18:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 04:46:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 03:46:08 2022
Response via : Initial Calibration

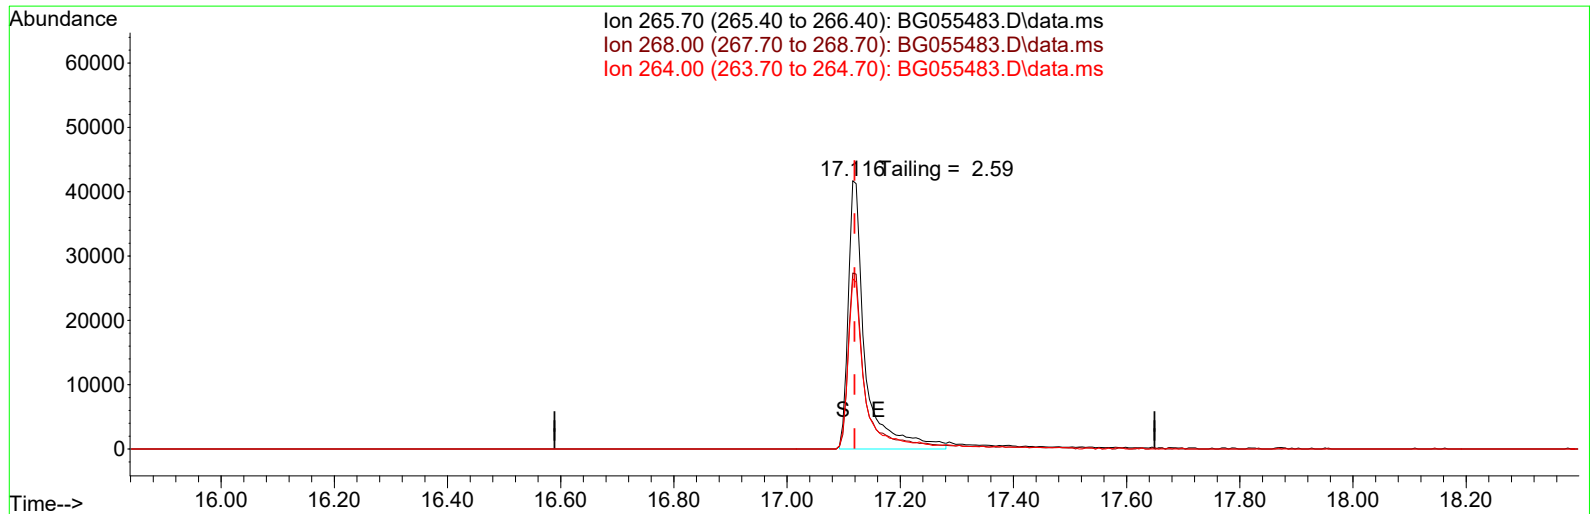

TIC: BG055483.D\data.ms

(70) Pentachlorophenol (C)




17.116min (-0.003) 38000.36 ng

response 87144

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.60
264.00	61.50	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110722\
Data File : BG055483.D
Acq On : 7 Nov 2022 18:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 04:46:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 03:46:08 2022
Response via : Initial Calibration

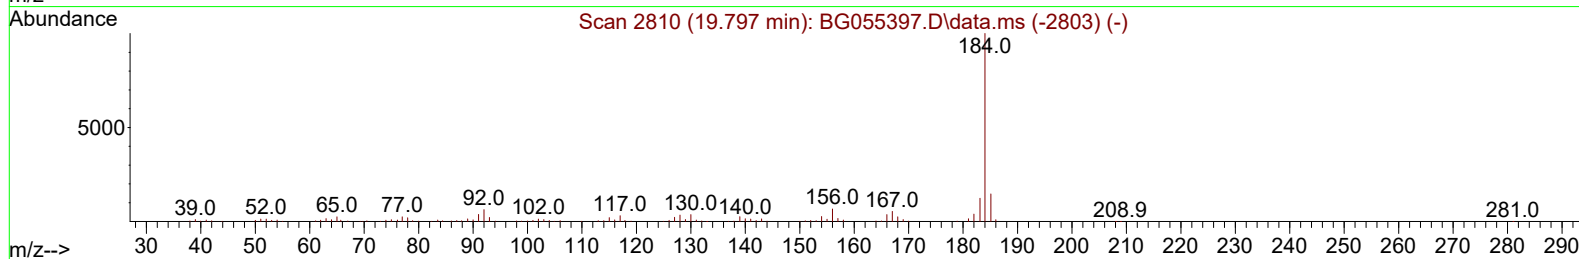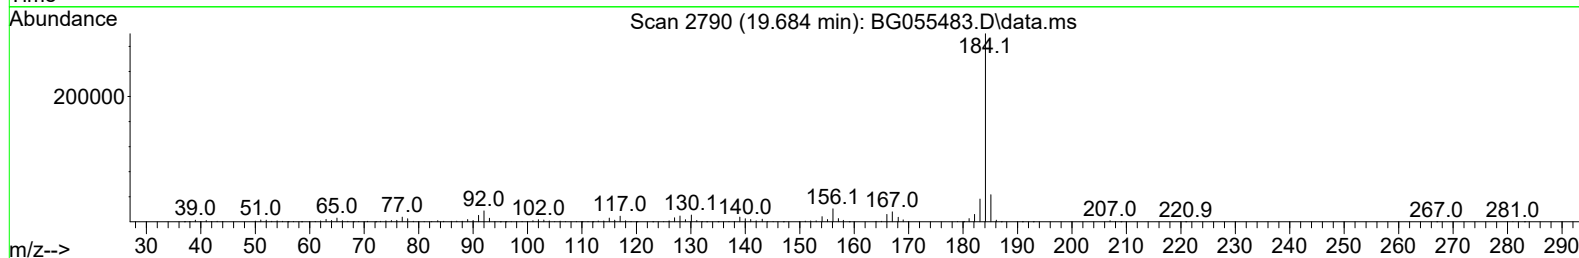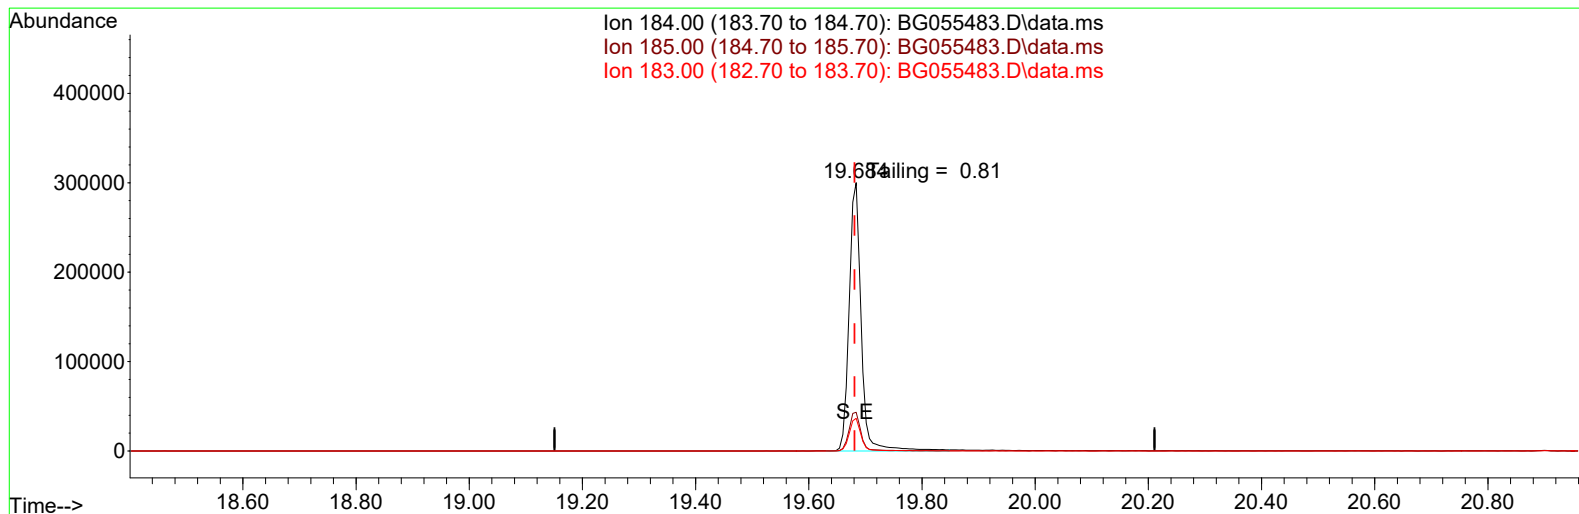

TIC: BG055483.D\data.ms

(77) Benzidine**19.684min (+ 0.003) 355825.06 ng****response 444482**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.42
183.00	12.30	12.15
0.00	0.00	0.00