
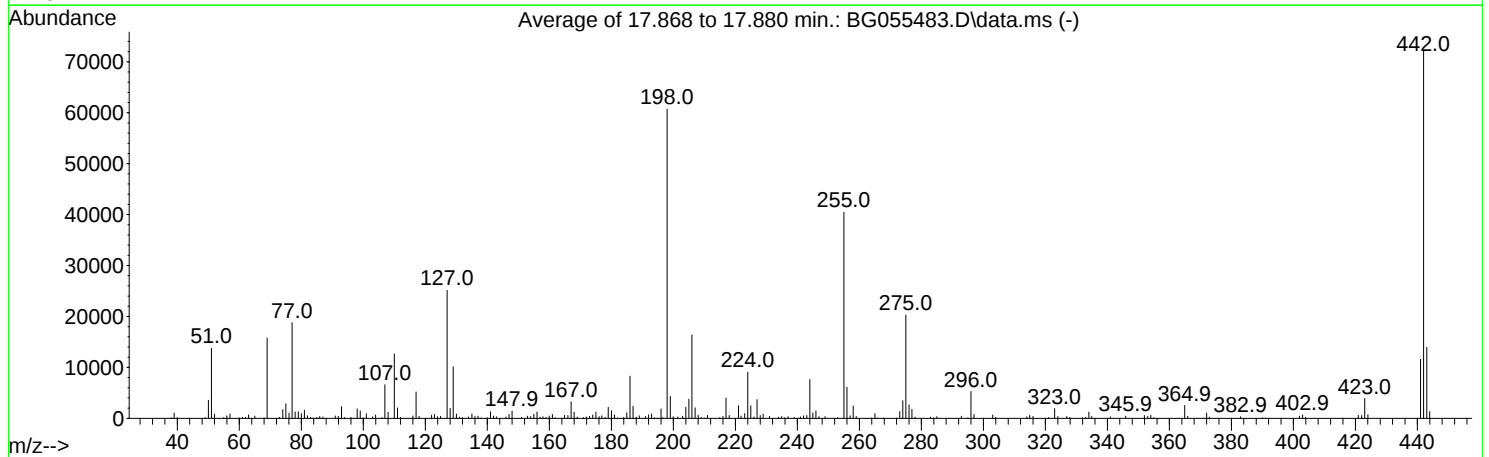


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110722\
Data File : BG055483.D
Acq On : 7 Nov 2022 18:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 08 03:46:08 2022

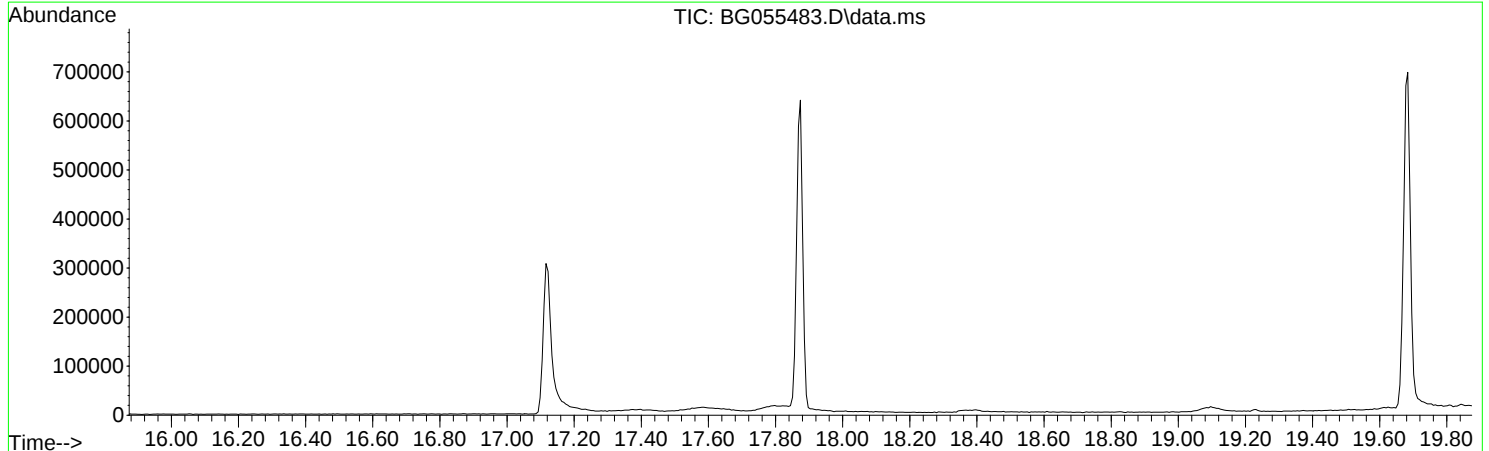




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	13761	PASS
68	69	0.00	2	0.6	89	PASS
69	198	0.00	100	26.0	15763	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.5	25152	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60677	PASS
199	198	5	9	7.1	4282	PASS
275	198	10	60	33.4	20288	PASS
365	198	1	100	4.2	2529	PASS
441	198	0.01	100	19.1	11591	PASS
442	442	50	100	100.0	72237	PASS
443	442	15	24	19.3	13937	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110722\
Data File : BG055483.D
Acq On : 7 Nov 2022 18:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 08 04:46:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 03:46:08 2022
Response via : Initial Calibration

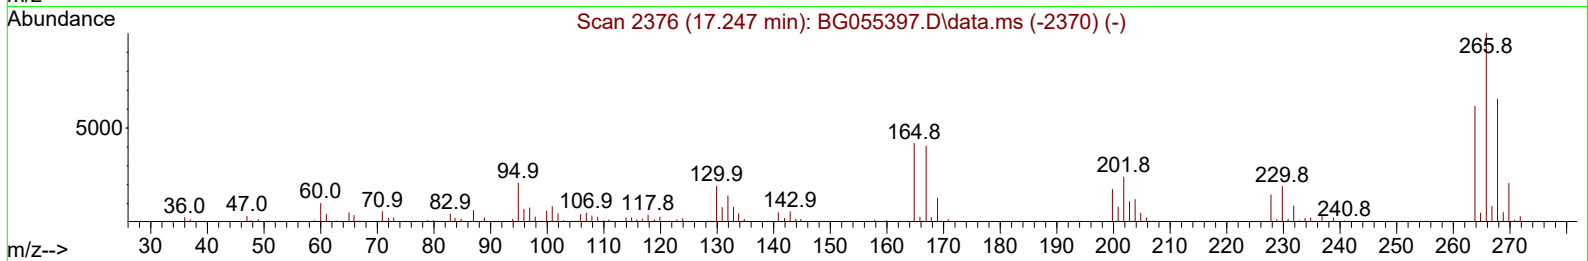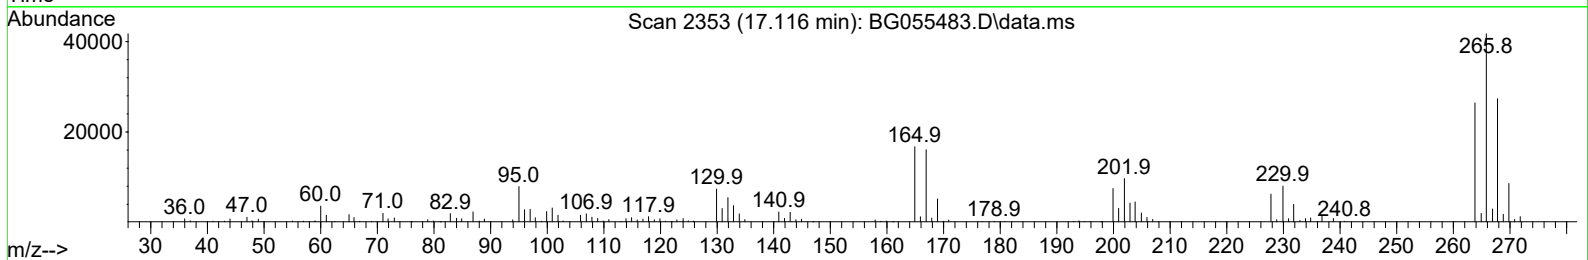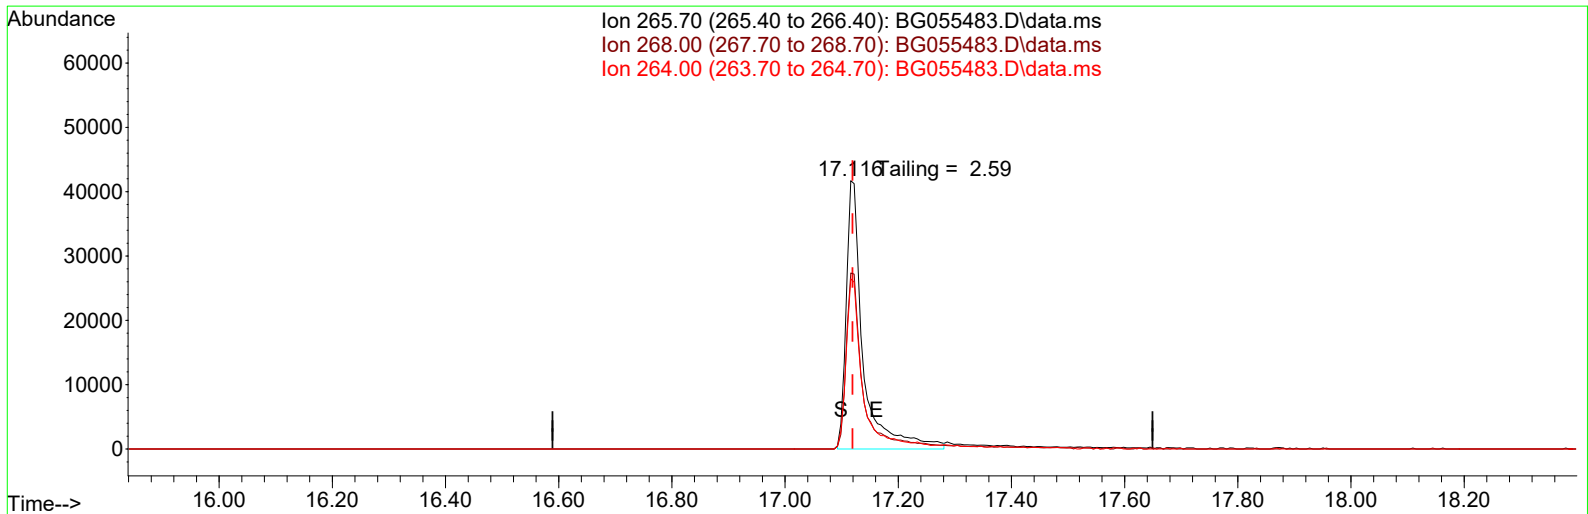

TIC: BG055483.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.003) 38000.36 ng




response 87144

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.60
264.00	61.50	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110722\
Data File : BG055483.D
Acq On : 7 Nov 2022 18:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 08 04:46:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 03:46:08 2022
Response via : Initial Calibration

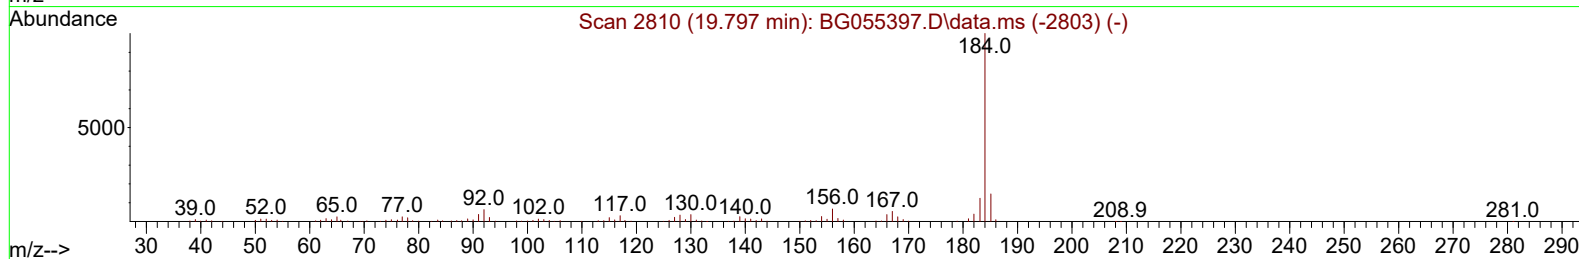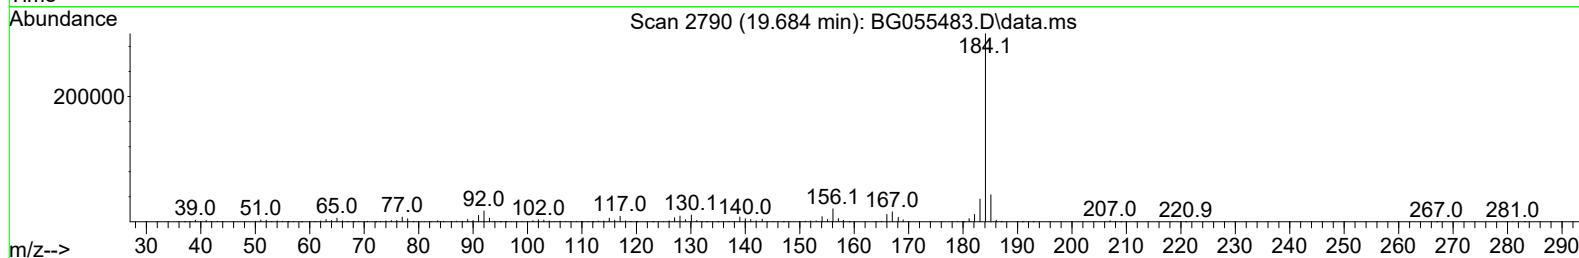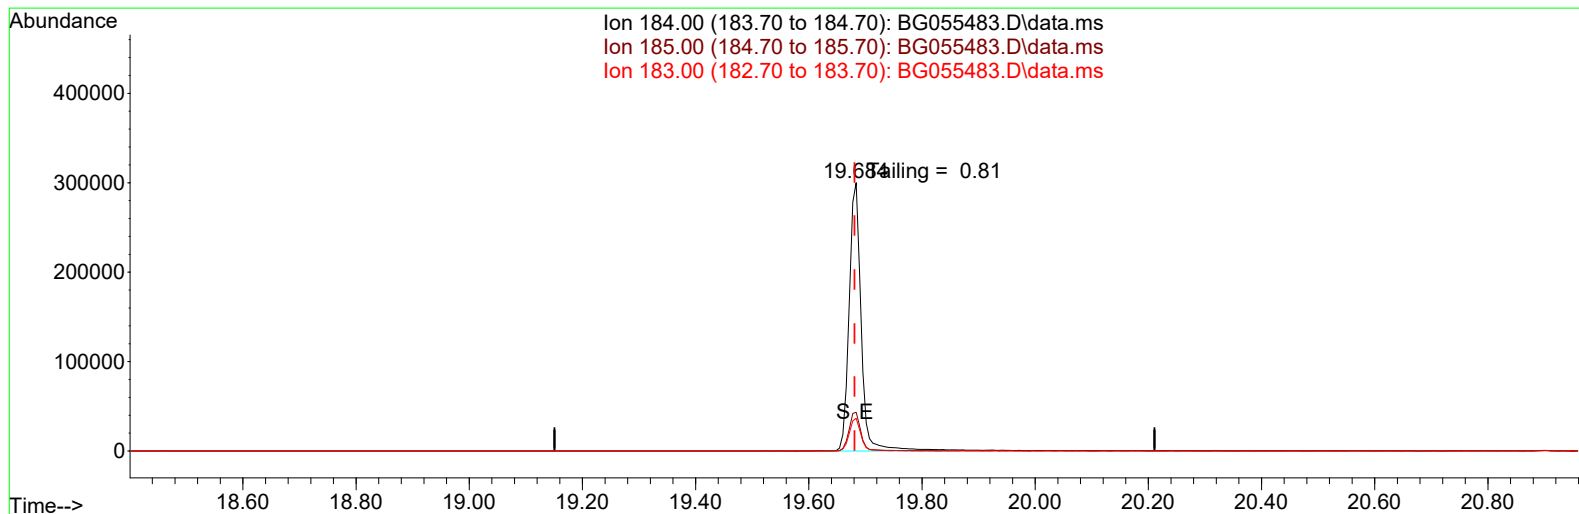

TIC: BG055483.D\data.ms

(77) Benzidine

19.684min (+ 0.003) 355825.06 ng

response 444482

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.42
183.00	12.30	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2022	BNA_G	BG055483.D
Compound Name	Response	Retention Time
DDT	200514	20.9
DDD	3562	20.512
DDE	0	19.936
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3562	204076	1.75

Instrument :
BNA_G
ClientSampleId :
DFTPP