
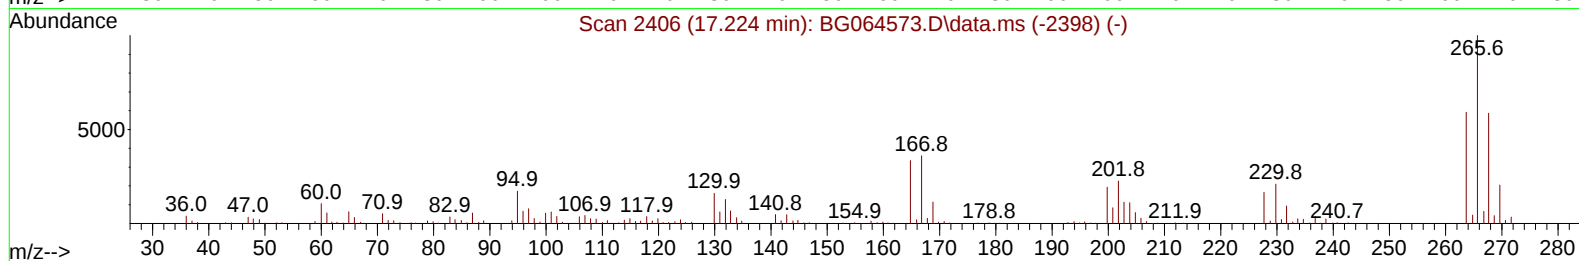
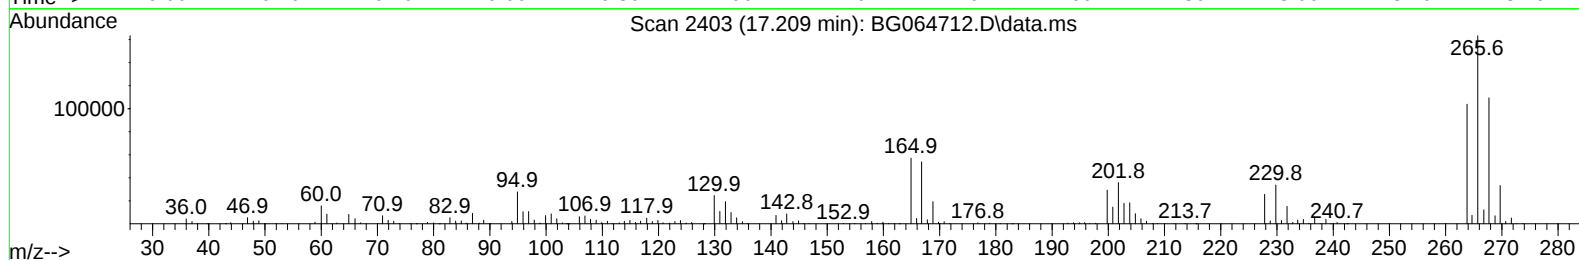


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110725\
Data File : BG064712.D
Acq On : 7 Nov 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 11:06:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

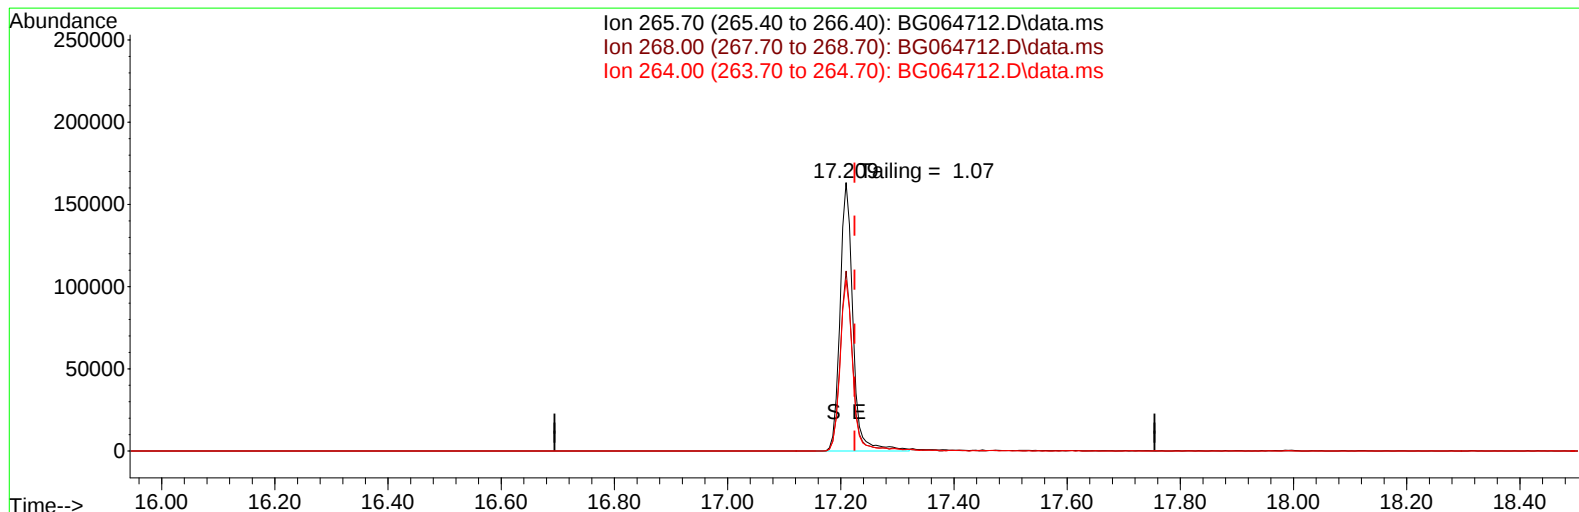

TIC: BG064712.D\data.ms

(70) Pentachlorophenol (C)




17.209min (-0.015) 37237.71 ng

response 262760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	67.03
264.00	59.10	68.17
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110725\  
Data File : BG064712.D  
Acq On    : 7 Nov 2025 10:25  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Nov 07 11:06:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

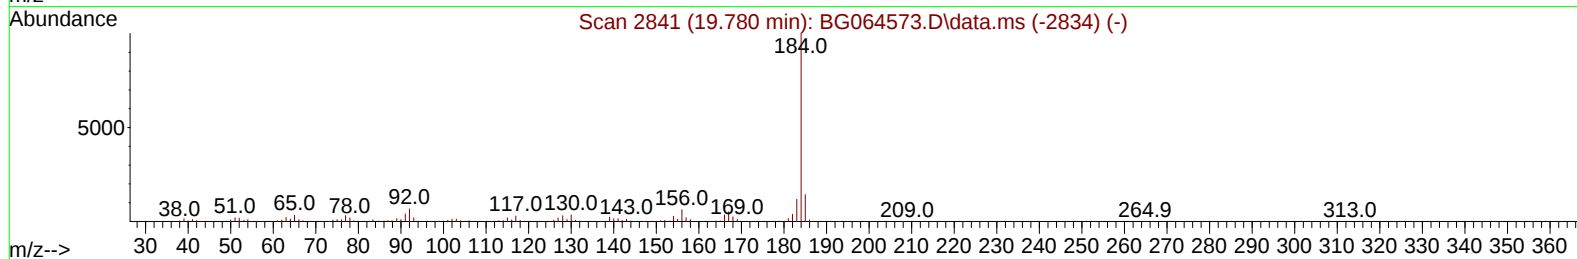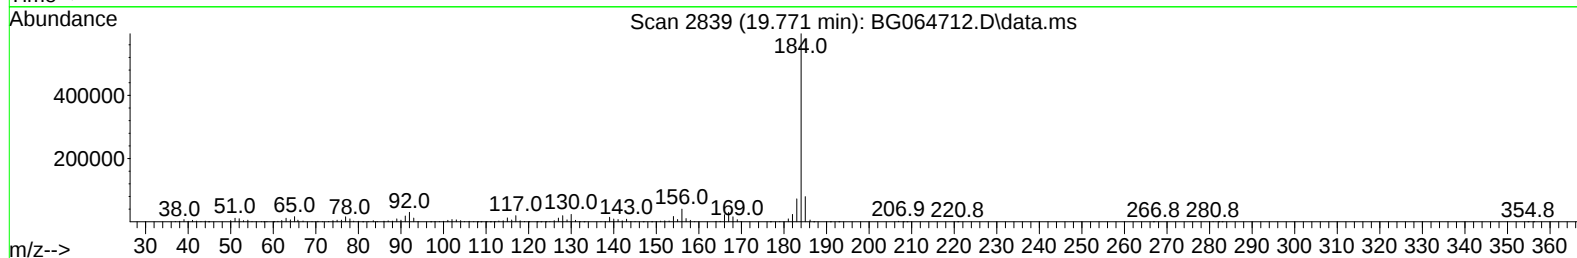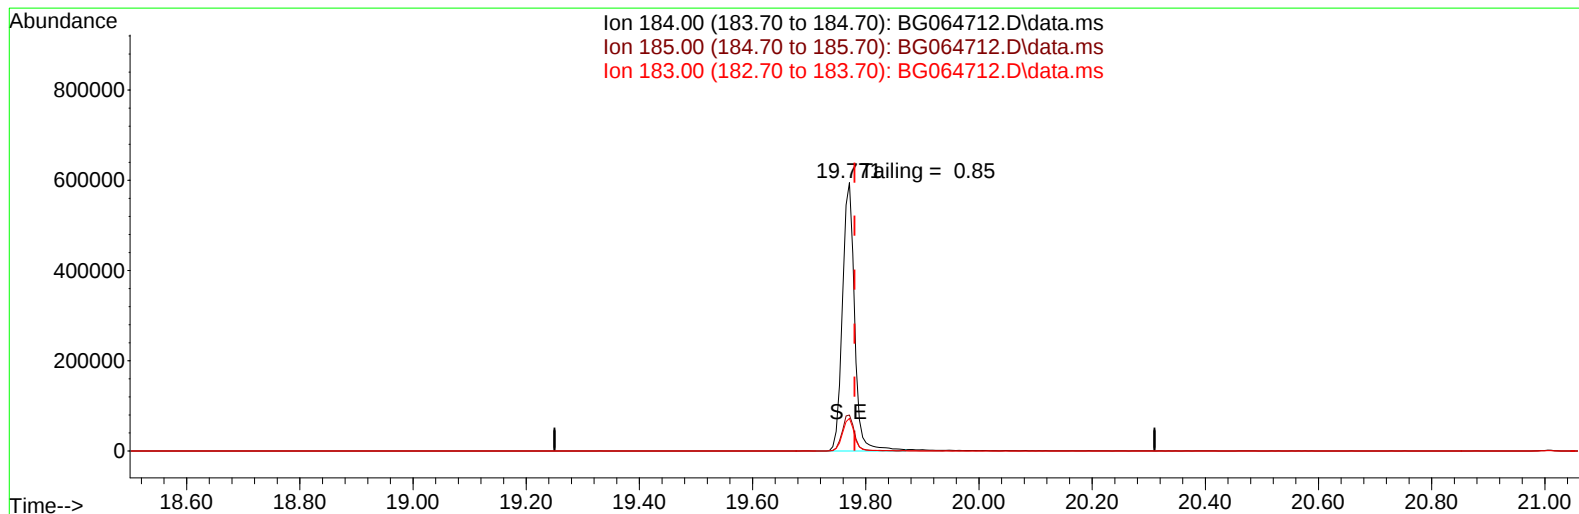

TIC: BG064712.D\data.ms

(77) Benzidine

19.771min (-0.009) 0.00 ng

response **897795**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.41
183.00	11.80	12.17
0.00	0.00	0.00