


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110818\
 Data File : BG037882.D
 Acq On : 8 Nov 2018 12:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

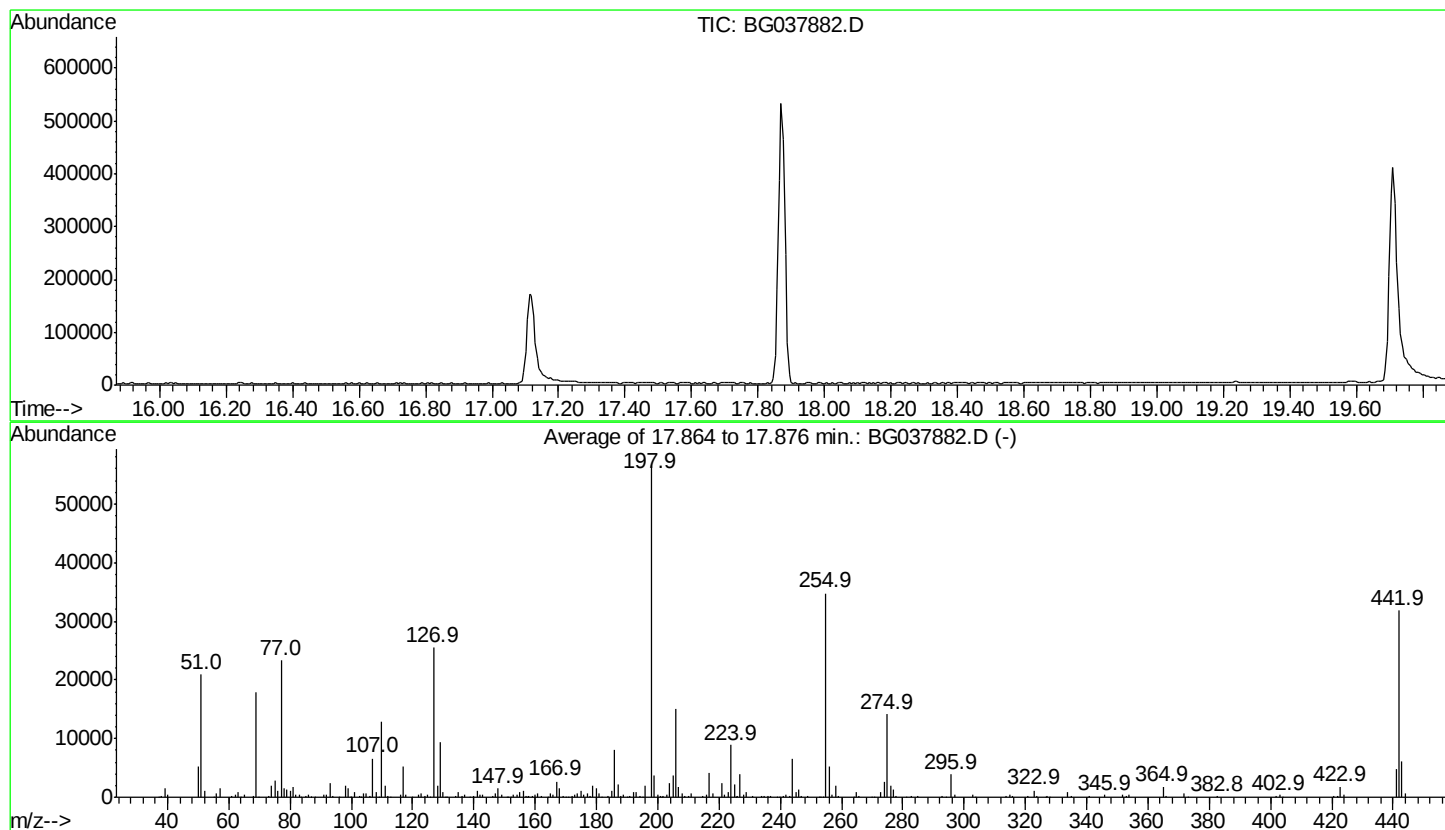

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	20880	PASS
68	69	0.00	2	1.7	307	PASS
69	198	0.00	100	31.9	18012	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	45.1	25520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56538	PASS
199	198	5	9	6.7	3767	PASS
275	198	10	60	25.1	14167	PASS
365	198	1	100	3.1	1757	PASS
441	198	0.01	100	8.4	4758	PASS
442	198	50	100	56.2	31802	PASS
443	442	15	24	19.0	6042	PASS