
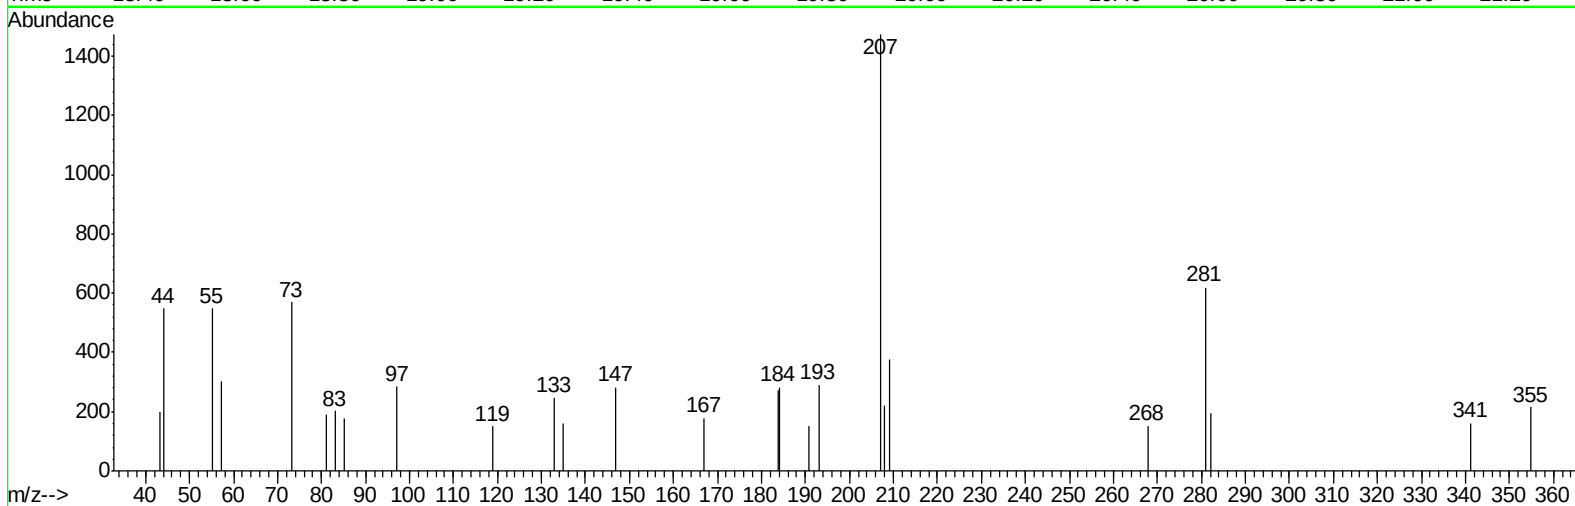


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110819\
 Data File : BG043566.D
 Acq On : 8 Nov 2019 12:16
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 06:22:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration

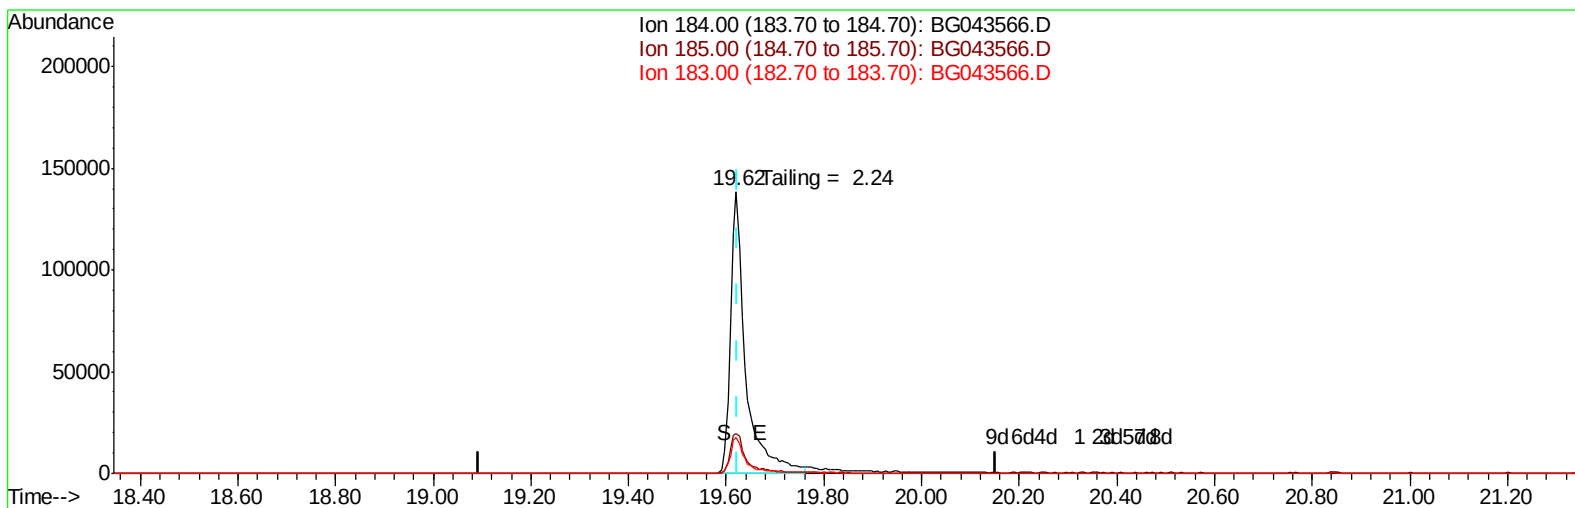

TIC: BG043566.D

(77) Benzidine



20.326min (+0.702) 232.47ng

response 262

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	0.00#
183.00	12.50	49.01#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110819\
Data File : BG043566.D
Acq On : 8 Nov 2019 12:16
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 06:22:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

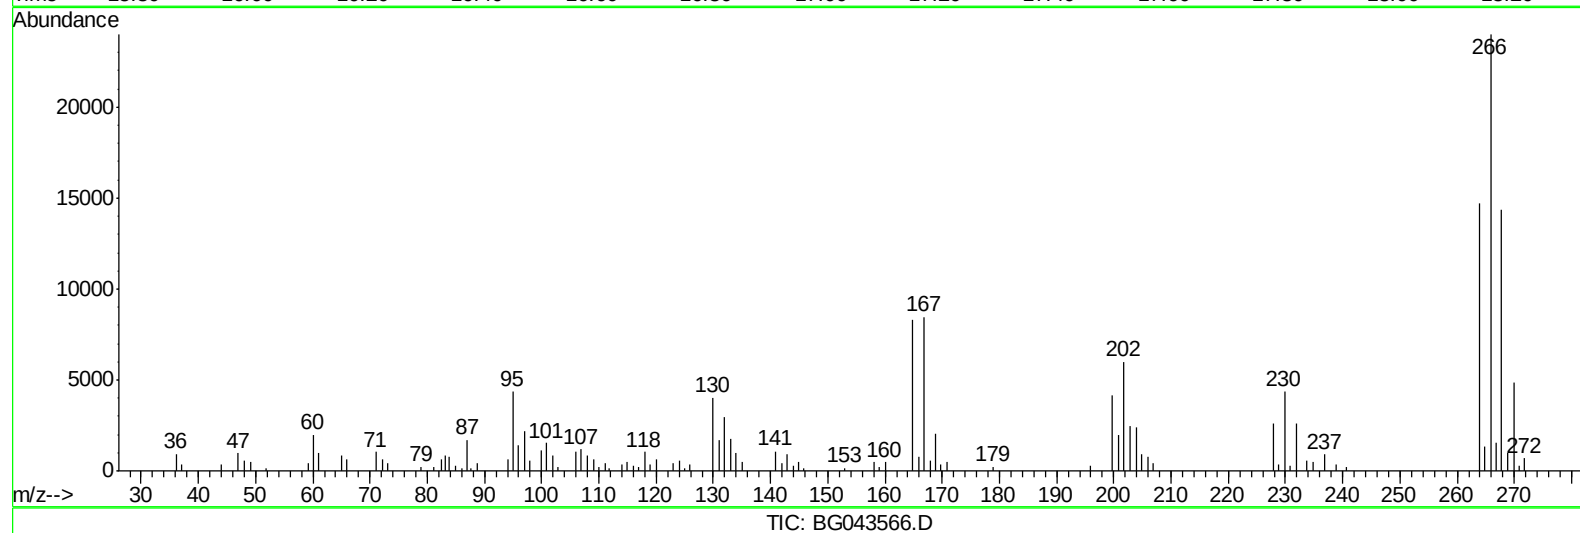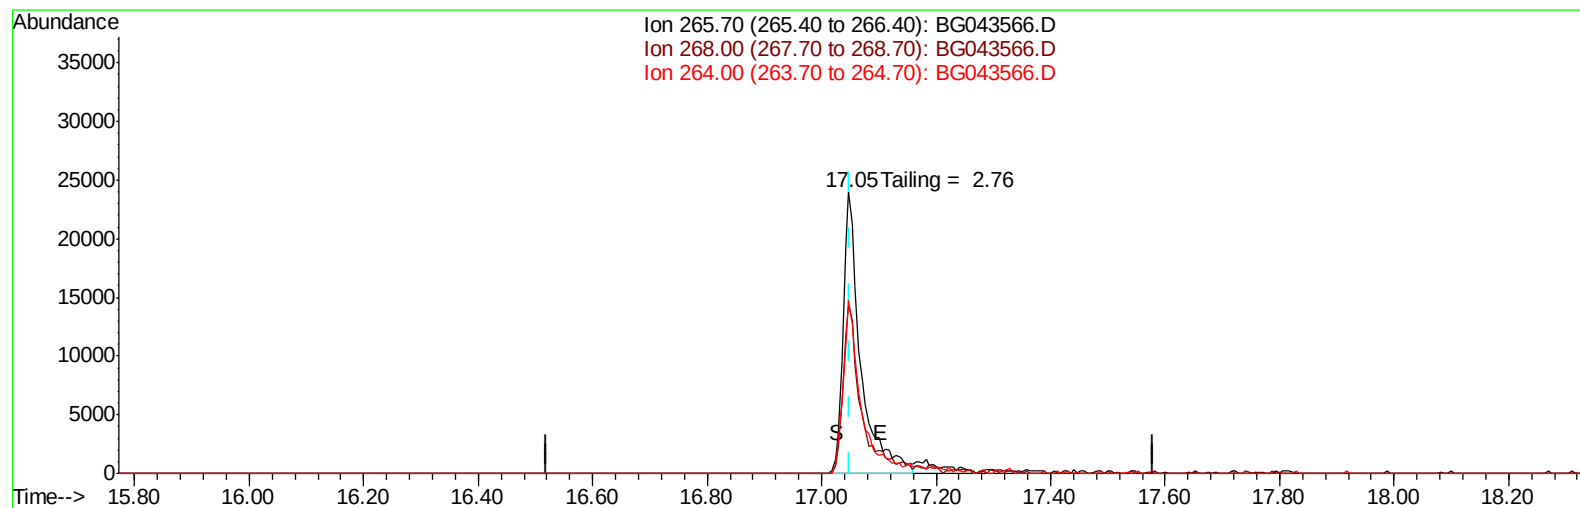

(70) Pentachlorophenol (C)

17.047min (-0.003) 29037.58ng

response 51712

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	59.73
264.00	61.10	61.33
0.00	0.00	0.00