

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110819\
 Data File : BG043572.D
 Acq On : 8 Nov 2019 16:45
 Operator : JU
 Sample : K5717-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VC-TP

Quant Time: Nov 11 03:14:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 04 15:22:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	30724	20.00	ng	0.00
21) Naphthalene-d8	10.81	136	110873	20.00	ng	0.00
39) Acenaphthene-d10	14.64	164	84721	20.00	ng	0.00
64) Phenanthrene-d10	17.39	188	201890	20.00	ng	0.00
76) Chrysene-d12	21.65	240	201821	20.00	ng	0.00
87) Perylene-d12	24.84	264	234778	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	165321	98.60	ng	0.01
7) Phenol-d6	7.20	99	229523	95.15	ng	0.00
23) Nitrobenzene-d5	9.17	82	137310	63.85	ng	-0.01
42) 2,4,6-Tribromophenol	16.13	330	140943	87.42	ng	0.00
45) 2-Fluorobiphenyl	13.25	172	352440	57.48	ng	-0.01
79) Terphenyl-d14	19.99	244	690877	64.22	ng	-0.01
Target Compounds						
10) Phenol	7.23	94	15074	6.838	ng	93
50) Dimethylphthalate	14.09	163	36371	5.542	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110819\
Data File : BG043572.D
Acq On : 8 Nov 2019 16:45
Operator : JU
Sample : K5717-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VC-TP

Quant Time: Nov 11 03:14:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

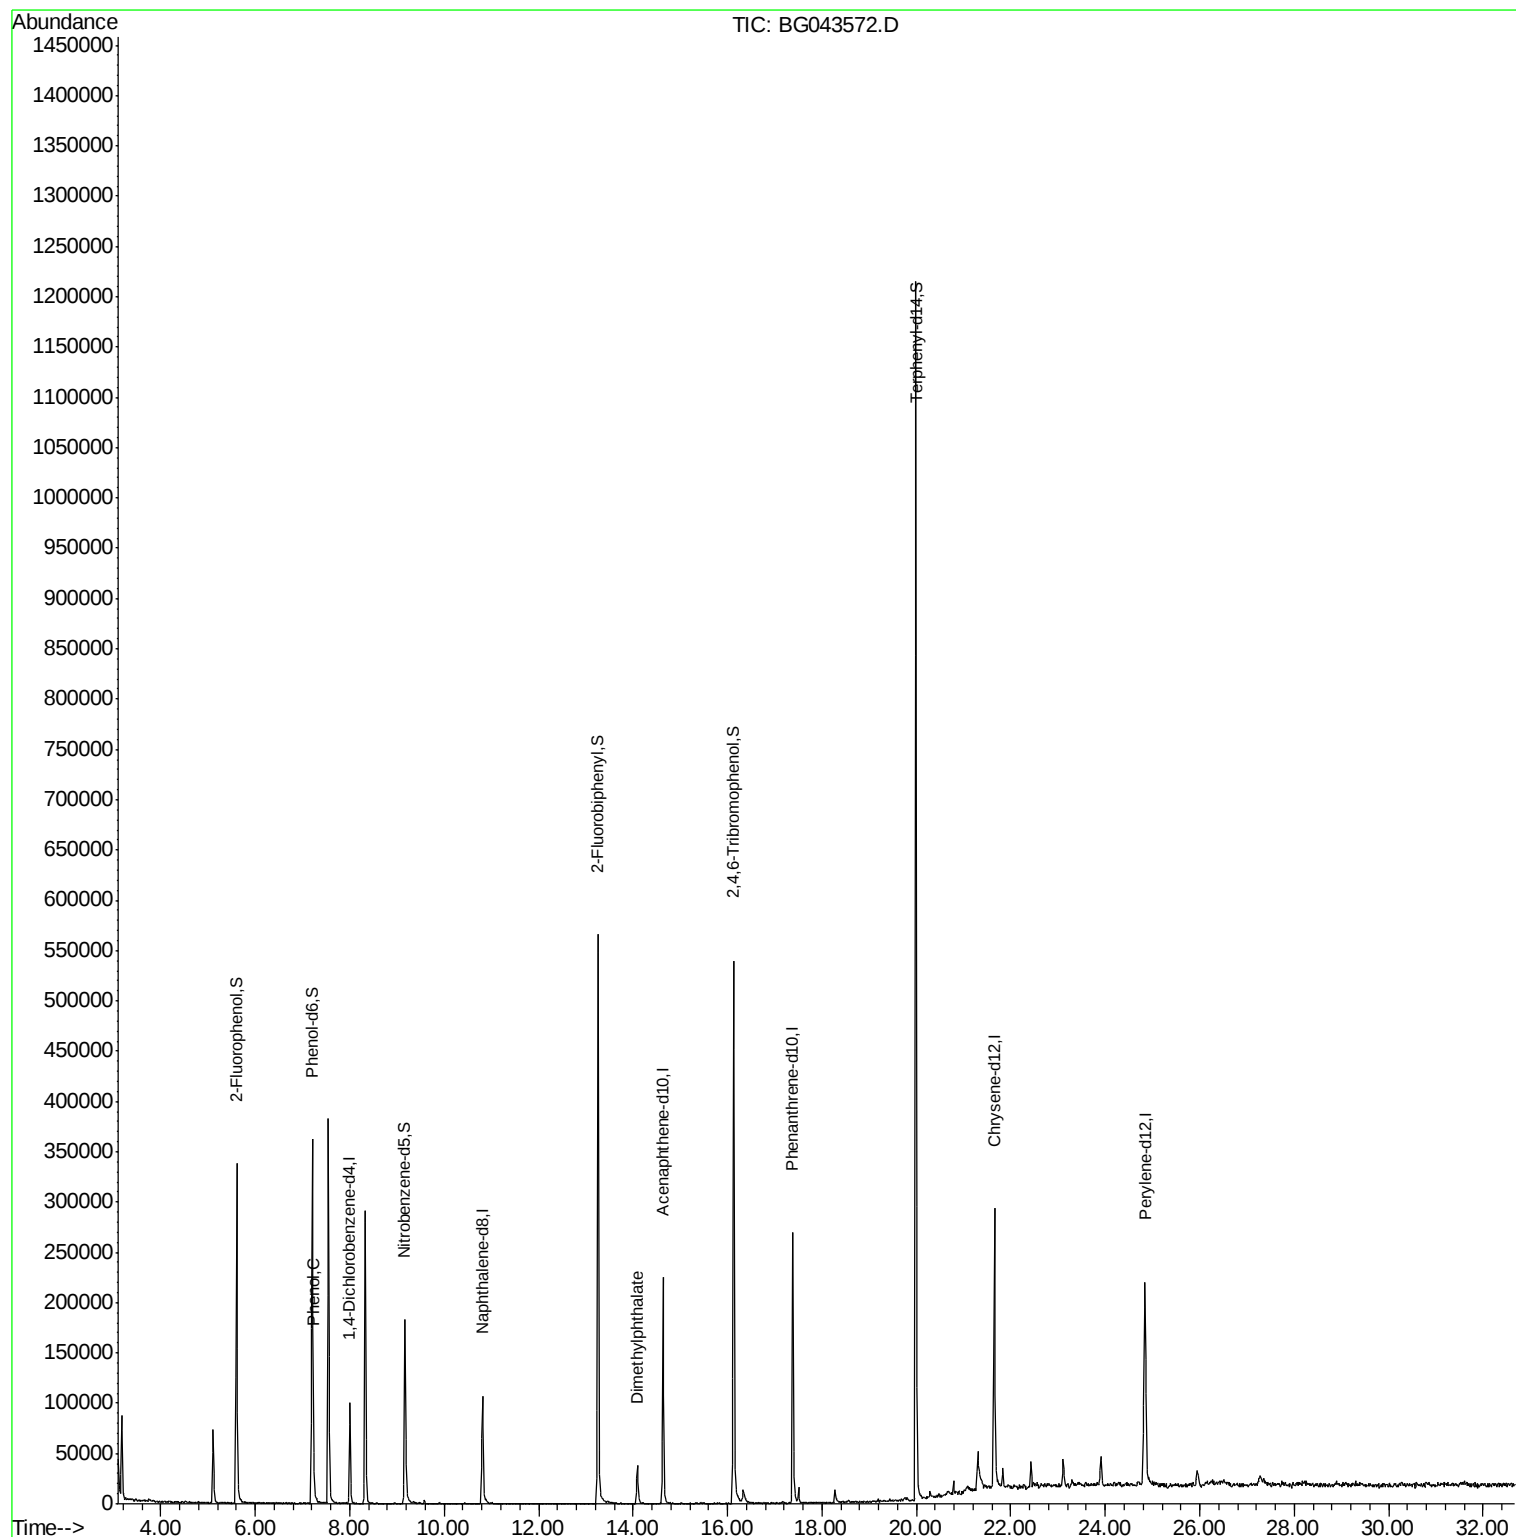




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 836
Delta R.T. -0.01 min
Lab File: BG043572.D
Acq: 8 Nov 2019 16:45

Instrument :
BNA_G
ClientSampleId :
VC-TP

Tot Ion:152 Resp: 30724
Ion Ratio Lower Upper
152 100
150 145.0 129.4 194.0
115 60.2 48.8 73.2

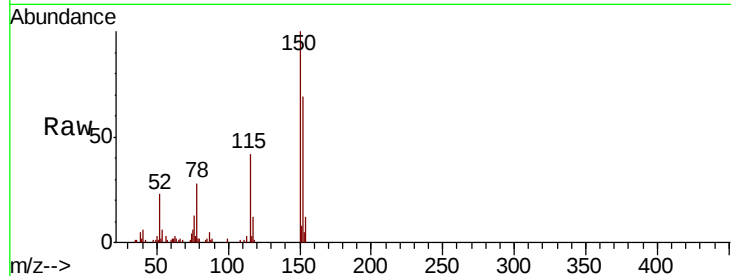


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

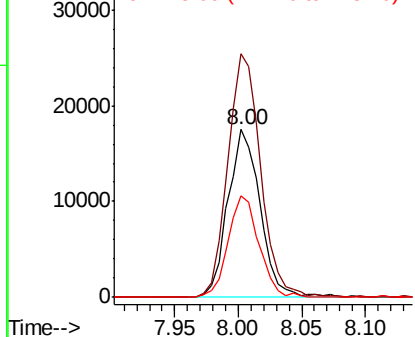



#5


2-Fluorophenol
Concen: 98.601 ng
RT: 5.60 min Scan# 428
Delta R.T. 0.01 min
Lab File: BG043572.D
Acq: 8 Nov 2019 16:45

Tgt Ion:112 Resp: 165321
Ion Ratio Lower Upper
112 100
64 59.9 50.0 75.0
63 36.7 26.6 40.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

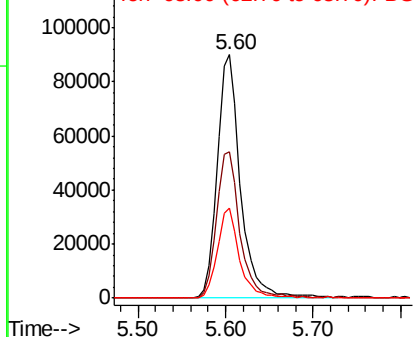

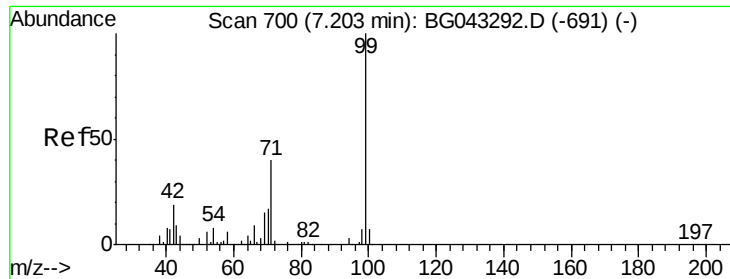

#7

Phenol-d6

Concen: 95.146 ng

RT: 7.20 min Scan# 700

Delta R.T. 0.01 min

Lab File: BG043572.D

Acq: 8 Nov 2019 16:45

Instrument :

BNA_G

ClientSampleId :

VC-TP


Tot Ion: 99 Resp: 229523

Ion Ratio Lower Upper




99 100

42 18.9 14.6 21.8

71 43.0 32.5 48.7

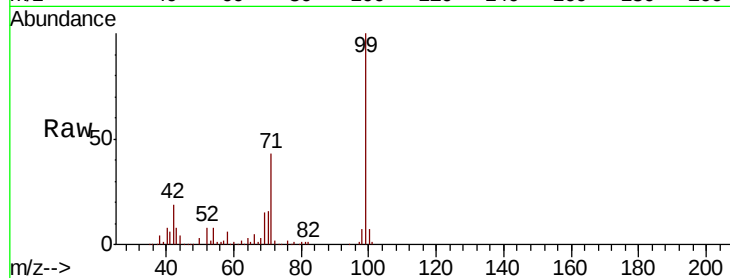

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

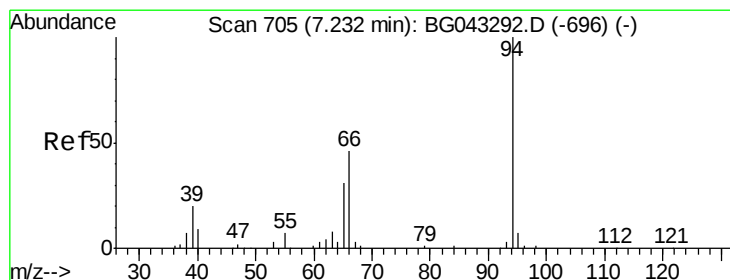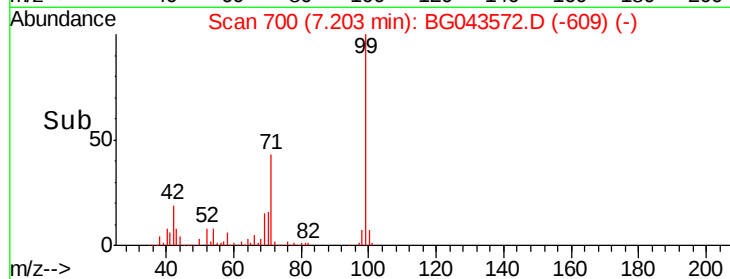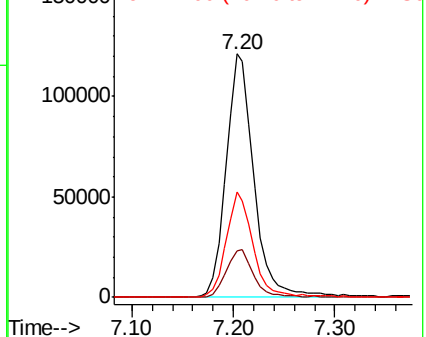

#10

Phenol

Concen: 6.838 ng

RT: 7.23 min Scan# 705

Delta R.T. 0.01 min

Lab File: BG043572.D

Acq: 8 Nov 2019 16:45


Tgt Ion: 94 Resp: 15074

Ion Ratio Lower Upper



94 100


65 31.1 12.6 52.6

66 57.7 30.7 70.7

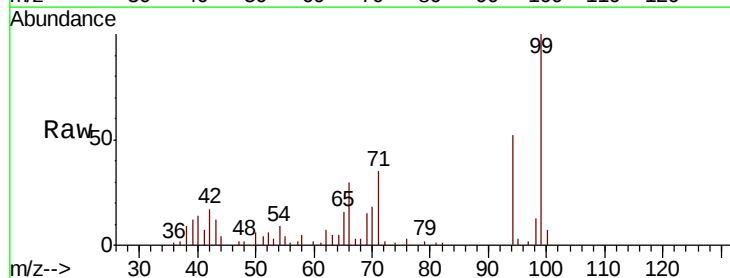

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

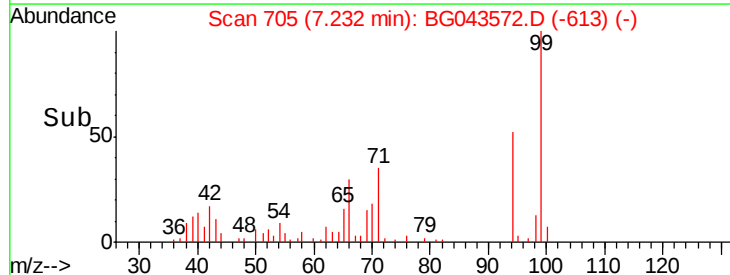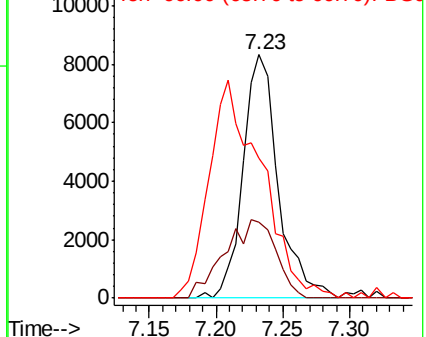







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.81 min Scan# 1314
Delta R.T. -0.01 min
Lab File: BG043572.D
Acq: 8 Nov 2019 16:45

Instrument :
BNA_G
ClientSampleId :
VC-TP

Tot Ion:136	Resp:	110873
Ion Ratio	Lower	Upper
136	100	
137	11.7	8.7 13.1
54	6.8	5.4 8.2
68	4.6	3.0 4.4

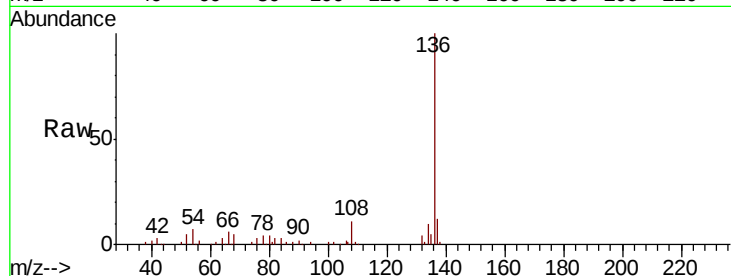


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


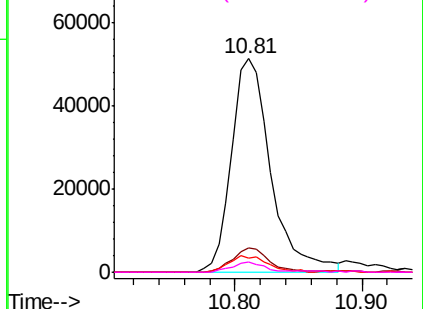



#23
Nitrobenzene-d5
Concen: 63.847 ng
RT: 9.17 min Scan# 1034
Delta R.T. -0.01 min
Lab File: BG043572.D
Acq: 8 Nov 2019 16:45

Tgt Ion: 82	Resp:	137310
Ion Ratio	Lower	Upper
82	100	
128	43.1	35.0 52.6
54	53.6	40.2 60.2



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC




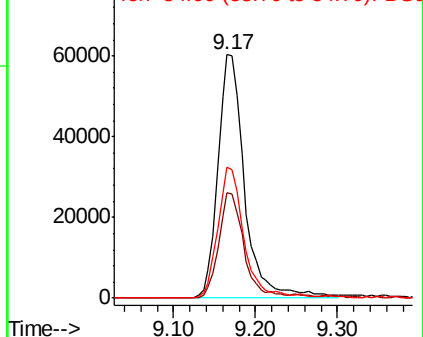




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.64 min Scan# 1965
Delta R.T. -0.01 min
Lab File: BG043572.D
Acq: 8 Nov 2019 16:45




Instrument :
BNA_G
ClientSampleId :
VC-TP


Tot Ion:164 Resp: 84721
Ion Ratio Lower Upper
164 100
162 99.2 83.5 125.3
160 43.6 36.5 54.7

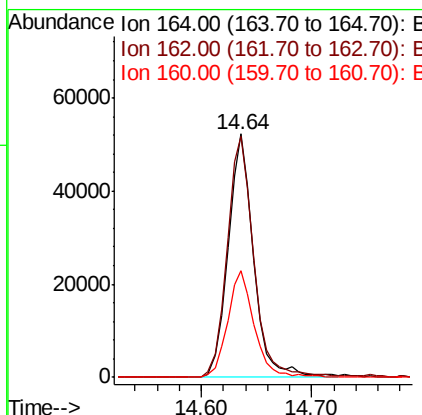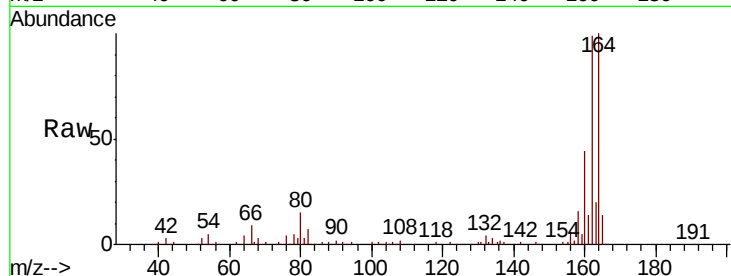

#42
2,4,6-Tribromophenol
Concen: 87.420 ng
RT: 16.13 min Scan# 2219
Delta R.T. -0.01 min
Lab File: BG043572.D
Acq: 8 Nov 2019 16:45

Tgt Ion:330 Resp: 140943
Ion Ratio Lower Upper
330 100
332 92.8 77.4 116.0
141 27.7 22.8 34.2

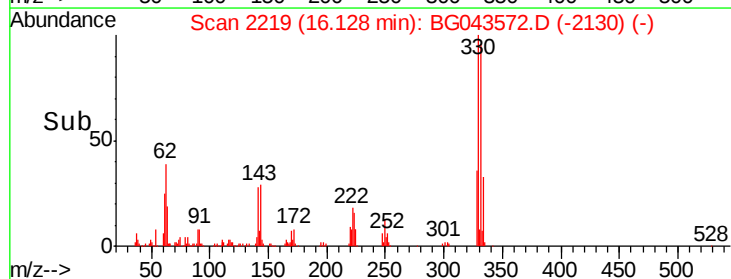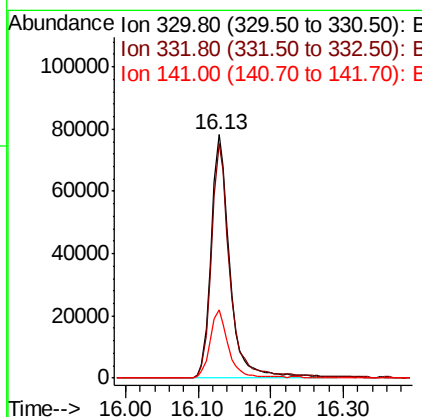







#45
 2-Fluorobiphenyl
 Concen: 57.483 ng
 RT: 13.25 min Scan# 1730
 Delta R.T. -0.01 min
 Lab File: BG043572.D
 Acq: 8 Nov 2019 16:45

Instrument :
 BNA_G
 ClientSampled :
 VC-TP

Tot Ion:172 Resp: 352440
 Ion Ratio Lower Upper
 172 100
 171 33.8 28.9 43.3
 170 22.8 18.5 27.7

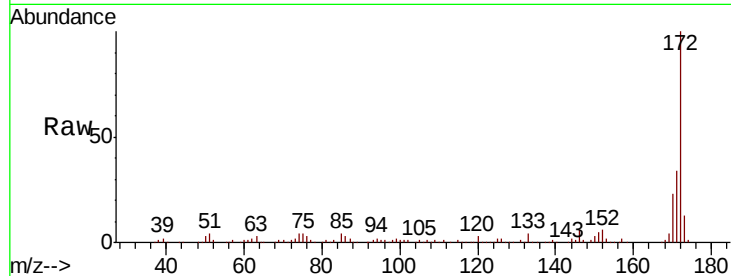


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

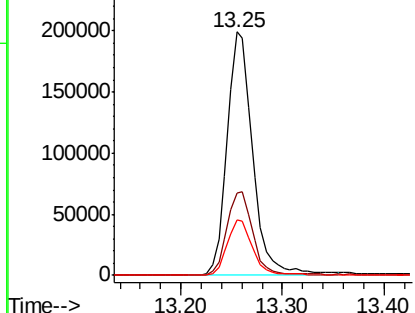




#50
 Dimethylphthalate
 Concen: 5.542 ng
 RT: 14.09 min Scan# 1872
 Delta R.T. -0.01 min
 Lab File: BG043572.D
 Acq: 8 Nov 2019 16:45

Tgt Ion:163 Resp: 36371
 Ion Ratio Lower Upper
 163 100
 194 5.4 3.8 5.6
 164 11.5 8.9 13.3

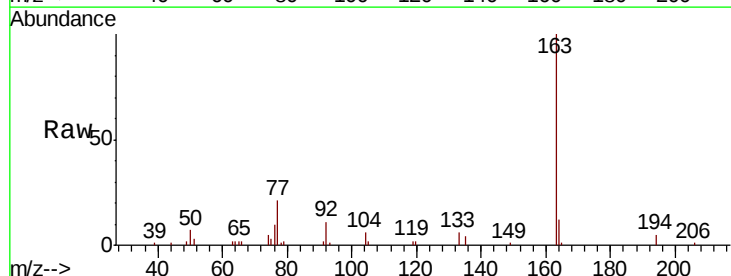

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E



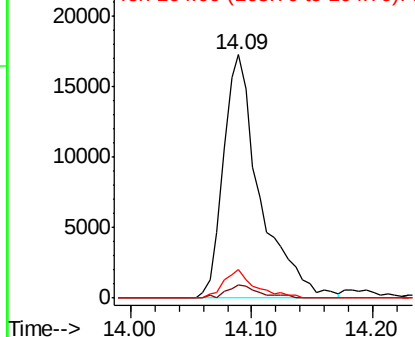



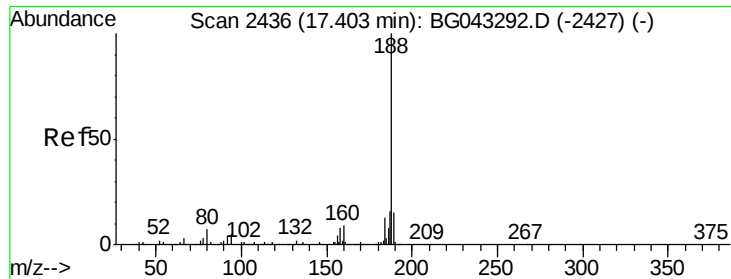

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.39 min Scan# 2433
 Delta R.T. -0.01 min
 Lab File: BG043572.D
 Acq: 8 Nov 2019 16:45




Instrument :
 BNA_G
 ClientSampleId :
 VC-TP


Tot Ion	Ratio	Lower	Upper
188	100		
94	4.7	4.2	6.4
80	6.1	4.5	6.7

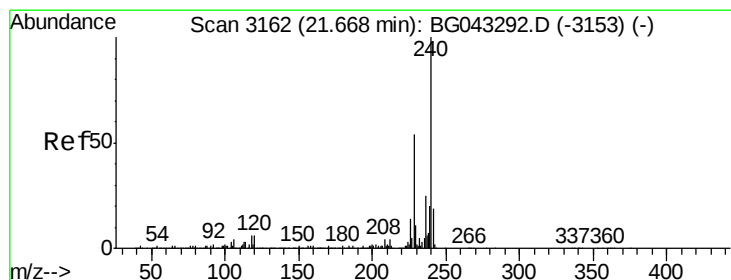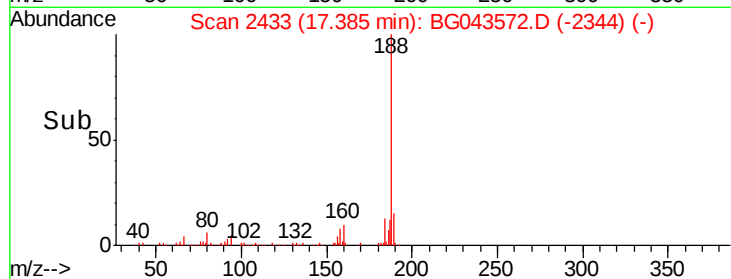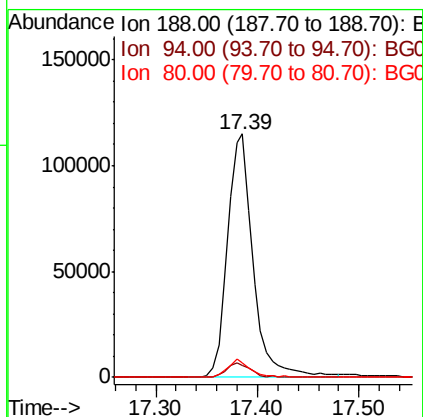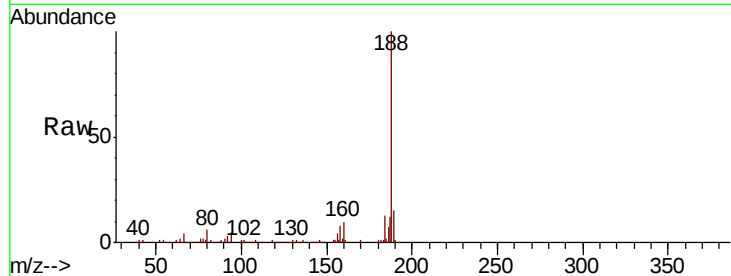

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.65 min Scan# 3159
 Delta R.T. -0.01 min
 Lab File: BG043572.D
 Acq: 8 Nov 2019 16:45

Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.4	4.6	6.8
236	25.2	19.8	29.8

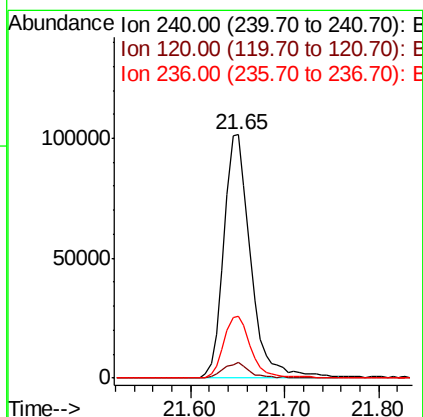



#79

Terphenyl-d14

Concen: 64.221 ng

RT: 19.99 min Scan# 2876

Delta R.T. -0.01 min

Lab File: BG043572.D

Acq: 8 Nov 2019 16:45

Instrument :

BNA_G

ClientSampleId :

VC-TP


Tot Ion:244 Resp: 690877

Ion Ratio Lower Upper




244 100

212 6.9 5.8 8.6

122 7.4 5.4 8.2

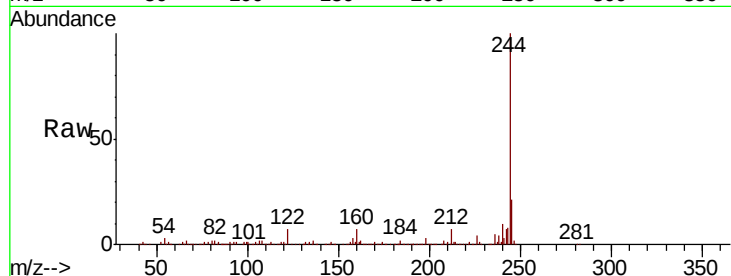

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

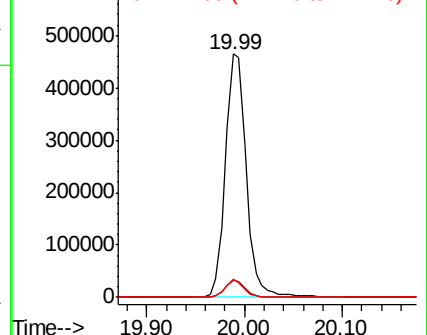

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.84 min Scan# 3701

Delta R.T. -0.02 min

Lab File: BG043572.D

Acq: 8 Nov 2019 16:45


Tgt Ion:264 Resp: 234778

Ion Ratio Lower Upper

264 100

260 22.9 17.5 26.3

265 21.2 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

