


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110819\
 Data File : BG043566.D
 Acq On : 8 Nov 2019 12:16
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

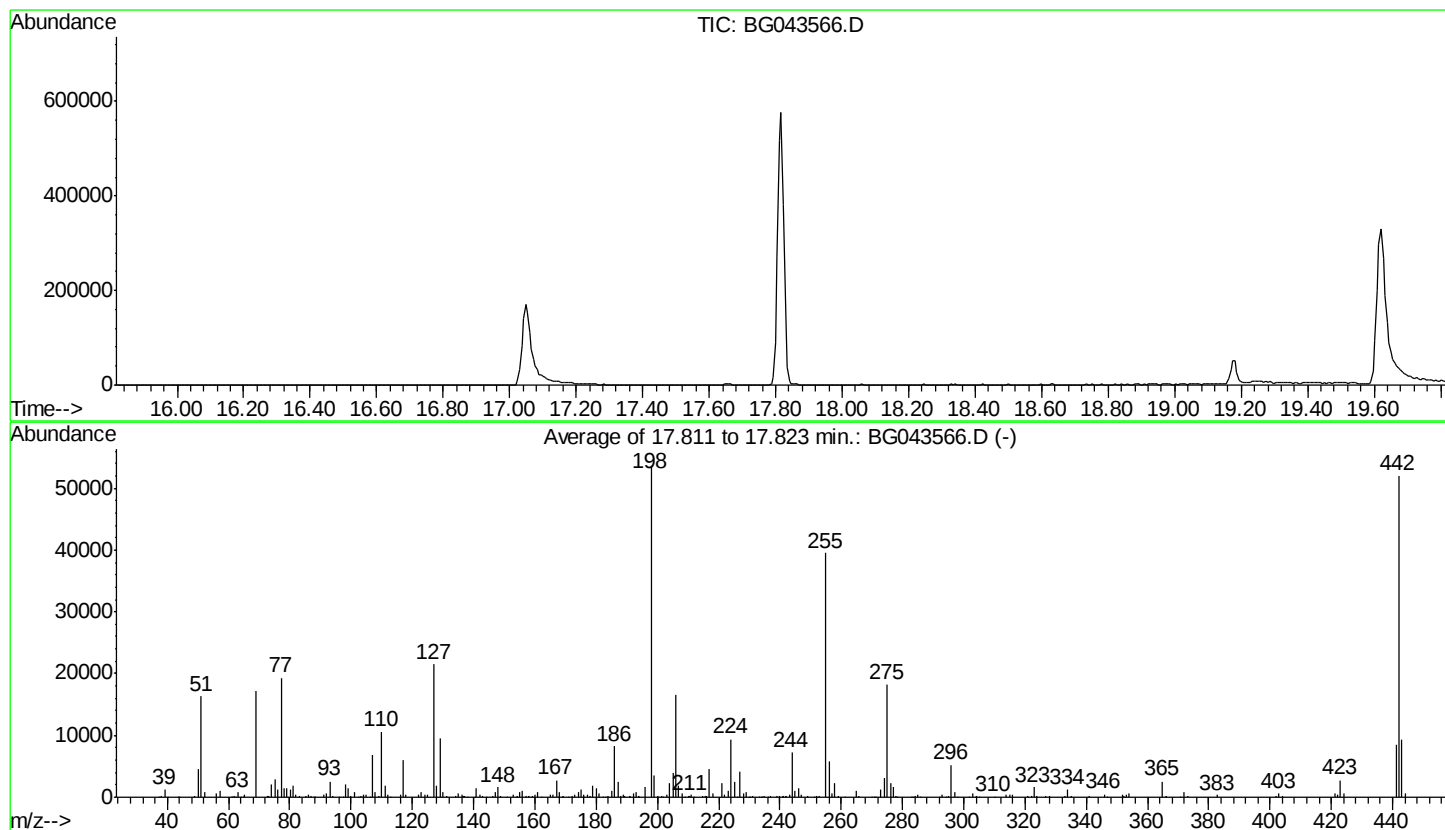

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	16330	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.2	17297	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.0	21451	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53648	PASS
199	198	5	9	6.8	3625	PASS
275	198	10	60	33.9	18200	PASS
365	198	1	100	4.8	2554	PASS
441	198	0.01	100	15.7	8445	PASS
442	198	50	100	96.9	51992	PASS
443	442	15	24	17.8	9252	PASS