Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\

Data File : BG050955.D

Acq On : 10 Nov 2021 23:48

Operator : CG/JU Sample : PB140524BS

Misc

ALS Vial : 34 Sample Multiplier: 1

Quant Time: Nov 11 01:56:02 2021


 $\label{lem:quant_method} {\tt Quant_Methods\SFAM-EPA-BG110321.M}$

Quant Title : SVOA CALIBRATION

QLast Update : Tue Nov 02 14:49:05 2021 Response via : Initial Calibration Instrument : BNA_G ClientSampleId : SLCS524

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021 Supervised By :mohammad ahmed 11/11/2021

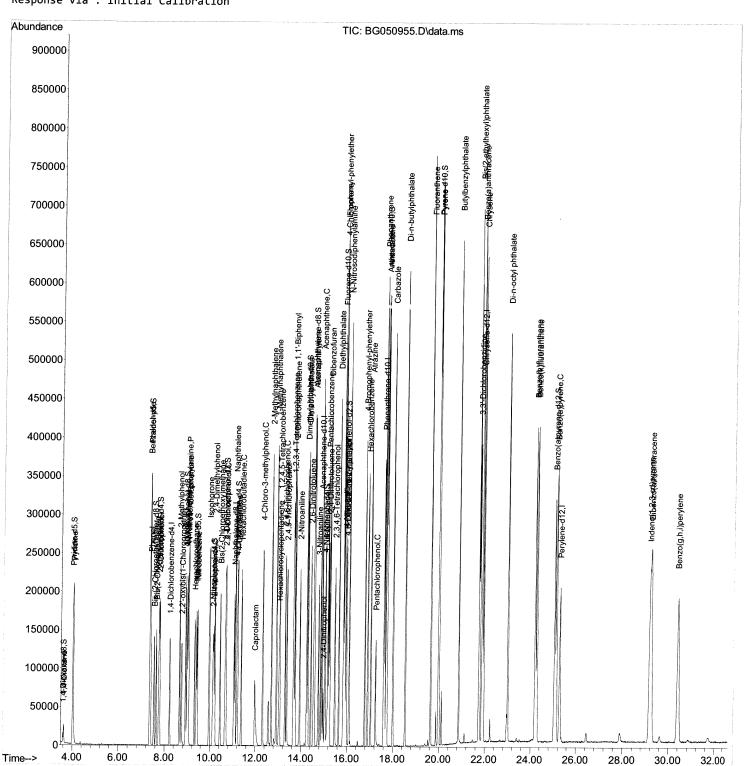

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\

Data File : BG050955.D

Acq On : 10 Nov 2021 23:48

Operator : CG/JU Sample : PB140524BS

Misc

ALS Vial : 34 Sample Multiplier: 1

Quant Time: Nov 11 01:56:02 2021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M


Quant Title : SVOA CALIBRATION

QLast Update : Tue Nov 02 14:49:05 2021 Response via : Initial Calibration



Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021 Supervised By :mohammad ahmed 11/11/2021

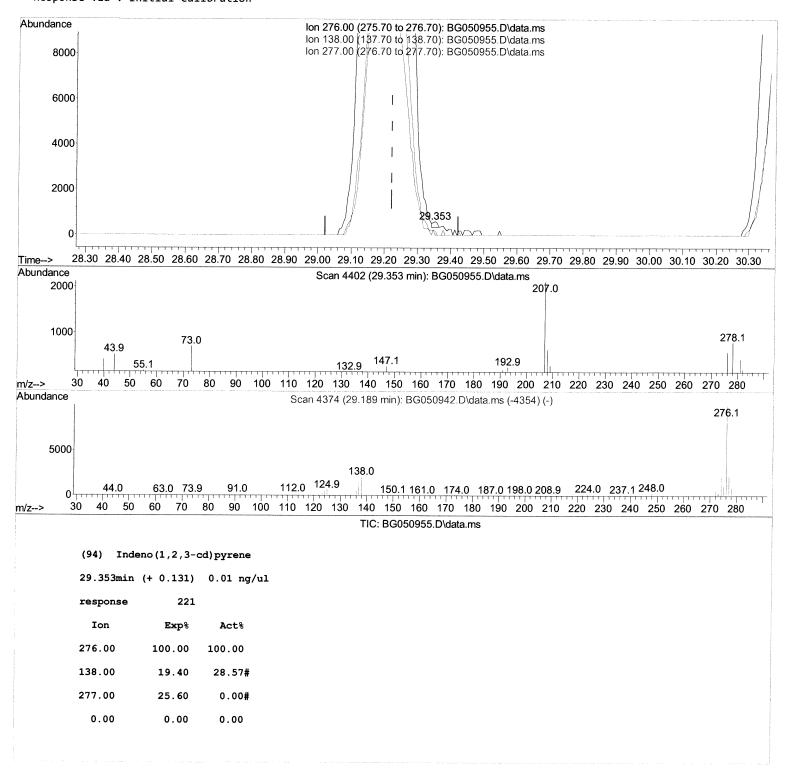

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\

Data File: BG050955.D

Acq On : 10 Nov 2021 23:48

Operator : CG/JU : PB140524BS Sample

Misc

ALS Vial : 34 Sample Multiplier: 1

Quant Time: Nov 11 01:56:02 2021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Nov 02 14:49:05 2021 Response via : Initial Calibration


Instrument: BNA_G

ClientSampleId:

SLCS524

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021 Supervised By:mohammad ahmed 11/11/2021

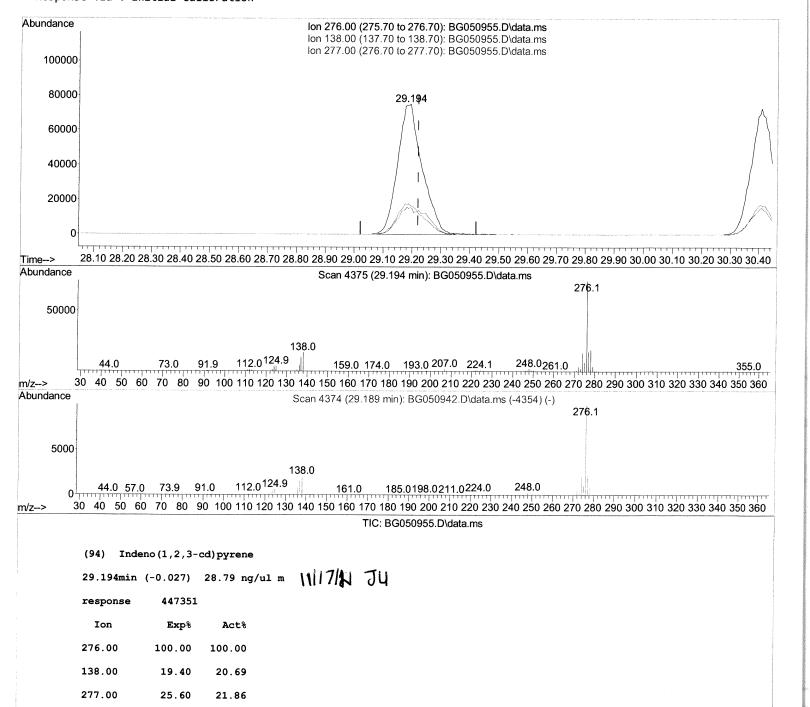

0.00

0.00

0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\

Data File : BG050955.D

Acq On : 10 Nov 2021 23:48

Operator : CG/JU Sample : PB140524BS

Misc :

ALS Vial : 34 Sample Multiplier: 1

Quant Time: Nov 11 01:56:02 2021

Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 14:49:05 2021
Response via : Initial Calibration

Instrument: BNA_G ClientSampleId: SLCS524

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021 Supervised By :mohammad ahmed 11/11/2021

Compound	R.T.	QIon	Response	Conc Units De	ev(Min)
Internal Standards					
1) 1,4-Dichlorobenzene-d4	0 220	150	27202	20 00 / 1	
20) Naphthalene-d8	8.230		37303	20.00 ng/ul	0.00
38) Acenaphthene-d10	11.051 14.852	136	163654	20.00 ng/ul	0.00
64) Phenanthrene-d10	17.596	164 188	105974	20.00 ng/ul	0.00
79) Chrysene-d12	21.891	240	235513 206524	20.00 ng/ul	0.00
88) Perylene-d12	25.287		205721	20.00 ng/ul 20.00 ng/ul	-0.02 -0.02
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.589	96	6893	5.96 ng/uL	0.00
4) Pyridine-d5	4.012	84	98357	28.45 ng/ul	0.00
7) Phenol-d5	7.367	99	113216	28.45 ng/ul	0.00
9) Bis-(2-Chloroethyl)eth	7.543	67	73475	28.58 ng/ul	0.00
<pre>11) 2-Chlorophenol-d4</pre>	7.755	132	80923	29.34 ng/ul	0.00
<pre>15) 4-Methylphenol-d8</pre>	8.924	113	84169	26.87 ng/ul	0.00
21) Nitrobenzene-d5	9.400	128	42292	30.41 ng/ul	0.00
24) 2-Nitrophenol-d4	10.122	143	45587	29.48 ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.663	165	76656	29.43 ng/ul	0.00
31) 4-Chloroaniline-d4	11.180	131	101253	25.67 ng/ul	0.00
46) Dimethylphthalate-d6	14.241	166	237250	29.26 ng/ul	0.00
49) Acenaphthylene-d8	14.547	160	304077	30.10 ng/ul	0.00
54) 4-Nitrophenol-d4	15.034	143	40140	27.31 ng/ul	0.00
60) Fluorene-d10	15.839	176	210240	29.27 ng/ul	0.00
65) 4,6-Dinitro-2-methylph73) Anthracene-d10	15.957	200	39423	27.61 ng/ul	0.00
	17.696	188	333717	29.97 ng/ul	0.00
81) Pyrene-d10 92) Benzo(a)pyrene-d12	19.970 25.052	212 264	392331 332041	29.41 ng/ul 29.20 ng/ul	0.00 -0.02
Target Compounds				٥	/alue
2) 1,4-Dioxane	3.624	88	14487	11.41 ng/uL#	92
5) Pyridine	4.029	79	101344	28.32 ng/ul	98
Benzaldehyde	7.361	77	75209	29.96 ng/ul	96
8) Phenol	7.396	94	115971	28.17 ng/ul	98
<pre>10) Bis(2-Chloroethyl)ether</pre>	7.637	93	85750	27.83 ng/ul	99
<pre>12) 2-Chlorophenol</pre>	7.784	128	79784	28.49 ng/ul	96
<pre>13) 2-Methylphenol</pre>	8.659	108	83219	27.35 ng/ul	97
<pre>14) 2,2'-oxybis(1-Chloropr</pre>	8.753	45	132212	27.24 ng/ul	99
16) Acetophenone	9.053	105	133285	27.39 ng/ul	99
17) N-Nitroso-di-n-propyla	9.030	70	76598	26.09 ng/ul	99
18) 4-Methylphenol	8.988	108	88460	27.30 ng/ul	99
19) Hexachloroethane	9.317	117	33884	28.94 ng/ul	95
22) Nitrobenzene	9.441	77	111707	28.80 ng/ul	99
23) Isophorone	9.964	82	208763	27.73 ng/ul	99
25) 2-Nitrophenol	10.158	139	45387	29.26 ng/ul	98
26) 2,4-Dimethylphenol27) Bis(2-Chloroethoxy)met	10.199	107	98910	28.97 ng/ul	99
29) 2,4-Dichlorophenol	10.440	93	115638	28.51 ng/ul	98
30) Naphthalene	10.692 11.104	162	74991	29.51 ng/ul	97
32) 4-Chloroaniline	11.104	128	262039	29.28 ng/ul	98
33) Hexachlorobutadiene	11.374	127 225	100138 50719	25.56 ng/ul	100
34) Caprolactam	11.374	113	26946	30.41 ng/ul 24.98 ng/ul	99 05
35) 4-Chloro-3-methylphenol	12.308	107	91924	28.32 ng/ul	95 97

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\

Data File : BG050955.D

Acq On : 10 Nov 2021 23:48

Operator : CG/JU Sample : PB140524BS

Misc

ALS Vial : 34 Sample Multiplier: 1

Quant Time: Nov 11 01:56:02 2021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M

Quant Title : SVOA CALIBRATION QLast Update : Tue Nov 02 14:49:05 2021 Response via : Initial Calibration

Instrument : BNA_G ClientSampleId : SLCS524

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021 Supervised By :mohammad ahmed 11/11/2021

Compound	R.T.	QIon	Response	Conc Units Dev	(Min)
36) 2-Methylnaphthalene	12.690	142	173443	28.45 ng/ul	97
37) 1-Methylnaphthalene	12.907	142	174710	28.28 ng/ul	98
39) 1,2,4,5-Tetrachloroben	13.054	216	94972	30.76 ng/ul	96
40) Hexachlorocyclopentadiene	13.025	237	34982	23.59 ng/ul	97
41) 2,4,6-Trichlorophenol	13.289	196	59701	29.55 ng/ul	97
42) 2,4,5-Trichlorophenol	13.366	196	62808	28.95 ng/ul	99
43) 1,1'-Biphenyl	13.683	154	230241	29.72 ng/ul	97
44) 2-Chloronaphthalene	13.736	162	183248	30.19 ng/ul	99
45) 2-Nitroaniline	13.936	65	69354	28.76 ng/ul	95
47) Dimethylphthalate	14.288	163	237182	29.26 ng/ul	99
48) 2,6-Dinitrotoluene	14.423	165	50864	29.98 ng/ul	96
50) Acenaphthylene	14.576	152	296680	29.31 ng/ul	98
51) 3-Nitroaniline	14.752	138	49478	28.19 ng/ul	98
52) Acenaphthene	14.911	153	197588	29.68 ng/ul	97
53) 2,4-Dinitrophenol	14.964	184	16772	17.92 ng/ul	91
55) 4-Nitrophenol	15.052	109	37197	27.59 ng/ul	96
56) Dibenzofuran	15.246	168	280454	29.43 ng/ul	100
57) 2,4-Dinitrotoluene	15.205	165	71967	29.72 ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.469	232	47536	27.88 ng/ul	98
59) Diethylphthalate	15.645	149	249115	28.71 ng/ul	100
61) Fluorene	15.892	166	219445	29.10 ng/ul	99
62) 4-Chlorophenyl-phenyle	15.880	204	117319	29.87 ng/ul	97
63) 4-Nitroaniline	15.916	138	52636	30.23 ng/ul	97
66) 4,6-Dinitro-2-methylph	15.968	198	37625	27.02 ng/ul#	95
67) N-Nitrosodiphenylamine	16.092	169	196141	29.79 ng/ul	97
68) 4-Bromophenyl-phenylether	16.773	248	72314	30.87 ng/ul	95
69) Hexachlorobenzene	16.897	284	72624	30.15 ng/ul	95
70) Atrazine	17.032	200	79226	28.38 ng/ul	97
71) Pentachlorophenol	17.243	266	26831	24.27 ng/ul	96
72) Phenanthrene	17.637	178	375179	29.84 ng/ul	99
74) Anthracene	17.731	178	375889	29.80 ng/ul	99
75) 1,2,3,4-Tetrachloroben	13.654	216	98120	30.60 ng/uL	97
76) Pentachlorobenzene	15.164	250	86425	29.09 ng/uL	98
77) Carbazole	17.995	167	347933	30.77 ng/ul	98
78) Di-n-butylphthalate	18.530	149	441326	29.71 ng/ul	100
80) Fluoranthene	19.635	202	465438	29.07 ng/ul	99
82) Pyrene	19.999	202	451135	28.84 ng/ul	99
83) Butylbenzylphthalate84) 3,3'-Dichlorobenzidine	20.863	149	191773	28.51 ng/ul	97
85) Benzo(a)anthracene	21.773	252	134194	26.68 ng/ul	99
86) Bis(2-ethylhexyl)phtha	21.867	228	414262	28.97 ng/ul	100
87) Chrysene	21.738	149	277544	28.75 ng/ul	100
89) Di-n-octyl phthalate	21.938 23.007	228 149	400104 470090	29.29 ng/ul	100
90) Benzo(b)fluoranthene	24.200	252	422406	28.07 ng/ul 28.82 ng/ul	100
91) Benzo(k)fluoranthene	24.270	252	390066	28.36 ng/ul	98 100
93) Benzo(a)pyrene	25.128	252	398730	28.57 ng/ul	100
94) Indeno(1,2,3-cd)pyrene	29.194	276	447351m >	28.79 ng/ul>	11117/21 70
95) Dibenzo(a,h)anthracene	29.247	278	377686	28.73 ng/ul >	100
96) Benzo(g,h,i)perylene	30.410	276	373968	28.75 ng/ul	98
, (6), -/per j =====	20.710	_, 0	3, 3300	-3.75 Hg/ u1	20

^{(#) =} qualifier out of range (m) = manual integration (+) = signals summed