

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050925.D
 Acq On : 10 Nov 2021 1:52
 Operator : CG/JU
 Sample : M4532-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB858

Quant Time: Nov 10 07:40:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 14:49:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.232	152	37780	20.000	ng/u1	0.00
20) Naphthalene-d8	11.052	136	164091	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.853	164	107831	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.597	188	247002	20.000	ng/u1	0.00
79) Chrysene-d12	21.892	240	215806	20.000	ng/u1	-0.01
88) Perylene-d12	25.288	264	210699	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.590	96	5922	5.059	ng/uL	0.00
4) Pyridine-d5	4.025	84	11131	3.179	ng/u1	0.00
7) Phenol-d5	7.368	99	28316	7.026	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.544	67	78880	30.297	ng/u1	0.00
11) 2-Chlorophenol-d4	7.756	132	66200	23.700	ng/u1	0.00
15) 4-Methylphenol-d8	8.925	113	46998	14.812	ng/u1	0.00
21) Nitrobenzene-d5	9.401	128	43134	30.932	ng/u1	0.00
24) 2-Nitrophenol-d4	10.129	143	44746	28.859	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.670	165	70024	26.810	ng/u1	0.00
31) 4-Chloroaniline-d4	11.187	131	73533	18.591	ng/u1	0.00
46) Dimethylphthalate-d6	14.242	166	289141	35.048	ng/u1	0.00
49) Acenaphthylene-d8	14.548	160	333987	32.495	ng/u1	0.00
54) 4-Nitrophenol-d4	15.041	143	9622	6.433	ng/u1	0.00
60) Fluorene-d10	15.840	176	249278	34.110	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.952	200	43906	29.319	ng/u1	0.00
73) Anthracene-d10	17.697	188	446014	38.193	ng/u1	0.00
81) Pyrene-d10	19.971	212	513031	36.806	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.053	264	427444	36.697	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.625	88	83989	65.326	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050925.D
Acq On : 10 Nov 2021 1:52
Operator : CG/JU
Sample : M4532-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB858


Quant Time: Nov 10 07:40:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 14:49:05 2021
Response via : Initial Calibration

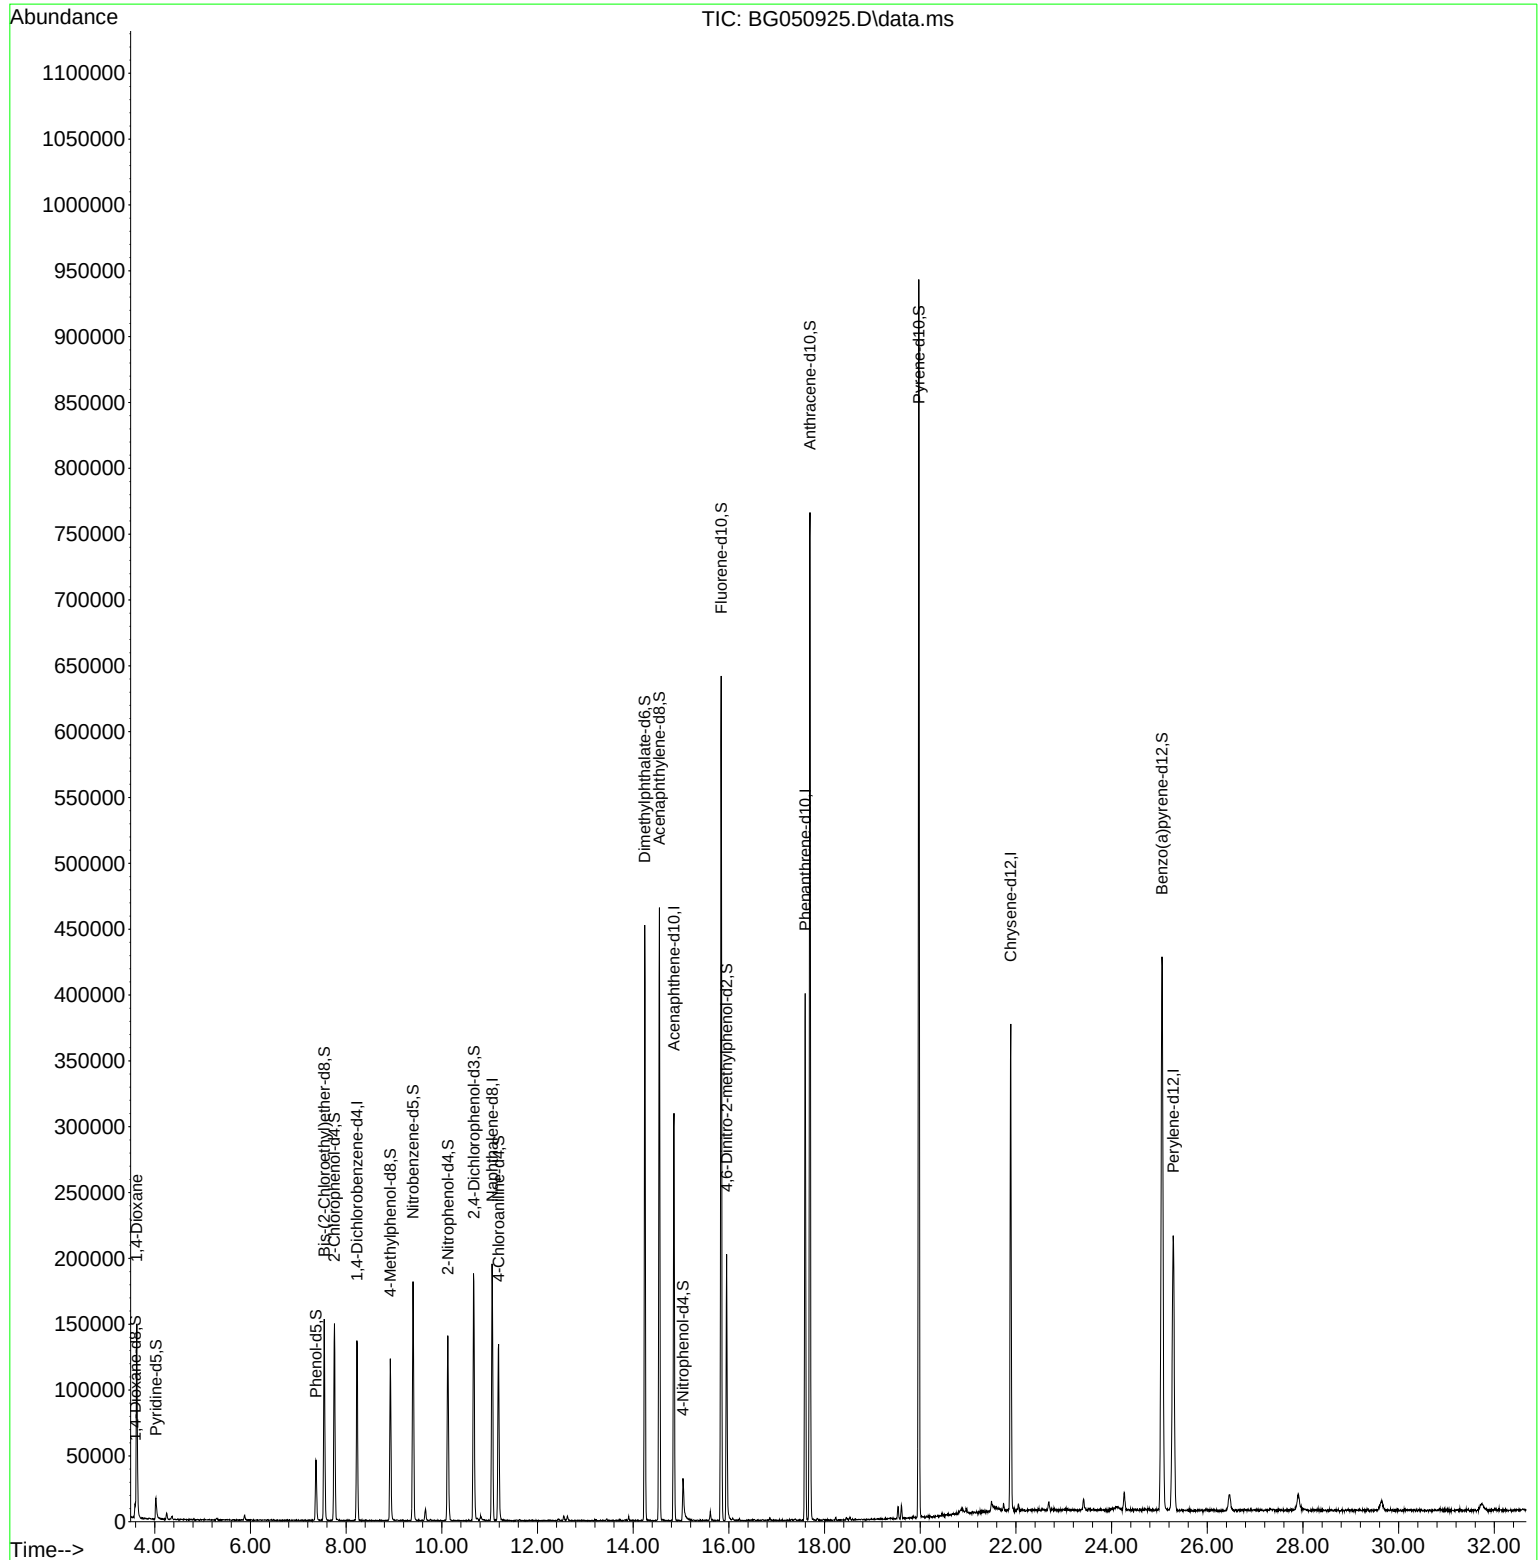

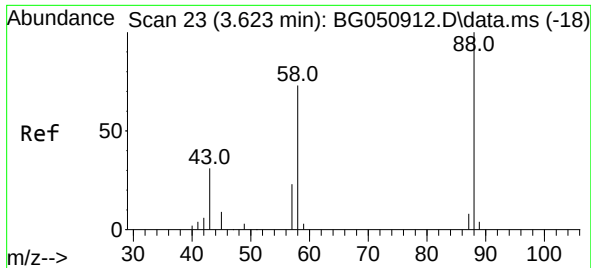

#2
 1,4-Dioxane
 Concen: 65.326 ng/uL
 RT: 3.625 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BG050925.D
 Acq: 10 Nov 2021 1:52

Instrument :
 BNA_G
 ClientSampleId :
 GB858

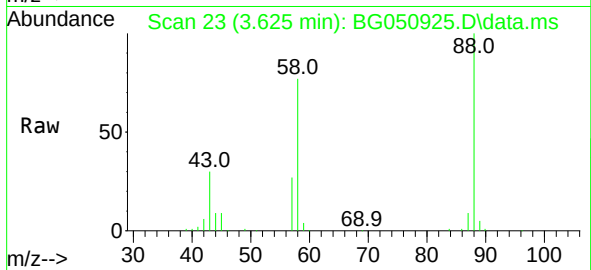

Tgt Ion:	88	Resp:	83989
Ion	Ratio	Lower	Upper
88	100		
43	30.2	23.0	34.4
58	77.0	62.4	93.6

