

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050931.D
 Acq On : 10 Nov 2021 6:41
 Operator : CG/JU
 Sample : M4532-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB8E8

Quant Time: Nov 10 09:17:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 14:49:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.225	152	34737	20.000	ng/u1	0.00
20) Naphthalene-d8	11.052	136	148730	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.853	164	98961	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.597	188	217889	20.000	ng/u1	0.00
79) Chrysene-d12	21.892	240	192790	20.000	ng/u1	-0.01
88) Perylene-d12	25.288	264	186358	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.590	96	7045	6.546	ng/uL	0.00
4) Pyridine-d5	4.019	84	39858	12.379	ng/u1	0.00
7) Phenol-d5	7.368	99	33665	9.084	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.544	67	85879	35.875	ng/u1	0.00
11) 2-Chlorophenol-d4	7.755	132	74596	29.046	ng/u1	0.00
15) 4-Methylphenol-d8	8.925	113	55564	19.046	ng/u1	0.00
21) Nitrobenzene-d5	9.401	128	48093	38.051	ng/u1	0.00
24) 2-Nitrophenol-d4	10.123	143	50928	36.238	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.664	165	78044	32.967	ng/u1	0.00
31) 4-Chloroaniline-d4	11.187	131	112155	31.284	ng/u1	0.00
46) Dimethylphthalate-d6	14.242	166	300408	39.678	ng/u1	0.00
49) Acenaphthylene-d8	14.547	160	360287	38.195	ng/u1	0.00
54) 4-Nitrophenol-d4	15.041	143	11812	8.605	ng/u1	0.00
60) Fluorene-d10	15.840	176	257905	38.453	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.952	200	43806	33.161	ng/u1	0.00
73) Anthracene-d10	17.697	188	427837	41.531	ng/u1	0.00
81) Pyrene-d10	19.970	212	490045	39.355	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.053	264	417964	40.570	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.625	88	44946	38.021	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050931.D
Acq On : 10 Nov 2021 6:41
Operator : CG/JU
Sample : M4532-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8E8


Quant Time: Nov 10 09:17:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 14:49:05 2021
Response via : Initial Calibration

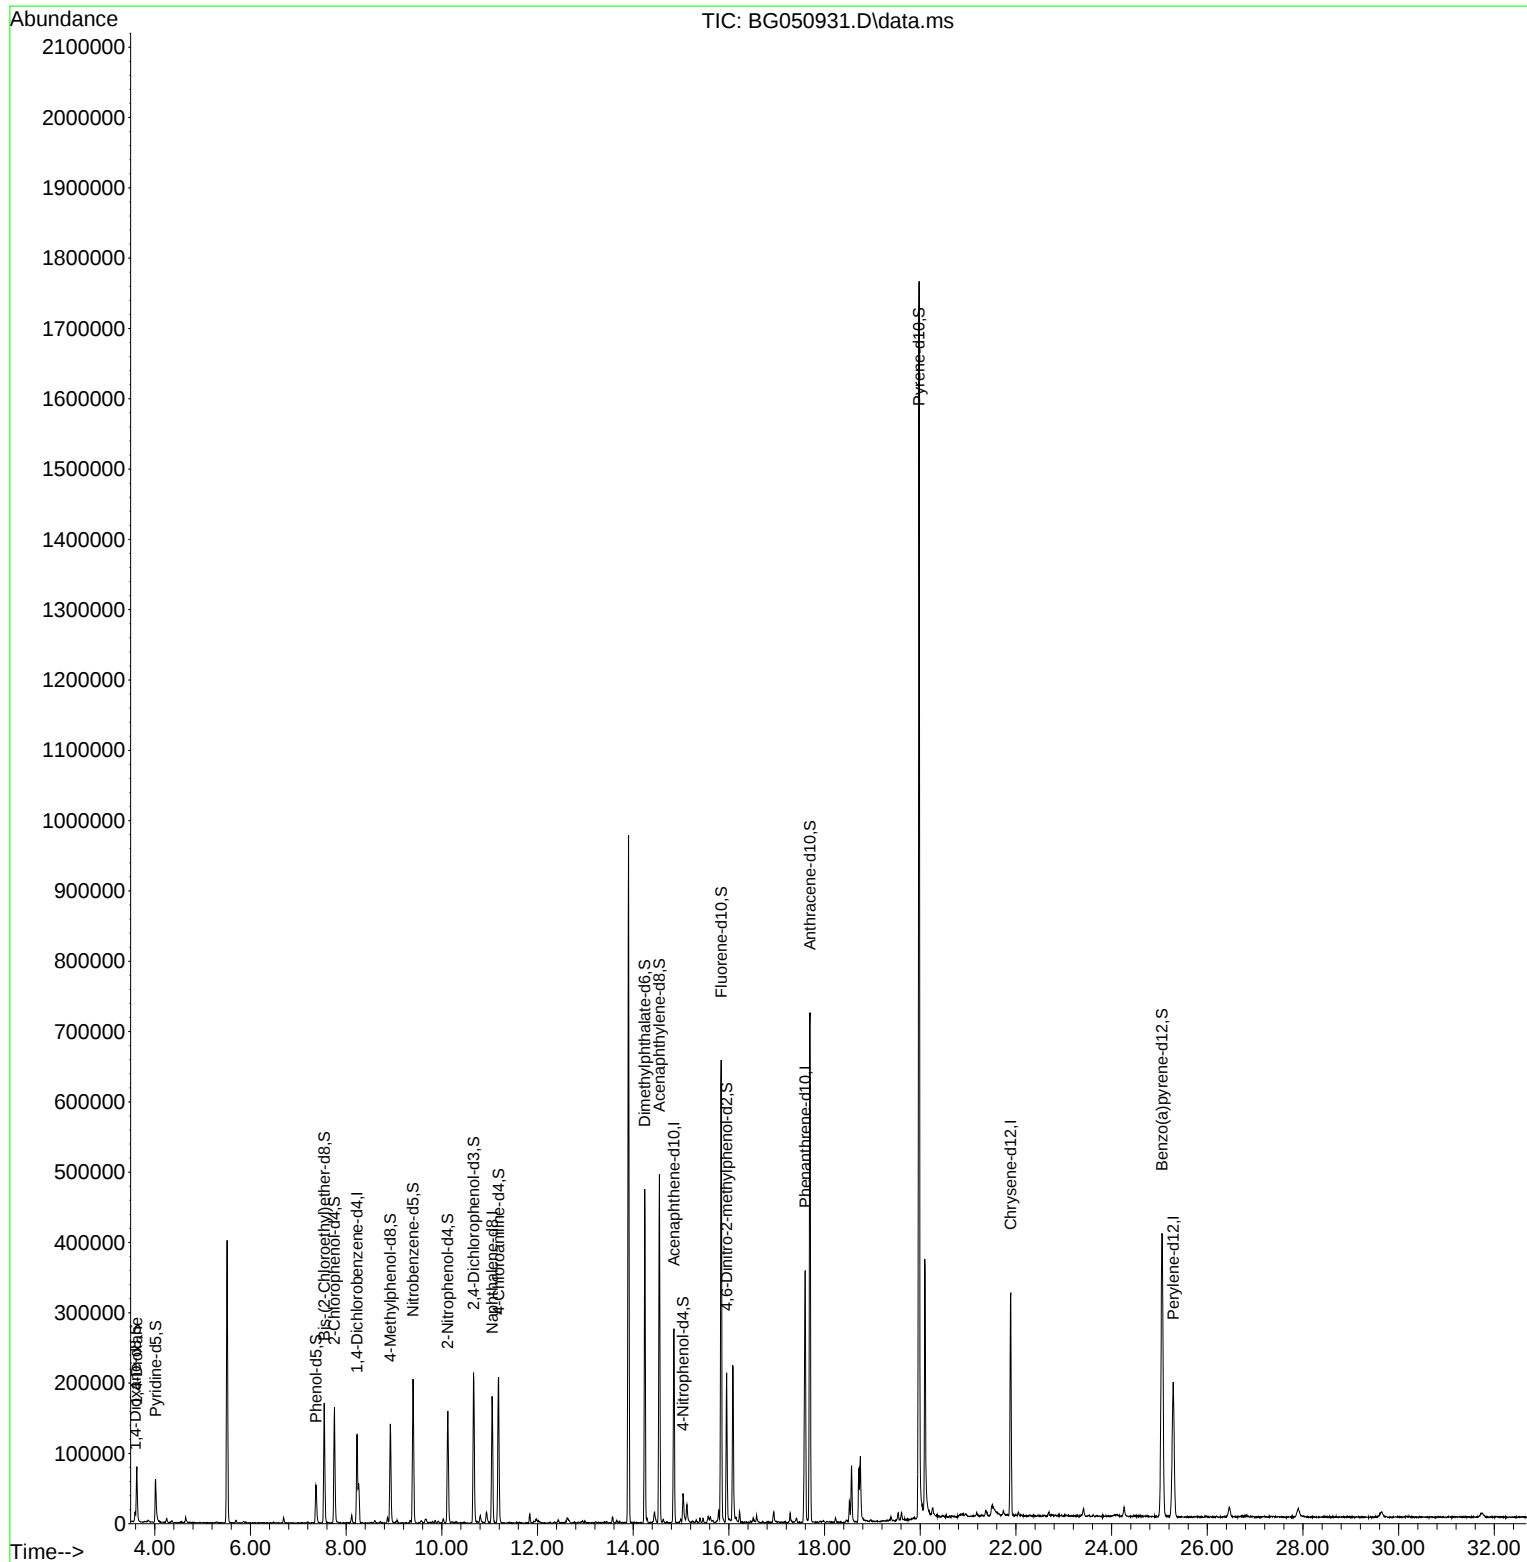

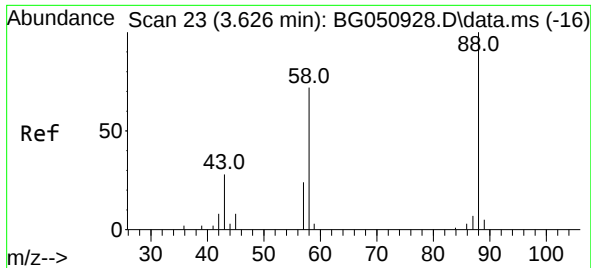

#2
 1,4-Dioxane
 Concen: 38.021 ng/uL
 RT: 3.625 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BG050931.D
 Acq: 10 Nov 2021 6:41

Instrument :
 BNA_G
 ClientSampleId :
 GB8E8

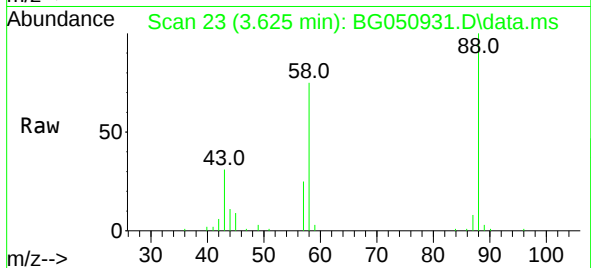

Tgt Ion:	88	Resp:	44946
Ion	Ratio	Lower	Upper
88	100		
43	30.8	23.0	34.4
58	74.8	62.4	93.6

