

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050935.D
 Acq On : 10 Nov 2021 9:26
 Operator : CG/JU
 Sample : M4532-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB860

Quant Time: Nov 10 10:43:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 14:49:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.230	152	44635	20.000	ng/u1	0.00
20) Naphthalene-d8	11.050	136	195413	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.852	164	127121	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.596	188	277203	20.000	ng/u1	-0.01
79) Chrysene-d12	21.890	240	245981	20.000	ng/u1	-0.02
88) Perylene-d12	25.292	264	240829	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.588	96	6648	4.807	ng/uL	0.00
4) Pyridine-d5	4.017	84	28053	6.781	ng/u1	0.00
7) Phenol-d5	7.372	99	32935	6.917	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.543	67	80645	26.218	ng/u1	0.00
11) 2-Chlorophenol-d4	7.754	132	71010	21.518	ng/u1	-0.01
15) 4-Methylphenol-d8	8.923	113	52700	14.058	ng/u1	-0.01
21) Nitrobenzene-d5	9.399	128	45354	27.311	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.128	143	47574	25.765	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.668	165	74516	23.957	ng/u1	0.00
31) 4-Chloroaniline-d4	11.185	131	100625	21.363	ng/u1	0.00
46) Dimethylphthalate-d6	14.246	166	312271	32.108	ng/u1	0.00
49) Acenaphthylene-d8	14.546	160	354854	29.286	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.046	143	12553	7.119	ng/u1	0.00
60) Fluorene-d10	15.839	176	270160	31.357	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.950	200	48565	28.897	ng/u1	-0.01
73) Anthracene-d10	17.695	188	451730	34.468	ng/u1	-0.01
81) Pyrene-d10	19.969	212	519830	32.719	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.057	264	441497	33.162	ng/u1	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.630	88	3079	2.027	ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050935.D
Acq On : 10 Nov 2021 9:26
Operator : CG/JU
Sample : M4532-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB860


Quant Time: Nov 10 10:43:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 14:49:05 2021
Response via : Initial Calibration

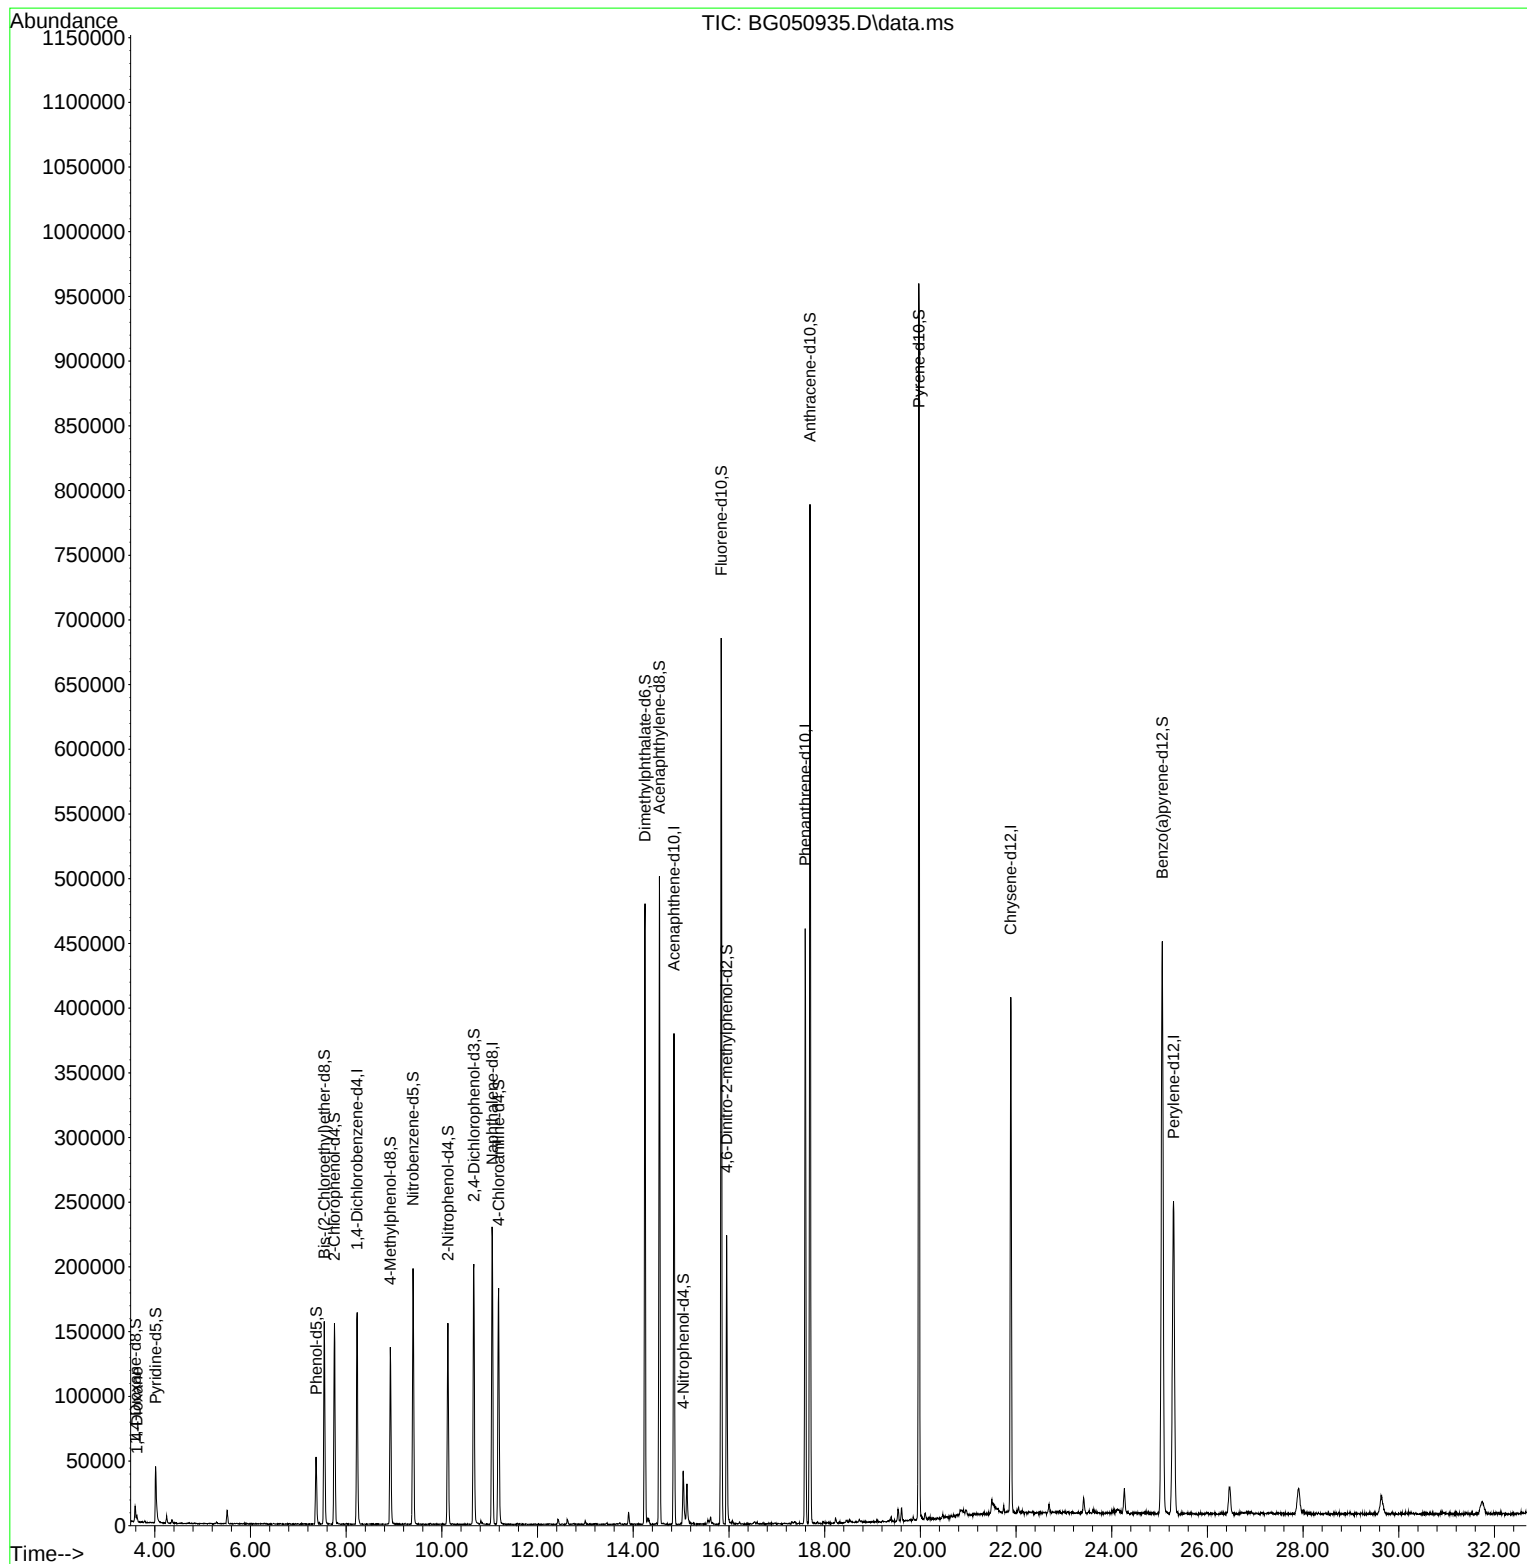

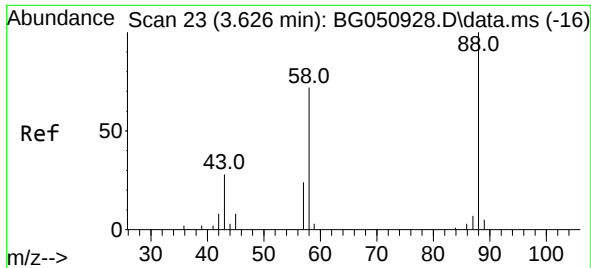

#2
 1,4-Dioxane
 Concen: 2.027 ng/uL
 RT: 3.630 min Scan# 24
 Delta R.T. 0.002 min
 Lab File: BG050935.D
 Acq: 10 Nov 2021 9:26

Instrument :
 BNA_G
 ClientSampleId :
 GB860

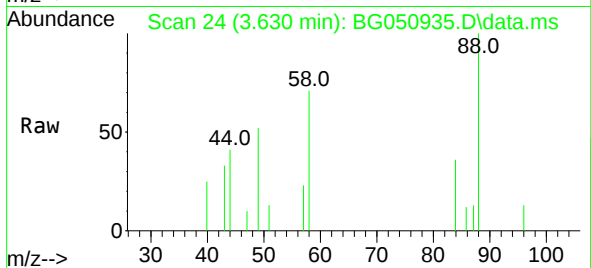

Tgt Ion:	88	Resp:	3079
Ion	Ratio	Lower	Upper
88	100		
43	32.6	23.0	34.4
58	71.1	62.4	93.6

