

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050936.D
 Acq On : 10 Nov 2021 10:06
 Operator : CG/JU
 Sample : M4532-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB8E9

Quant Time: Nov 10 10:43:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 14:49:05 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.229	152	38089	20.000	ng/u1	0.00
20) Naphthalene-d8	11.055	136	172072	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.851	164	114943	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.595	188	259499	20.000	ng/u1	-0.01
79) Chrysene-d12	21.890	240	226850	20.000	ng/u1	-0.02
88) Perylene-d12	25.292	264	225760	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.588	96	5282	4.476	ng/uL	0.00
4) Pyridine-d5	4.017	84	28264	8.006	ng/u1	0.00
7) Phenol-d5	7.371	99	25444	6.262	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.542	67	71636	27.291	ng/u1	0.00
11) 2-Chlorophenol-d4	7.753	132	58997	20.950	ng/u1	-0.01
15) 4-Methylphenol-d8	8.928	113	43659	13.648	ng/u1	0.00
21) Nitrobenzene-d5	9.404	128	39615	27.091	ng/u1	0.00
24) 2-Nitrophenol-d4	10.127	143	42546	26.167	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.668	165	63040	23.017	ng/u1	0.00
31) 4-Chloroaniline-d4	11.185	131	68026	16.401	ng/u1	0.00
46) Dimethylphthalate-d6	14.246	166	273138	31.060	ng/u1	0.00
49) Acenaphthylene-d8	14.551	160	323688	29.544	ng/u1	0.00
54) 4-Nitrophenol-d4	15.045	143	8697	5.454	ng/u1	0.00
60) Fluorene-d10	15.838	176	245425	31.505	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.955	200	40199	25.551	ng/u1	0.00
73) Anthracene-d10	17.695	188	423463	34.515	ng/u1	-0.01
81) Pyrene-d10	19.974	212	485979	33.168	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.057	264	410535	32.894	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.623	88	43837	33.820	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050936.D
Acq On : 10 Nov 2021 10:06
Operator : CG/JU
Sample : M4532-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8E9


Quant Time: Nov 10 10:43:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 14:49:05 2021
Response via : Initial Calibration

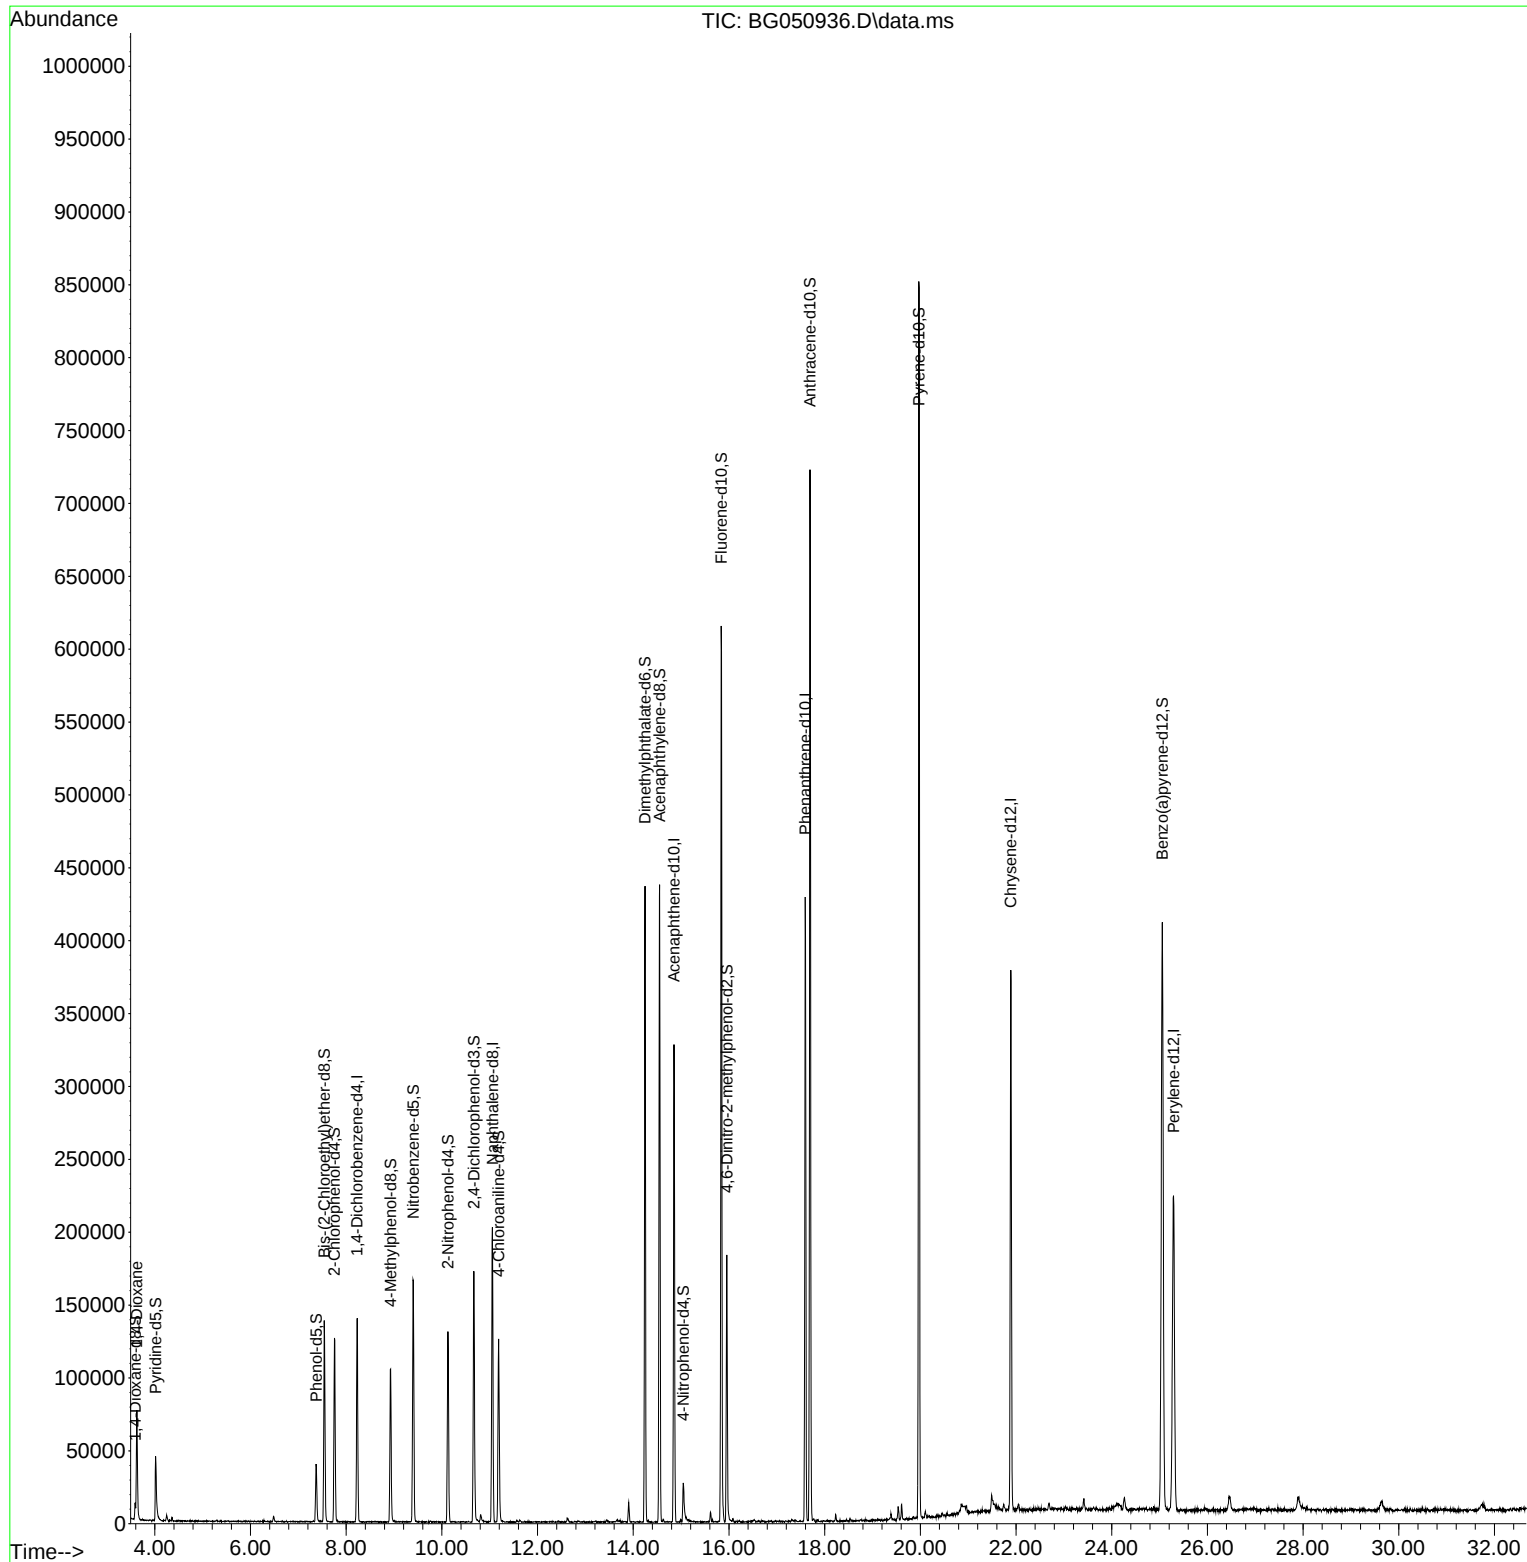

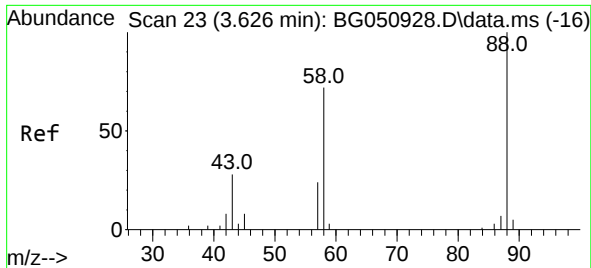

#2
 1,4-Dioxane
 Concen: 33.820 ng/uL
 RT: 3.623 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BG050936.D
 Acq: 10 Nov 2021 10:06

Instrument :
 BNA_G
 ClientSampleId :
 GB8E9

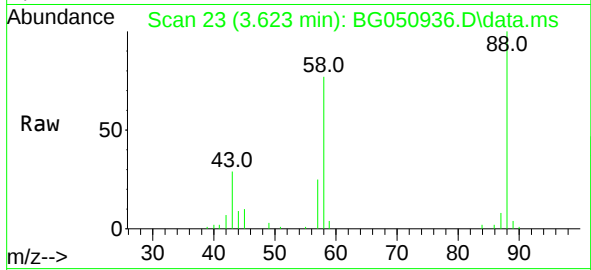

Tgt Ion: 88 Resp: 43837

Ion	Ratio	Lower	Upper
88	100		
43	29.1	23.0	34.4
58	77.4	62.4	93.6

