

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050946.D
 Acq On : 10 Nov 2021 16:57
 Operator : CG/JU
 Sample : M4532-12DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB8E9DL

Quant Time: Nov 10 17:30:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 14:49:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.230	152	39889	20.000	ng/u1	0.00
20) Naphthalene-d8	11.050	136	178130	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.852	164	120580	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.596	188	265522	20.000	ng/u1	-0.01
79) Chrysene-d12	21.890	240	234060	20.000	ng/u1	-0.02
88) Perylene-d12	25.287	264	225490	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.588	96	3195	2.585	ng/uL	0.00
4) Pyridine-d5	4.023	84	16102	4.355	ng/u1	0.00
7) Phenol-d5	7.372	99	14049	3.301	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.543	67	39163	14.247	ng/u1	0.00
11) 2-Chlorophenol-d4	7.754	132	31106	10.547	ng/u1	-0.01
15) 4-Methylphenol-d8	8.929	113	23039	6.877	ng/u1	0.00
21) Nitrobenzene-d5	9.399	128	21655	14.305	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.128	143	21616	12.842	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.668	165	34048	12.009	ng/u1	0.00
31) 4-Chloroaniline-d4	11.185	131	35887	8.358	ng/u1	0.00
46) Dimethylphthalate-d6	14.241	166	150223	16.284	ng/u1	-0.01
49) Acenaphthylene-d8	14.546	160	177306	15.427	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.057	143	3753	2.244	ng/u1	0.01
60) Fluorene-d10	15.839	176	135350	16.562	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.956	200	16776	10.421	ng/u1	0.00
73) Anthracene-d10	17.690	188	231774	18.463	ng/u1	-0.02
81) Pyrene-d10	19.969	212	266780	17.647	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.046	264	218417	17.522	ng/u1	-0.03
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.624	88	24461	18.020	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050946.D
Acq On : 10 Nov 2021 16:57
Operator : CG/JU
Sample : M4532-12DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8E9DL


Quant Time: Nov 10 17:30:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 14:49:05 2021
Response via : Initial Calibration

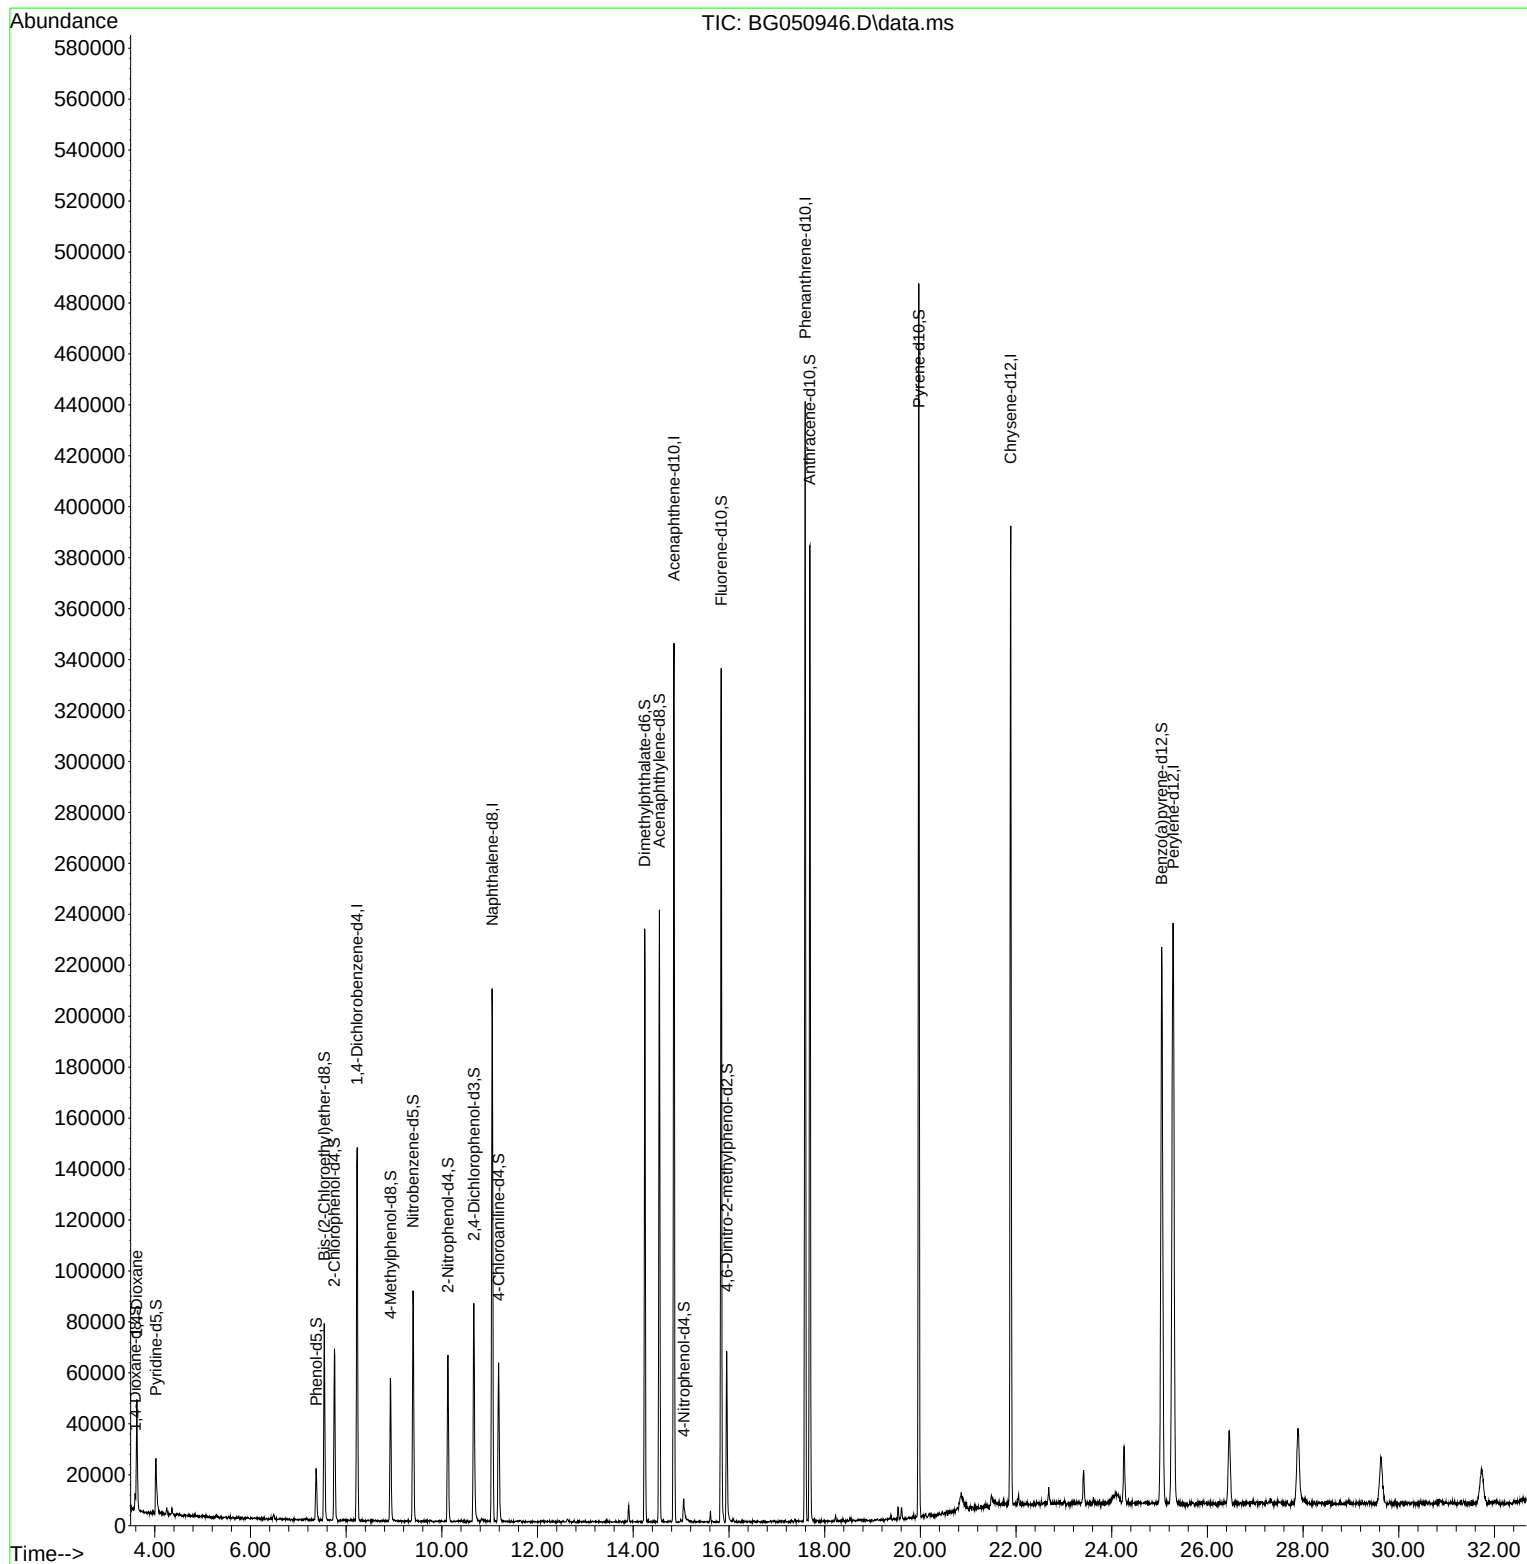

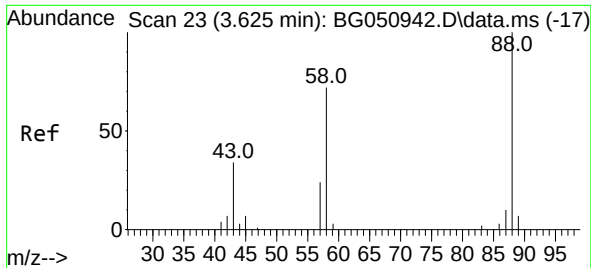

#2
 1,4-Dioxane
 Concen: 18.020 ng/uL
 RT: 3.624 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BG050946.D
 Acq: 10 Nov 2021 16:57

Instrument :
 BNA_G
 ClientSampleId :
 GB8E9DL

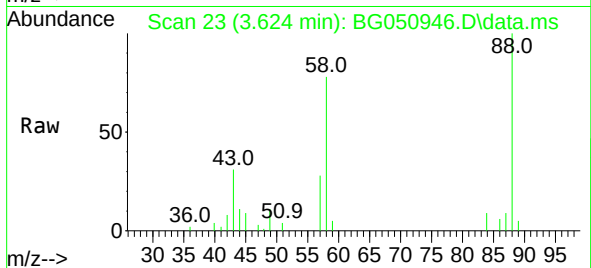

Tgt Ion:	88	Resp:	24461
Ion	Ratio	Lower	Upper
88	100		
43	30.9	23.0	34.4
58	78.0	62.4	93.6

