

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050877.D
 Acq On : 8 Nov 2021 12:49
 Operator : CG/JU
 Sample : PB140507BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK507

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.590	12	17	23	rBV	10287	16724	1.77%	0.163%
2	4.013	84	89	109	rBV	124415	227699	24.09%	2.221%
3	4.219	122	124	127	rVB2	942	1044	0.11%	0.010%
4	4.260	127	131	132	rBV2	830	1132	0.12%	0.011%
5	4.360	144	148	154	rVB3	2401	3818	0.40%	0.037%
6	7.374	653	661	673	rBV	141137	259419	27.45%	2.530%
7	7.544	684	690	699	rVB	118806	203633	21.54%	1.986%
8	7.756	718	726	738	rBV	141978	245961	26.02%	2.399%
9	8.232	800	807	815	rBV	133051	224738	23.78%	2.192%
10	8.925	918	925	938	rBV	168695	306926	32.47%	2.993%
11	9.401	999	1006	1014	rBV	145704	258809	27.38%	2.524%
12	10.130	1123	1130	1140	rVB	116406	206359	21.83%	2.013%
13	10.670	1214	1222	1236	rBV	148229	287277	30.39%	2.802%
14	11.058	1279	1288	1296	rBB	186631	342390	36.23%	3.339%
15	11.187	1302	1310	1324	rBV	164571	319814	33.84%	3.119%
16	12.627	1551	1555	1563	rVB4	1986	3837	0.41%	0.037%
17	14.248	1824	1831	1839	rBV	326819	498513	52.74%	4.862%
18	14.548	1875	1882	1895	rVB	360727	588225	62.23%	5.737%
19	14.854	1924	1934	1943	rBV	306499	482808	51.08%	4.709%
20	15.042	1960	1966	1979	rBV	103946	208915	22.10%	2.038%
21	15.841	2095	2102	2110	rBV	460663	726650	76.88%	7.087%
22	15.958	2116	2122	2133	rBV	114954	185292	19.60%	1.807%
23	16.082	2141	2143	2146	rVB2	1700	1236	0.13%	0.012%
24	17.392	2362	2366	2369	rVB3	1332	1666	0.18%	0.016%
25	17.597	2394	2401	2408	rBV	386411	593679	62.81%	5.790%
26	17.697	2411	2418	2431	rVV	547399	830252	87.84%	8.098%
27	19.342	2691	2698	2699	rBV3	954	1131	0.12%	0.011%
28	19.542	2726	2732	2738	rBV4	6296	9375	0.99%	0.091%
29	19.613	2739	2744	2748	rVB	6437	9308	0.98%	0.091%
30	19.971	2798	2805	2816	rBV	645938	945168	100.00%	9.218%
31	20.147	2829	2835	2837	rBV3	787	1387	0.15%	0.014%
32	20.324	2863	2865	2866	rBV2	1335	1232	0.13%	0.012%
33	20.465	2885	2889	2891	rBV3	1480	1837	0.19%	0.018%
34	20.576	2905	2908	2911	rBV4	1328	1645	0.17%	0.016%
35	20.835	2950	2952	2953	rBV2	1337	964	0.10%	0.009%
36	20.876	2958	2959	2960	rBV	1516	964	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050877.D
 Acq On : 8 Nov 2021 12:49
 Operator : CG/JU
 Sample : PB140507BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK507

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	21.234	3018	3020	3021	rVB2	1508	1009	0.11%	0.010%
38	21.293	3028	3030	3033	rBV3	1536	1776	0.19%	0.017%
39	21.387	3045	3046	3050	rBV4	1516	1974	0.21%	0.019%
40	21.487	3061	3063	3067	rVB5	2222	1877	0.20%	0.018%

41	21.892	3125	3132	3141	rBV2	332157	584882	61.88%	5.704%
42	22.198	3182	3184	3186	rVB2	1921	1294	0.14%	0.013%
43	22.245	3190	3192	3194	rBV3	1590	1028	0.11%	0.010%
44	22.744	3275	3277	3279	rBV3	1972	1977	0.21%	0.019%
45	22.903	3302	3304	3305	rBV2	1362	960	0.10%	0.009%

46	23.173	3348	3350	3353	rBV4	2134	1996	0.21%	0.019%
47	23.420	3387	3392	3397	rBV6	6535	12551	1.33%	0.122%
48	23.637	3427	3429	3432	rBV4	2048	1985	0.21%	0.019%
49	24.237	3528	3531	3532	rBV3	2942	3048	0.32%	0.030%
50	24.272	3532	3537	3546	rVB6	8944	21219	2.24%	0.207%

51	24.619	3594	3596	3598	rBV3	1912	1412	0.15%	0.014%
52	24.736	3614	3616	3618	rBV2	2060	1688	0.18%	0.016%
53	25.059	3661	3671	3685	rVB2	285725	839163	88.78%	8.184%
54	25.294	3699	3711	3725	rVB3	199490	613925	64.95%	5.988%
55	25.647	3769	3771	3774	rBV4	2103	2032	0.21%	0.020%

56	25.706	3779	3781	3783	rBV2	2997	1278	0.14%	0.012%
57	25.847	3803	3805	3808	rBV4	2410	2051	0.22%	0.020%
58	25.876	3808	3810	3811	rVB2	1826	1174	0.12%	0.011%
59	26.170	3858	3860	3862	rBV2	1779	1495	0.16%	0.015%
60	26.475	3904	3912	3921	rVB7	11846	36355	3.85%	0.355%

61	26.663	3942	3944	3946	rBV3	1517	1255	0.13%	0.012%
62	26.804	3966	3968	3969	rBV2	1656	1392	0.15%	0.014%
63	26.939	3990	3991	3994	rBV2	1860	1191	0.13%	0.012%
64	27.027	4004	4006	4008	rBV3	1581	1258	0.13%	0.012%
65	27.127	4021	4023	4024	rBV	1623	996	0.11%	0.010%

66	27.274	4046	4048	4050	rBV2	1500	1507	0.16%	0.015%
67	27.915	4147	4157	4169	rBV6	12178	44488	4.71%	0.434%
68	28.273	4216	4218	4221	rBV4	1637	1540	0.16%	0.015%
69	28.508	4256	4258	4260	rVB3	2059	1372	0.15%	0.013%
70	28.614	4275	4276	4278	rBV2	1717	1136	0.12%	0.011%

71	28.796	4305	4307	4309	rVB2	1963	1275	0.13%	0.012%
72	29.278	4387	4389	4390	rBV	1852	1268	0.13%	0.012%
73	29.401	4409	4410	4412	rBV2	2302	1468	0.16%	0.014%
74	29.472	4420	4422	4425	rBV4	1680	1521	0.16%	0.015%
75	29.589	4440	4442	4443	rBV2	1876	1246	0.13%	0.012%

76	29.648	4443	4452	4461	rVV2	9326	33442	3.54%	0.326%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050877.D
 Acq On : 8 Nov 2021 12:49
 Operator : CG/JU
 Sample : PB140507BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK507

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

77	29.824	4480	4482	4485	rBV4	1874	1660	0.18%	0.016%
78	29.953	4502	4504	4505	rBV2	2442	1554	0.16%	0.015%
79	30.612	4614	4616	4617	rVB2	2302	1225	0.13%	0.012%
80	30.823	4650	4652	4655	rBV3	1742	1273	0.13%	0.012%
81	30.882	4658	4662	4666	rBV7	2635	3592	0.38%	0.035%
82	31.070	4692	4694	4697	rVB4	1448	1111	0.12%	0.011%
83	31.481	4762	4764	4766	rBV3	1748	1298	0.14%	0.013%
84	31.657	4793	4794	4795	rBV	2034	1012	0.11%	0.010%
85	31.710	4801	4803	4806	rBV3	2847	3776	0.40%	0.037%
86	32.527	4940	4942	4943	rBV2	2295	1282	0.14%	0.013%
87	32.633	4959	4960	4961	rBV	1961	1011	0.11%	0.010%




Sum of corrected areas: 10253125

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050877.D
Acq On : 8 Nov 2021 12:49
Operator : CG/JU
Sample : PB140507BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK507

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

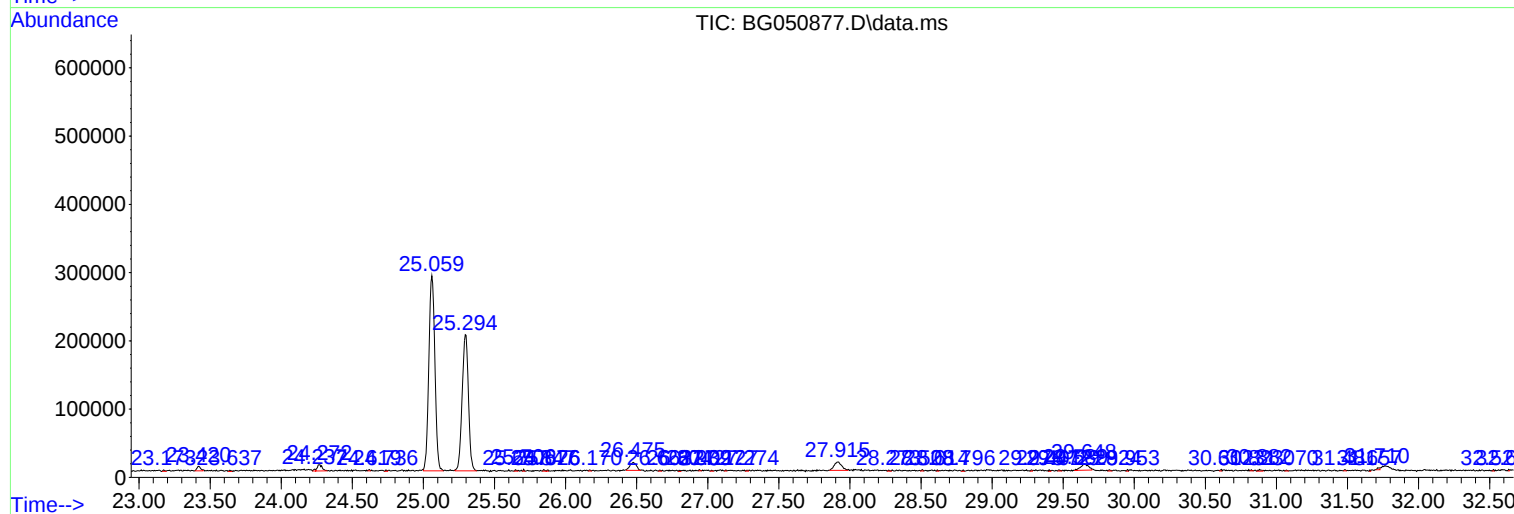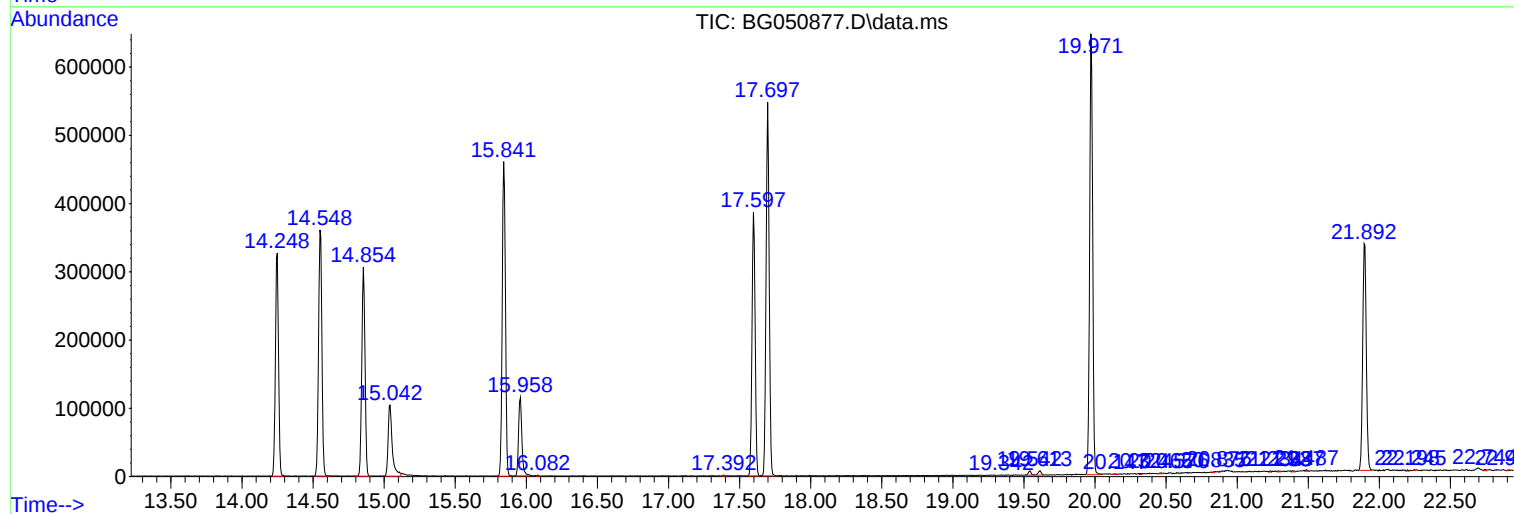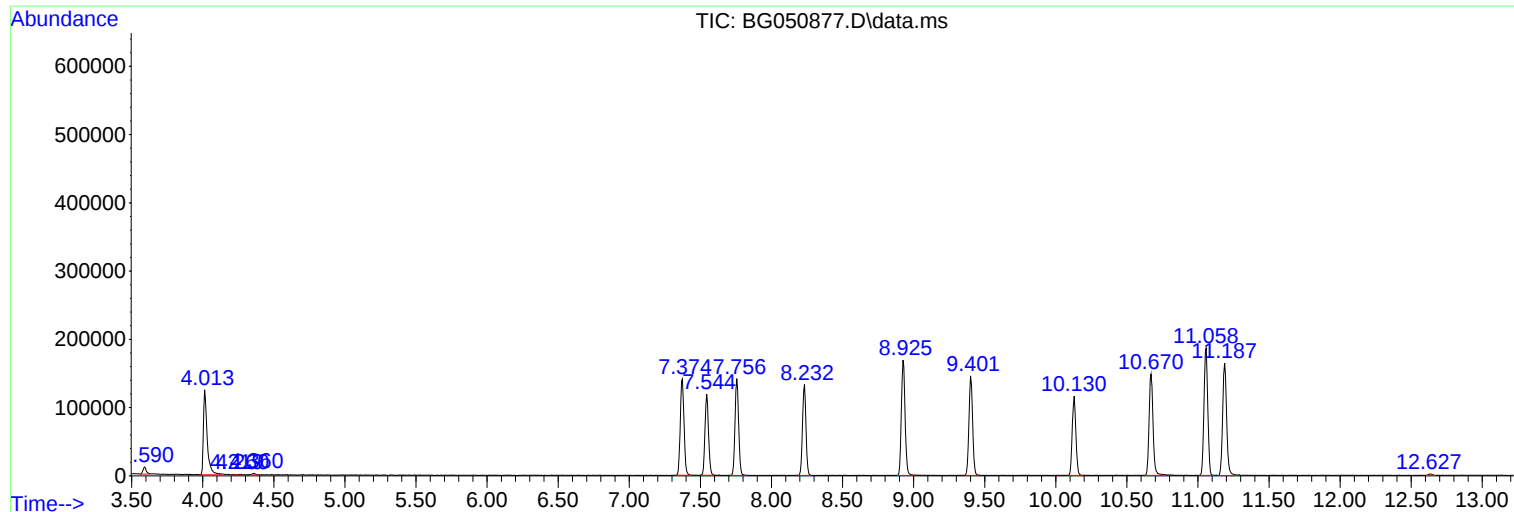

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050877.D
Acq On : 8 Nov 2021 12:49
Operator : CG/JU
Sample : PB140507BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK507

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050877.D
Acq On : 8 Nov 2021 12:49
Operator : CG/JU
Sample : PB140507BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK507

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
