

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050886.D
 Acq On : 8 Nov 2021 18:57
 Operator : CG/JU
 Sample : M4492-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG1S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	13	17	27	rVB	10927	18478	1.43%	0.165%
2	4.022	87	91	106	rBV	38066	78609	6.08%	0.703%
3	4.251	126	130	136	rVB2	4677	7387	0.57%	0.066%
4	4.357	144	148	153	rBV	2731	3880	0.30%	0.035%
5	5.291	304	307	312	rBV4	2117	3456	0.27%	0.031%
6	7.371	654	661	671	rBV2	38521	72124	5.58%	0.645%
7	7.541	683	690	701	rVB	134624	231008	17.86%	2.067%
8	7.758	719	727	736	rVV	125877	225299	17.42%	2.016%
9	8.228	797	807	814	rBV	141717	244736	18.92%	2.190%
10	8.928	919	926	933	rBV	103246	183751	14.20%	1.644%
11	9.404	999	1007	1014	rBV	159303	297359	22.99%	2.661%
12	9.762	1062	1068	1072	rBV4	1455	2222	0.17%	0.020%
13	10.126	1121	1130	1139	rBV	124700	230172	17.79%	2.060%
14	10.667	1213	1222	1232	rBV2	163051	306143	23.67%	2.740%
15	11.055	1280	1288	1297	rVB	192451	355560	27.49%	3.182%
16	11.184	1300	1310	1322	rBV	160993	315093	24.36%	2.820%
17	12.629	1551	1556	1564	rVB	2560	4228	0.33%	0.038%
18	13.652	1725	1730	1735	rVB3	1582	2450	0.19%	0.022%
19	14.245	1824	1831	1838	rBV	382721	564930	43.67%	5.056%
20	14.550	1876	1883	1891	rBV	411714	662718	51.23%	5.931%
21	14.850	1927	1934	1943	rVB	317038	492233	38.05%	4.405%
22	15.044	1961	1967	1979	rBV2	21192	49413	3.82%	0.442%
23	15.837	2095	2102	2110	rBV	559519	877802	67.86%	7.856%
24	15.955	2116	2122	2140	rBV	163095	270250	20.89%	2.419%
25	16.078	2140	2143	2144	rVV3	2109	1903	0.15%	0.017%
26	17.312	2351	2353	2355	rBV2	1719	1406	0.11%	0.013%
27	17.594	2395	2401	2409	rVB	405074	616306	47.64%	5.515%
28	17.694	2411	2418	2427	rVV2	707271	1106064	85.50%	9.898%
29	17.770	2427	2431	2435	rVV5	7344	9873	0.76%	0.088%
30	17.841	2439	2443	2446	rBV3	896	1626	0.13%	0.015%
31	18.229	2504	2509	2513	rBV4	4072	5313	0.41%	0.048%
32	18.769	2597	2601	2603	rBV2	1208	1492	0.12%	0.013%
33	19.104	2652	2658	2659	rBV3	855	1344	0.10%	0.012%
34	19.386	2699	2706	2711	rBV5	2912	5045	0.39%	0.045%
35	19.533	2725	2731	2735	rBV3	8817	13555	1.05%	0.121%
36	19.609	2738	2744	2752	rVB	9279	13929	1.08%	0.125%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050886.D
 Acq On : 8 Nov 2021 18:57
 Operator : CG/JU
 Sample : M4492-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG1S5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	19.715	2759	2762	2765	rVB2	1382	1336	0.10%	0.012%
38	19.786	2770	2774	2776	rBV3	1114	1475	0.11%	0.013%
39	19.968	2797	2805	2814	rBV	887809	1293635	100.00%	11.577%
40	20.120	2827	2831	2832	rBV4	1571	1323	0.10%	0.012%
41	20.214	2843	2847	2848	rBV3	1253	1717	0.13%	0.015%
42	20.391	2873	2877	2879	rBV4	1204	1604	0.12%	0.014%
43	20.461	2882	2889	2890	rBV5	3547	4979	0.38%	0.045%
44	20.596	2909	2912	2914	rVB4	1600	1513	0.12%	0.014%
45	20.955	2972	2973	2978	rVB4	2571	3296	0.25%	0.029%
46	21.031	2984	2986	2987	rBV2	1562	1492	0.12%	0.013%
47	21.266	3024	3026	3028	rBV3	1605	1361	0.11%	0.012%
48	21.489	3060	3064	3068	rBV4	9364	18796	1.45%	0.168%
49	21.707	3099	3101	3104	rBV4	1265	1471	0.11%	0.013%
50	21.742	3104	3107	3112	rVB7	4340	6934	0.54%	0.062%
51	21.889	3125	3132	3142	rBV2	370053	615420	47.57%	5.507%
52	22.112	3168	3170	3172	rBV3	1664	1832	0.14%	0.016%
53	22.159	3177	3178	3180	rBV2	1786	1347	0.10%	0.012%
54	22.241	3191	3192	3194	rBV2	1932	1393	0.11%	0.012%
55	22.553	3243	3245	3248	rBV4	1865	1961	0.15%	0.018%
56	22.929	3307	3309	3313	rBV5	1811	2360	0.18%	0.021%
57	23.046	3327	3329	3330	rBV2	1880	1295	0.10%	0.012%
58	23.346	3378	3380	3382	rBV3	2370	1359	0.11%	0.012%
59	23.411	3389	3391	3395	rVB5	5008	6056	0.47%	0.054%
60	23.493	3403	3405	3407	rBV3	1428	1368	0.11%	0.012%
61	24.257	3531	3535	3542	rVB6	8883	18292	1.41%	0.164%
62	25.050	3659	3670	3685	rBV2	393257	1157560	89.48%	10.359%
63	25.285	3698	3710	3724	rBV3	204683	632541	48.90%	5.661%
64	25.643	3769	3771	3773	rVB4	1966	1313	0.10%	0.012%
65	25.731	3784	3786	3787	rBV	3347	1609	0.12%	0.014%
66	25.749	3787	3789	3791	rVV3	1913	1906	0.15%	0.017%
67	26.143	3854	3856	3861	rVB4	2845	2851	0.22%	0.026%
68	26.260	3874	3876	3881	rVB4	1866	2597	0.20%	0.023%
69	26.466	3904	3911	3922	rVB8	10011	32601	2.52%	0.292%
70	26.795	3963	3967	3970	rBV6	2085	3997	0.31%	0.036%
71	27.665	4113	4115	4118	rVB4	1989	1441	0.11%	0.013%
72	27.782	4134	4135	4140	rBV5	2096	3023	0.23%	0.027%
73	27.894	4144	4154	4164	rVV7	10925	37357	2.89%	0.334%
74	28.082	4184	4186	4188	rBV3	1776	1711	0.13%	0.015%
75	28.276	4218	4219	4222	rBV3	2746	2844	0.22%	0.025%
76	28.569	4267	4269	4271	rVB3	2109	1612	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050886.D
Acq On : 8 Nov 2021 18:57
Operator : CG/JU
Sample : M4492-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG1S5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION

77	29.744	4468	4469	4471	rBV2	1593	1296	0.10%	0.012%
78	29.921	4497	4499	4500	rBV2	2355	1627	0.13%	0.015%
79	30.144	4533	4537	4539	rBV5	2296	2154	0.17%	0.019%
80	31.049	4689	4691	4694	rBV4	2109	2519	0.19%	0.023%
81	31.301	4732	4734	4735	rBV2	2409	2106	0.16%	0.019%
82	31.372	4744	4746	4750	rBV4	1486	1991	0.15%	0.018%
83	31.425	4753	4755	4756	rVV2	2532	1449	0.11%	0.013%
84	31.707	4801	4803	4804	rBV2	2274	1515	0.12%	0.014%
85	32.453	4926	4930	4931	rBV3	1814	1920	0.15%	0.017%
86	32.541	4944	4945	4948	rBV3	1651	1910	0.15%	0.017%




Sum of corrected areas: 11174222

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050886.D
Acq On : 8 Nov 2021 18:57
Operator : CG/JU
Sample : M4492-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG1S5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

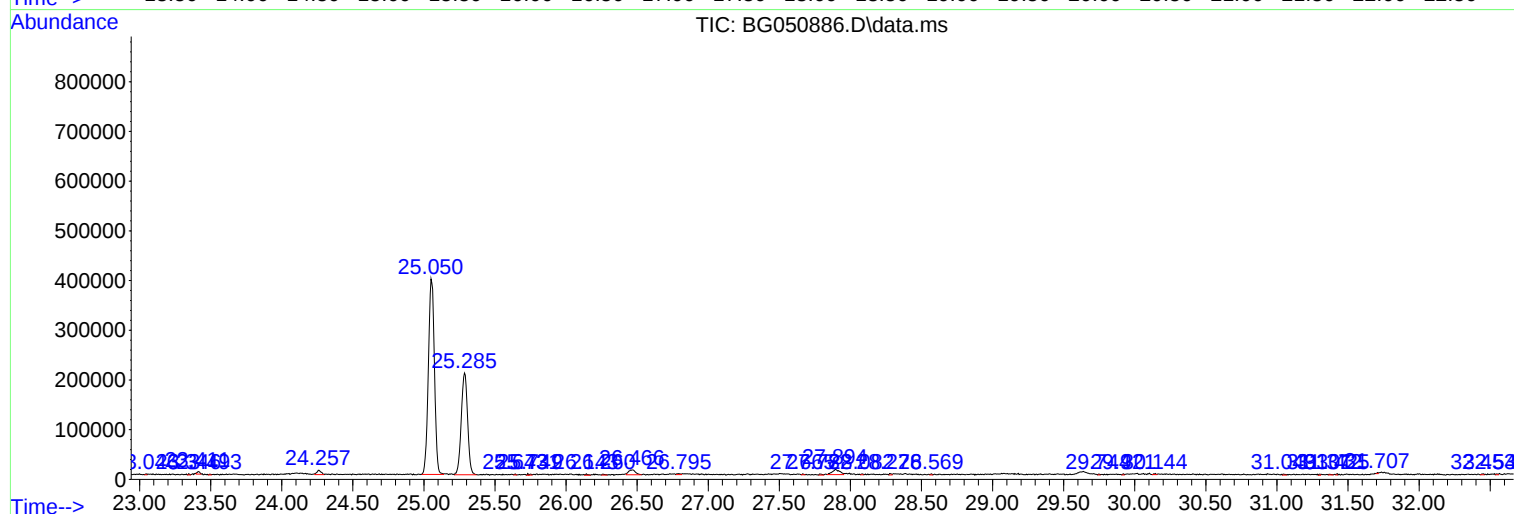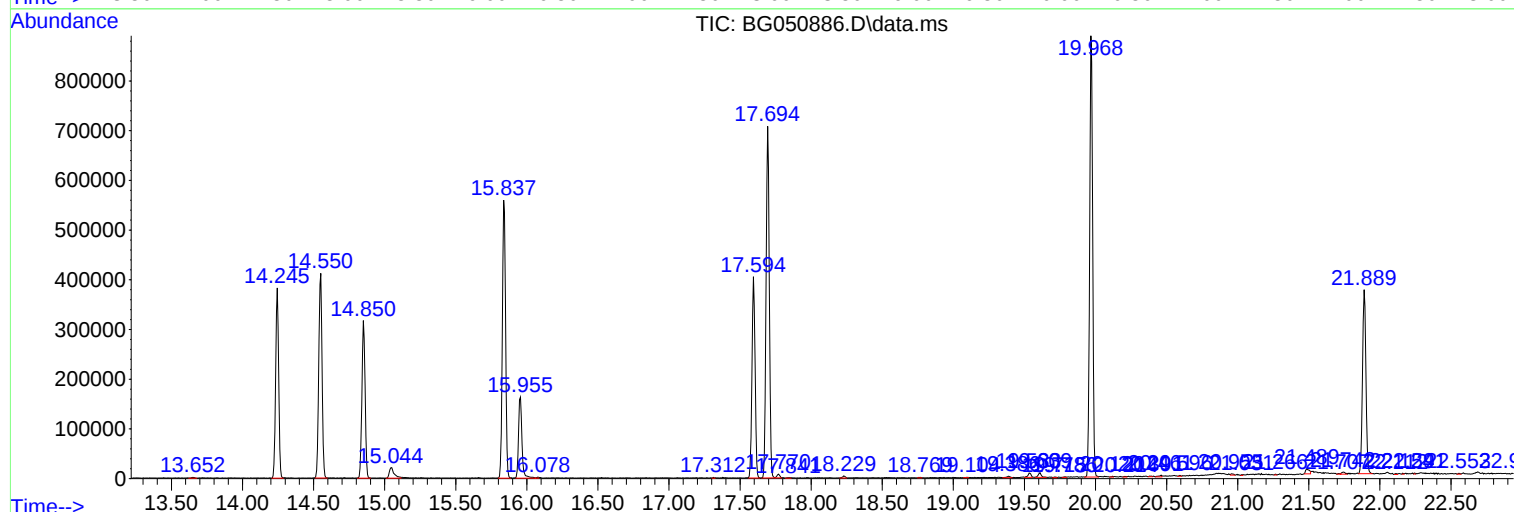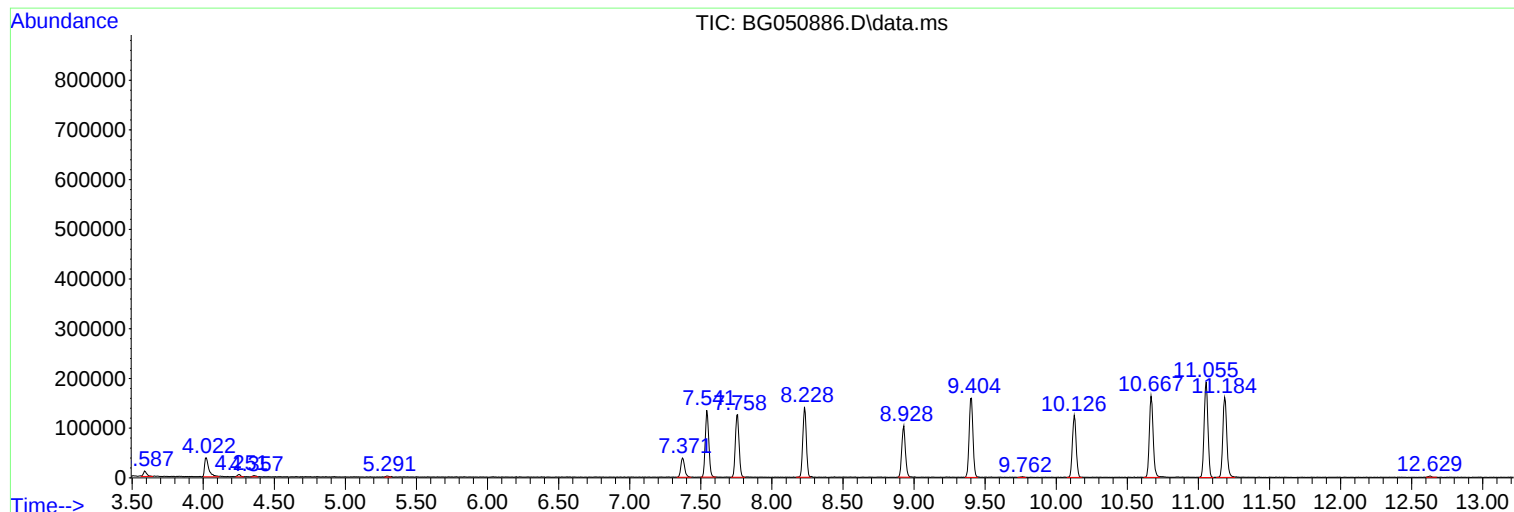

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050886.D
Acq On : 8 Nov 2021 18:57
Operator : CG/JU
Sample : M4492-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG1S5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050886.D
Acq On : 8 Nov 2021 18:57
Operator : CG/JU
Sample : M4492-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG1S5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc