

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050892.D
 Acq On : 8 Nov 2021 23:46
 Operator : CG/JU
 Sample : PB140481BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK481

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.593	13	18	26	rVB2	12985	21021	1.89%	0.178%
2	3.922	72	74	77	rBV2	886	1159	0.10%	0.010%
3	4.010	85	89	109	rVV	152229	291439	26.23%	2.474%
4	4.363	144	149	154	rBV3	2627	3918	0.35%	0.033%
5	7.371	653	661	672	rBV	186357	328818	29.59%	2.791%
6	7.541	683	690	702	rBV	145641	255591	23.00%	2.170%
7	7.753	719	726	736	rVB	173954	307222	27.65%	2.608%
8	8.229	800	807	817	rVB	137963	239808	21.58%	2.036%
9	8.922	918	925	934	rBV	213052	383424	34.50%	3.255%
10	9.398	999	1006	1016	rBV	174198	320512	28.84%	2.721%
11	10.127	1122	1130	1138	rBV	145161	267032	24.03%	2.267%
12	10.667	1214	1222	1236	rBV	192331	360864	32.47%	3.063%
13	11.055	1279	1288	1297	rBV	193588	354291	31.88%	3.007%
14	11.184	1303	1310	1326	rBV	206339	398311	35.84%	3.381%
15	12.630	1552	1556	1563	rVB2	2899	5480	0.49%	0.047%
16	14.245	1824	1831	1844	rVB	402569	601710	54.15%	5.108%
17	14.545	1875	1882	1890	rBV	440466	718340	64.64%	6.098%
18	14.851	1926	1934	1942	rVB	320567	499256	44.93%	4.238%
19	15.039	1959	1966	1976	rBV	136051	256057	23.04%	2.174%
20	15.127	1980	1981	1983	rVB	1578	1203	0.11%	0.010%
21	15.838	2095	2102	2110	rBV	560290	878161	79.02%	7.454%
22	15.955	2116	2122	2137	rBV	150674	240803	21.67%	2.044%
23	16.078	2140	2143	2149	rVB	2521	3700	0.33%	0.031%
24	17.383	2361	2365	2366	rBV	1884	1338	0.12%	0.011%
25	17.400	2366	2368	2376	rVB2	1060	1621	0.15%	0.014%
26	17.594	2394	2401	2411	rBV	401678	605358	54.48%	5.139%
27	17.694	2411	2418	2429	rVB	640945	975023	87.74%	8.277%
28	19.539	2727	2732	2737	rVV2	8436	12006	1.08%	0.102%
29	19.610	2739	2744	2752	rVB2	7068	11250	1.01%	0.095%
30	19.798	2774	2776	2778	rVB3	1152	1161	0.10%	0.010%
31	19.915	2791	2796	2799	rVV5	1105	1435	0.13%	0.012%
32	19.968	2799	2805	2815	rVV	762975	1111257	100.00%	9.433%
33	20.068	2819	2822	2824	rBV4	1206	1333	0.12%	0.011%
34	20.221	2846	2848	2851	rBV2	953	1494	0.13%	0.013%
35	20.362	2870	2872	2875	rVB3	1971	2228	0.20%	0.019%
36	20.556	2903	2905	2909	rVB4	2255	2504	0.23%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050892.D
 Acq On : 8 Nov 2021 23:46
 Operator : CG/JU
 Sample : PB140481BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK481

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	20.591	2909	2911	2914	rBV4	1979	2196	0.20%	0.019%
38	20.791	2941	2945	2946	rBV4	1282	1469	0.13%	0.012%
39	20.832	2950	2952	2953	rBV	2351	1913	0.17%	0.016%
40	20.843	2953	2954	2955	rBV	2611	1797	0.16%	0.015%
41	21.108	2997	2999	3001	rBV3	1310	1167	0.11%	0.010%
42	21.267	3025	3026	3028	rBV2	1534	1304	0.12%	0.011%
43	21.601	3082	3083	3087	rBV3	1940	1489	0.13%	0.013%
44	21.648	3089	3091	3094	rVV4	1604	1353	0.12%	0.011%
45	21.701	3098	3100	3103	rVV3	1247	1273	0.11%	0.011%
46	21.889	3125	3132	3144	rVV	348780	600941	54.08%	5.101%
47	22.148	3174	3176	3177	rBV2	1335	1235	0.11%	0.010%
48	22.212	3186	3187	3191	rBV3	1383	2002	0.18%	0.017%
49	22.483	3231	3233	3234	rBV2	1607	1231	0.11%	0.010%
50	22.688	3264	3268	3269	rBV4	2329	2081	0.19%	0.018%
51	22.841	3292	3294	3297	rBV4	1685	1759	0.16%	0.015%
52	23.241	3359	3362	3363	rBV3	1412	1614	0.15%	0.014%
53	23.417	3388	3392	3399	rVB7	4164	7543	0.68%	0.064%
54	23.722	3442	3444	3448	rBV4	1347	1685	0.15%	0.014%
55	23.769	3450	3452	3455	rBV3	1399	1488	0.13%	0.013%
56	24.087	3504	3506	3507	rBV2	1897	1443	0.13%	0.012%
57	24.104	3507	3509	3511	rBV2	2539	2918	0.26%	0.025%
58	24.269	3532	3537	3544	rVB6	6231	13429	1.21%	0.114%
59	25.056	3659	3671	3685	rVV2	348719	1001835	90.15%	8.504%
60	25.291	3699	3711	3722	rBV2	200803	605590	54.50%	5.141%
61	26.314	3883	3885	3886	rBV2	1505	1177	0.11%	0.010%
62	26.384	3895	3897	3899	rBV3	1778	1908	0.17%	0.016%
63	27.254	4043	4045	4048	rBV4	1774	1948	0.18%	0.017%
64	27.389	4067	4068	4070	rBV2	1504	1209	0.11%	0.010%
65	27.900	4145	4155	4156	rBV6	7874	15929	1.43%	0.135%
66	28.311	4223	4225	4227	rBV2	2270	2031	0.18%	0.017%
67	28.787	4304	4306	4308	rBV3	1476	1355	0.12%	0.012%
68	29.163	4368	4370	4372	rBV4	1443	1299	0.12%	0.011%
69	29.204	4375	4377	4379	rVB3	2298	1602	0.14%	0.014%
70	29.522	4429	4431	4434	rBV3	1857	1521	0.14%	0.013%
71	29.598	4441	4444	4445	rBV3	2285	2506	0.23%	0.021%
72	29.804	4478	4479	4485	rVB6	1804	2198	0.20%	0.019%
73	30.397	4576	4580	4581	rBV4	1435	2050	0.18%	0.017%
74	30.509	4597	4599	4602	rBV3	2031	2810	0.25%	0.024%
75	30.544	4602	4605	4608	rVV3	1805	2510	0.23%	0.021%
76	30.726	4635	4636	4639	rVV3	1546	1403	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050892.D
Acq On : 8 Nov 2021 23:46
Operator : CG/JU
Sample : PB140481BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK481

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION

77	30.767	4642	4643	4645	rBV2	1641	1226	0.11%	0.010%
78	31.002	4681	4683	4684	rBV2	1637	1424	0.13%	0.012%
79	31.196	4714	4716	4719	rBV4	1815	1382	0.12%	0.012%
80	31.308	4733	4735	4740	rBV5	1493	1824	0.16%	0.015%
81	31.731	4805	4807	4808	rBV2	2089	1530	0.14%	0.013%
82	32.495	4935	4937	4938	rBV2	1377	1140	0.10%	0.010%
83	32.577	4949	4951	4954	rBV4	1680	1625	0.15%	0.014%




Sum of corrected areas: 11780490

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050892.D
Acq On : 8 Nov 2021 23:46
Operator : CG/JU
Sample : PB140481BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK481

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

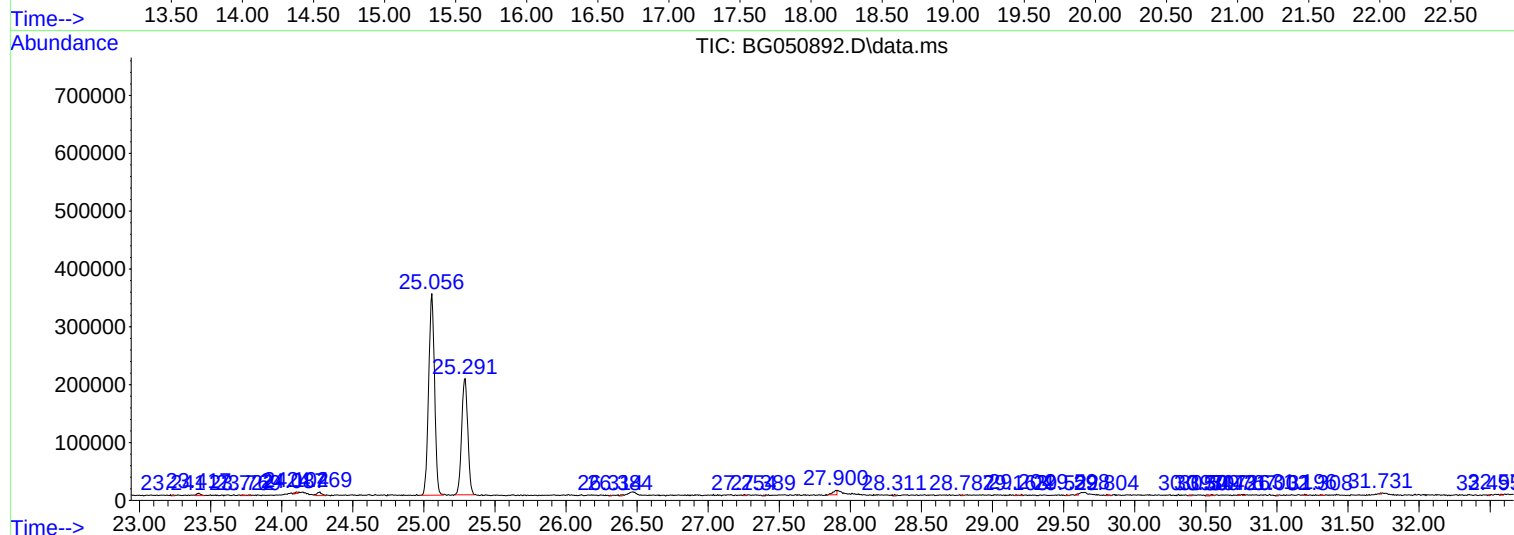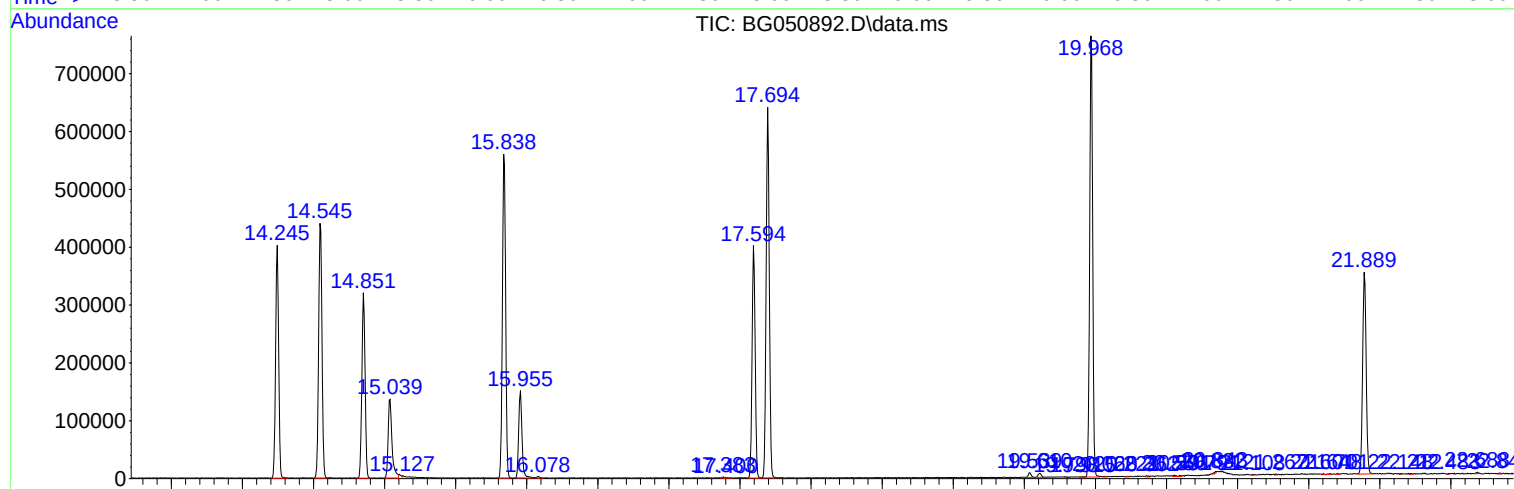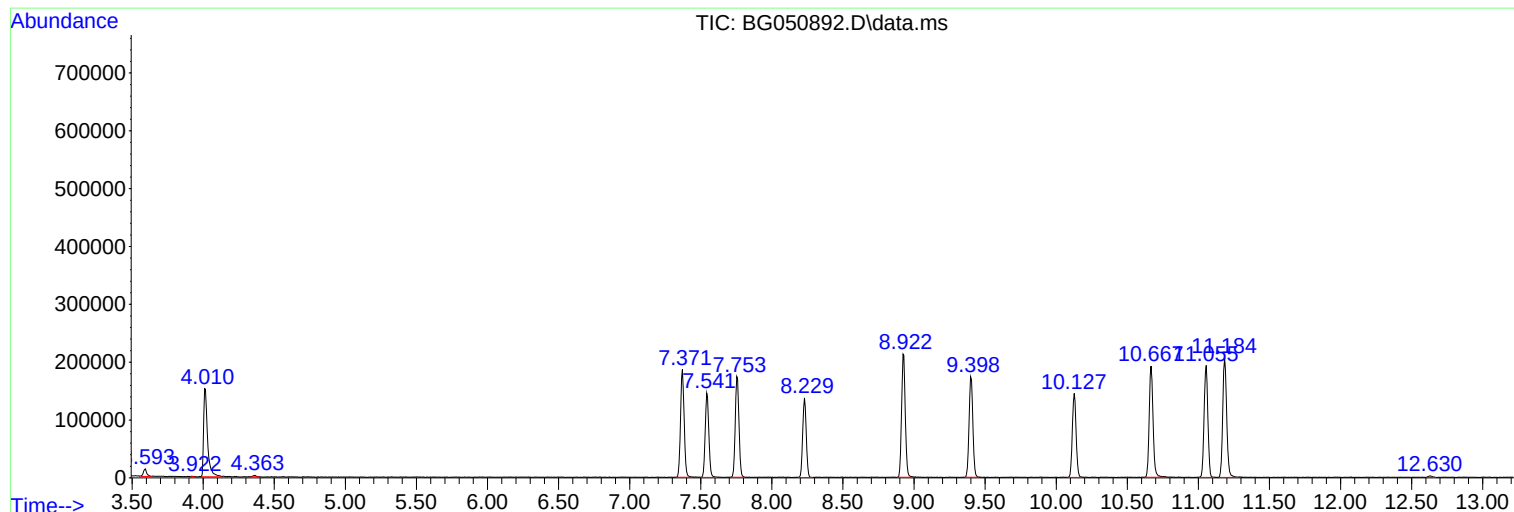

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050892.D
Acq On : 8 Nov 2021 23:46
Operator : CG/JU
Sample : PB140481BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK481

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050892.D
Acq On : 8 Nov 2021 23:46
Operator : CG/JU
Sample : PB140481BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK481

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc