

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050918.D
 Acq On : 9 Nov 2021 21:03
 Operator : CG/JU
 Sample : M4490-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.343	143	145	146	rBV	1523	1039	0.19%	0.038%
2	4.819	224	226	227	rBV2	1016	839	0.15%	0.031%
3	4.983	252	254	258	rBV3	967	906	0.16%	0.033%
4	5.130	277	279	281	rBV2	1129	890	0.16%	0.032%
5	5.435	330	331	333	rBV	1173	751	0.13%	0.027%
6	5.618	361	362	365	rBV3	1071	1003	0.18%	0.037%
7	6.211	461	463	465	rVB2	912	663	0.12%	0.024%
8	6.452	502	504	507	rVB3	913	806	0.14%	0.029%
9	6.757	553	556	557	rBV2	681	754	0.13%	0.027%
10	7.997	765	767	771	rVB3	565	795	0.14%	0.029%
11	8.226	800	806	816	rBV	125789	222939	39.72%	8.124%
12	8.297	816	818	821	rVB3	835	860	0.15%	0.031%
13	8.767	895	898	900	rBV3	613	973	0.17%	0.035%
14	8.943	924	928	931	rVB3	513	793	0.14%	0.029%
15	9.014	938	940	941	rBV2	853	669	0.12%	0.024%
16	9.143	959	962	965	rVB4	592	892	0.16%	0.033%
17	9.172	965	967	970	rBV2	724	836	0.15%	0.030%
18	9.196	970	971	974	rBV3	720	689	0.12%	0.025%
19	9.301	987	989	992	rVB3	631	726	0.13%	0.026%
20	9.325	992	993	998	rBV3	584	830	0.15%	0.030%
21	9.595	1035	1039	1041	rBV3	796	889	0.16%	0.032%
22	9.819	1075	1077	1081	rVB2	909	798	0.14%	0.029%
23	10.112	1123	1127	1128	rVB3	706	812	0.14%	0.030%
24	10.136	1128	1131	1133	rBV3	545	732	0.13%	0.027%
25	10.183	1136	1139	1141	rBV2	583	739	0.13%	0.027%
26	10.441	1178	1183	1186	rBV4	580	968	0.17%	0.035%
27	10.529	1195	1198	1204	rVB5	515	834	0.15%	0.030%
28	11.052	1280	1287	1299	rBV	172458	324897	57.89%	11.839%
29	11.282	1323	1326	1328	rVB2	765	912	0.16%	0.033%
30	11.405	1345	1347	1350	rVB	713	674	0.12%	0.025%
31	11.464	1354	1357	1359	rVB2	544	673	0.12%	0.025%
32	12.169	1472	1477	1478	rBV3	480	686	0.12%	0.025%
33	12.216	1482	1485	1487	rVB2	559	718	0.13%	0.026%
34	12.439	1520	1523	1524	rBV2	680	757	0.13%	0.028%
35	12.604	1548	1551	1553	rVB3	679	700	0.12%	0.026%
36	13.074	1629	1631	1635	rVB2	610	760	0.14%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050918.D
 Acq On : 9 Nov 2021 21:03
 Operator : CG/JU
 Sample : M4490-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	13.220	1655	1656	1661	rVB2	685	760	0.14%	0.028%
38	13.385	1683	1684	1687	rBV2	695	696	0.12%	0.025%
39	13.485	1697	1701	1704	rVB3	631	1018	0.18%	0.037%
40	14.113	1805	1808	1810	rBV2	667	676	0.12%	0.025%
41	14.149	1810	1814	1817	rBV2	733	899	0.16%	0.033%
42	14.548	1879	1882	1886	rVB3	529	649	0.12%	0.024%
43	14.619	1890	1894	1897	rVV4	461	759	0.14%	0.028%
44	14.789	1918	1923	1925	rBV	788	1049	0.19%	0.038%
45	14.848	1926	1933	1948	rVV	276439	462471	82.40%	16.852%
46	15.165	1986	1987	1991	rBV2	605	671	0.12%	0.024%
47	15.430	2030	2032	2035	rBV2	674	907	0.16%	0.033%
48	15.765	2087	2089	2092	rBV2	652	1020	0.18%	0.037%
49	15.817	2097	2098	2103	rBV3	623	1064	0.19%	0.039%
50	15.900	2108	2112	2115	rBV3	573	809	0.14%	0.029%
51	16.223	2164	2167	2170	rBV3	448	841	0.15%	0.031%
52	16.358	2187	2190	2193	rVB3	517	688	0.12%	0.025%
53	16.599	2230	2231	2234	rBV	766	693	0.12%	0.025%
54	16.740	2251	2255	2256	rBV2	659	713	0.13%	0.026%
55	17.075	2306	2312	2313	rBV2	915	1621	0.29%	0.059%
56	17.128	2319	2321	2325	rBV3	579	709	0.13%	0.026%
57	17.163	2325	2327	2330	rBV2	511	722	0.13%	0.026%
58	17.292	2346	2349	2353	rVB4	703	985	0.18%	0.036%
59	17.380	2362	2364	2369	rBV2	727	1100	0.20%	0.040%
60	17.598	2394	2401	2410	rBV	340338	554430	98.78%	20.203%
61	17.662	2410	2412	2416	rVV3	1665	1729	0.31%	0.063%
62	17.709	2418	2420	2423	rVB	901	812	0.14%	0.030%
63	18.009	2469	2471	2474	rBV2	729	675	0.12%	0.025%
64	18.074	2479	2482	2487	rBV2	649	1111	0.20%	0.040%
65	18.244	2509	2511	2515	rBV3	622	649	0.12%	0.024%
66	18.702	2585	2589	2591	rBV3	661	1140	0.20%	0.042%
67	19.260	2681	2684	2687	rVB2	585	651	0.12%	0.024%
68	19.407	2707	2709	2712	rBV3	711	778	0.14%	0.028%
69	19.578	2733	2738	2741	rBV2	838	1805	0.32%	0.066%
70	19.760	2767	2769	2771	rBV	751	723	0.13%	0.026%
71	19.977	2804	2806	2808	rVB	1103	796	0.14%	0.029%
72	20.007	2808	2811	2812	rBV3	863	1077	0.19%	0.039%
73	20.506	2894	2896	2899	rBV4	1238	1404	0.25%	0.051%
74	21.229	3017	3019	3021	rBV3	1731	1428	0.25%	0.052%
75	21.893	3125	3132	3143	rVB	322787	557089	99.25%	20.300%
76	25.283	3699	3709	3724	rVB2	182603	561280	100.00%	20.453%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050918.D
Acq On : 9 Nov 2021 21:03
Operator : CG/JU
Sample : M4490-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION




Sum of corrected areas: 2744299

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050918.D
Acq On : 9 Nov 2021 21:03
Operator : CG/JU
Sample : M4490-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

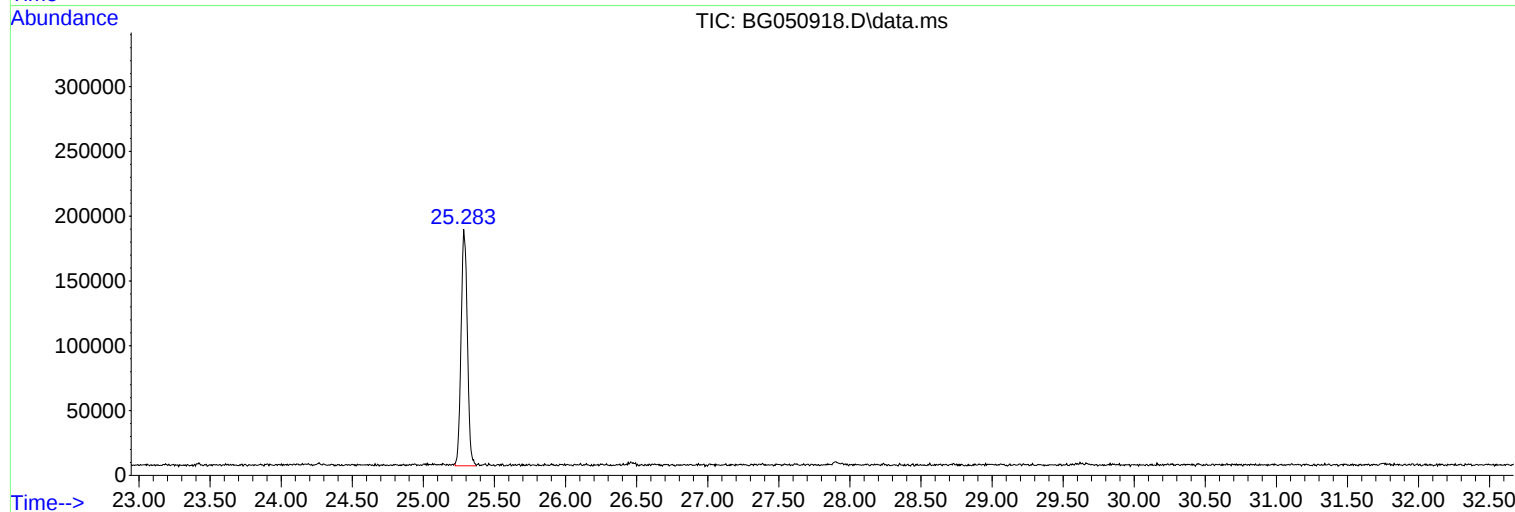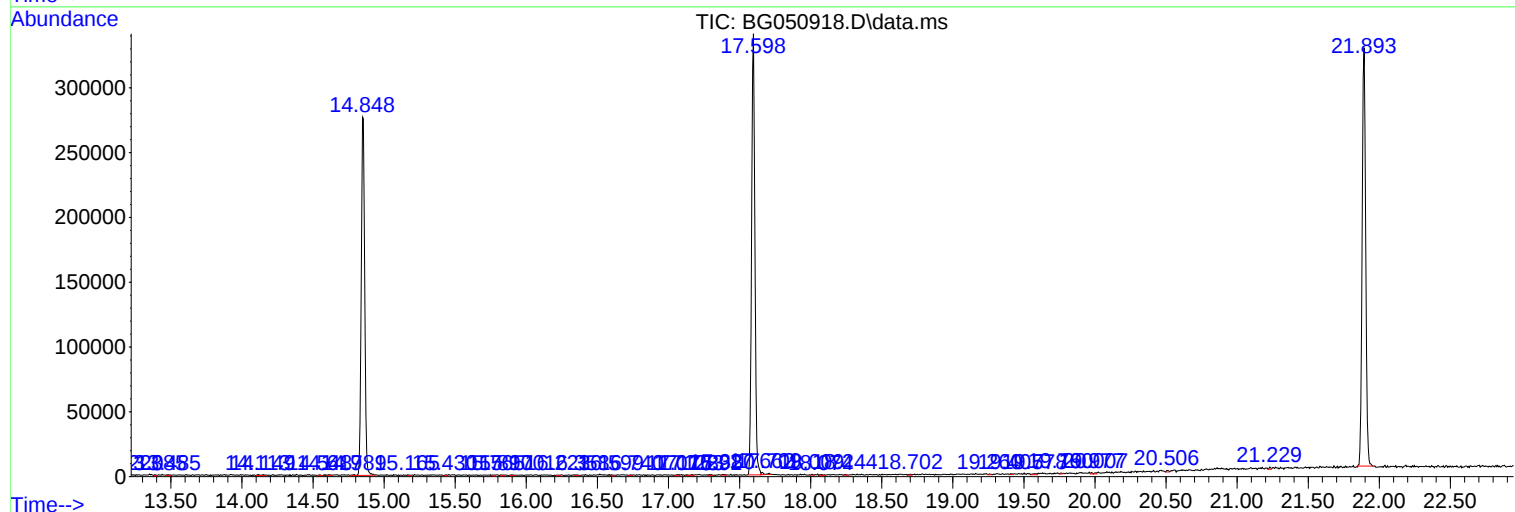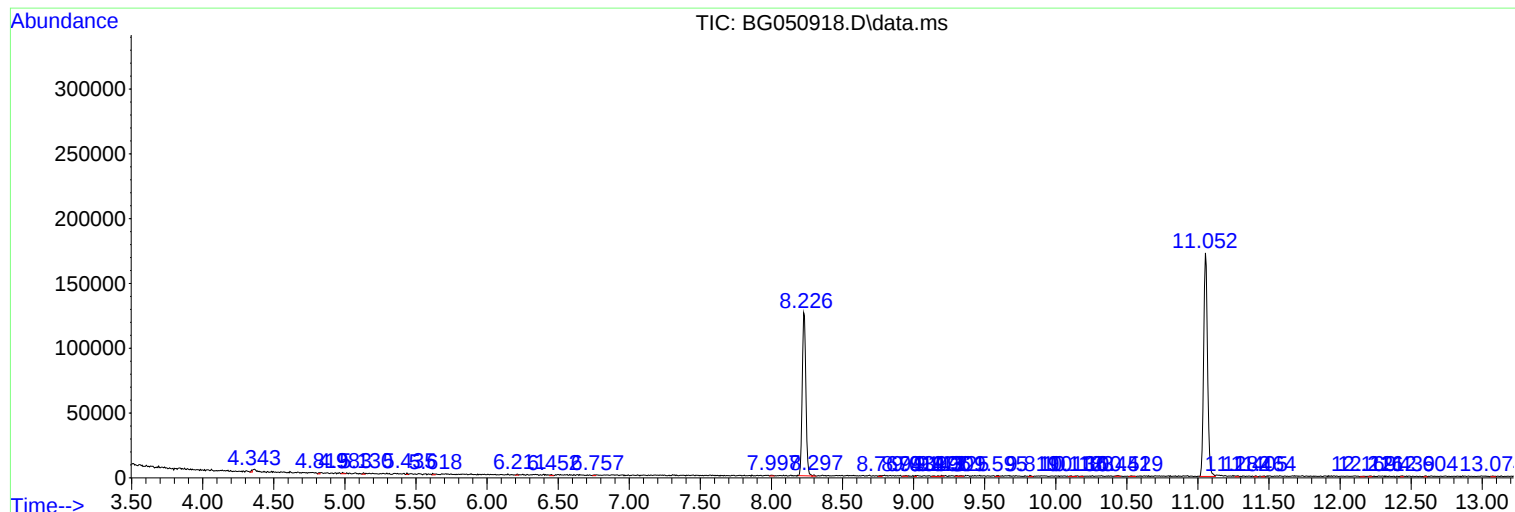

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050918.D
Acq On : 9 Nov 2021 21:03
Operator : CG/JU
Sample : M4490-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050918.D
Acq On : 9 Nov 2021 21:03
Operator : CG/JU
Sample : M4490-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc