

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050932.D
 Acq On : 10 Nov 2021 7:22
 Operator : CG/JU
 Sample : M4532-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB859

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.588	13	17	25	rBV3	10441	18239	1.25%	0.146%
2	4.017	86	90	101	rBV	44415	83110	5.71%	0.665%
3	4.111	104	106	111	rVB2	1353	1574	0.11%	0.013%
4	4.252	125	130	135	rBV3	4876	7945	0.55%	0.064%
5	4.358	144	148	153	rBV3	2694	4287	0.29%	0.034%
6	7.372	654	661	669	rBV2	46480	81041	5.57%	0.648%
7	7.542	682	690	701	rVB	148270	260300	17.88%	2.083%
8	7.754	719	726	734	rBV	145258	252704	17.36%	2.022%
9	8.230	799	807	819	rBV	140182	244893	16.82%	1.959%
10	8.923	919	925	935	rBV2	118594	212867	14.62%	1.703%
11	9.399	997	1006	1016	rBV	187254	337076	23.15%	2.697%
12	9.763	1062	1068	1072	rVB2	976	1728	0.12%	0.014%
13	10.127	1123	1130	1140	rVB	142220	263921	18.13%	2.112%
14	10.668	1215	1222	1232	rBV	186214	353807	24.30%	2.831%
15	11.050	1280	1287	1298	rVB	197267	366732	25.19%	2.934%
16	11.185	1302	1310	1321	rBV	170896	322463	22.15%	2.580%
17	11.567	1371	1375	1378	rBV3	1008	1499	0.10%	0.012%
18	12.624	1550	1555	1560	rBV3	3534	5802	0.40%	0.046%
19	13.723	1738	1742	1746	rBV3	1263	1870	0.13%	0.015%
20	14.246	1823	1831	1837	rBV	430644	654890	44.98%	5.239%
21	14.546	1874	1882	1890	rBV	486780	777569	53.41%	6.221%
22	14.851	1927	1934	1944	rBV	333317	521000	35.78%	4.168%
23	15.045	1961	1967	1978	rBV	30966	66088	4.54%	0.529%
24	15.257	2000	2003	2006	rBV2	1108	1459	0.10%	0.012%
25	15.574	2051	2057	2060	rBV	3288	5007	0.34%	0.040%
26	15.615	2060	2064	2069	rVV	3895	5512	0.38%	0.044%
27	15.838	2095	2102	2114	rBV	671857	1023758	70.32%	8.191%
28	15.950	2115	2121	2132	rBV	202338	316411	21.73%	2.531%
29	17.384	2360	2365	2369	rVB2	1304	2435	0.17%	0.019%
30	17.595	2393	2401	2410	rVB	429144	658674	45.24%	5.270%
31	17.695	2410	2418	2426	rBV	825996	1244213	85.46%	9.954%
32	17.771	2427	2431	2437	rVV4	6294	8749	0.60%	0.070%
33	18.230	2506	2509	2516	rVB4	3174	4817	0.33%	0.039%
34	18.523	2554	2559	2566	rBV2	2413	4563	0.31%	0.037%
35	18.741	2591	2596	2599	rVB3	1308	2017	0.14%	0.016%
36	19.393	2703	2707	2709	rVV3	2762	3889	0.27%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050932.D
 Acq On : 10 Nov 2021 7:22
 Operator : CG/JU
 Sample : M4532-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB859

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	19.422	2709	2712	2717	rVB3	1965	3536	0.24%	0.028%
38	19.534	2726	2731	2738	rVB2	10619	15976	1.10%	0.128%
39	19.605	2738	2743	2748	rBV	11264	15612	1.07%	0.125%
40	19.851	2782	2785	2790	rVB3	1727	2731	0.19%	0.022%

41	19.969	2798	2805	2814	rBV	995851	1455919	100.00%	11.648%
42	20.456	2884	2888	2892	rBV6	2330	4762	0.33%	0.038%
43	20.809	2944	2948	2949	rBV4	1890	2313	0.16%	0.019%
44	20.832	2949	2952	2954	rBV4	3128	4225	0.29%	0.034%
45	20.885	2959	2961	2962	rBV2	2290	1806	0.12%	0.014%

46	20.962	2971	2974	2978	rVB5	2641	3125	0.21%	0.025%
47	21.120	2999	3001	3004	rBV4	1489	1585	0.11%	0.013%
48	21.485	3059	3063	3069	rBV8	7676	15018	1.03%	0.120%
49	21.708	3099	3101	3103	rBV3	1688	1932	0.13%	0.015%
50	21.737	3103	3106	3110	rVB4	4494	5881	0.40%	0.047%

51	21.890	3125	3132	3140	rBV	382934	657043	45.13%	5.257%
52	21.996	3144	3150	3154	rBV3	4893	8266	0.57%	0.066%
53	22.043	3156	3158	3163	rBV5	3795	6985	0.48%	0.056%
54	22.143	3174	3175	3178	rVB3	2717	1627	0.11%	0.013%
55	22.313	3202	3204	3207	rBV3	1295	1462	0.10%	0.012%

56	22.578	3246	3249	3254	rVB5	1977	2671	0.18%	0.021%
57	22.689	3264	3268	3273	rVB6	4732	7024	0.48%	0.056%
58	23.059	3329	3331	3336	rBV6	2536	3217	0.22%	0.026%
59	23.412	3387	3391	3400	rVB6	8413	16842	1.16%	0.135%
60	23.512	3405	3408	3409	rBV2	1359	1767	0.12%	0.014%

61	24.035	3496	3497	3500	rBV3	2397	1683	0.12%	0.013%
62	24.264	3530	3536	3544	rVB5	10761	23503	1.61%	0.188%
63	24.928	3647	3649	3652	rVB3	2043	1468	0.10%	0.012%
64	25.057	3658	3671	3685	rBV2	434863	1304892	89.63%	10.440%
65	25.286	3698	3710	3723	rVB2	227370	675566	46.40%	5.405%

66	25.492	3743	3745	3748	rVB4	1930	2175	0.15%	0.017%
67	25.521	3748	3750	3753	rBV3	1801	1715	0.12%	0.014%
68	25.944	3820	3822	3824	rBV3	1338	1590	0.11%	0.013%
69	26.467	3902	3911	3920	rVB6	13415	41484	2.85%	0.332%
70	27.202	4034	4036	4039	rBV3	1588	1783	0.12%	0.014%

71	27.319	4054	4056	4061	rBV3	1770	2189	0.15%	0.018%
72	27.354	4061	4062	4067	rVB5	2539	2140	0.15%	0.017%
73	27.901	4145	4155	4166	rBB7	11564	42030	2.89%	0.336%
74	28.570	4267	4269	4272	rBV4	1727	1994	0.14%	0.016%
75	28.853	4315	4317	4321	rBV5	1594	2272	0.16%	0.018%

76	28.935	4329	4331	4334	rBV3	1634	1669	0.11%	0.013%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050932.D
Acq On : 10 Nov 2021 7:22
Operator : CG/JU
Sample : M4532-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB859

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION

77	29.640	4443	4451	4454	rBV6	6106	15986	1.10%	0.128%
78	30.521	4598	4601	4602	rBV3	1618	1540	0.11%	0.012%
79	31.250	4724	4725	4727	rBV	1878	1630	0.11%	0.013%
80	31.726	4803	4806	4808	rBV5	3305	4147	0.28%	0.033%
81	32.008	4851	4854	4856	rVB4	1845	1890	0.13%	0.015%
82	32.284	4899	4901	4903	rBV3	1684	1638	0.11%	0.013%




Sum of corrected areas: 12499218

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050932.D
Acq On : 10 Nov 2021 7:22
Operator : CG/JU
Sample : M4532-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB859

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

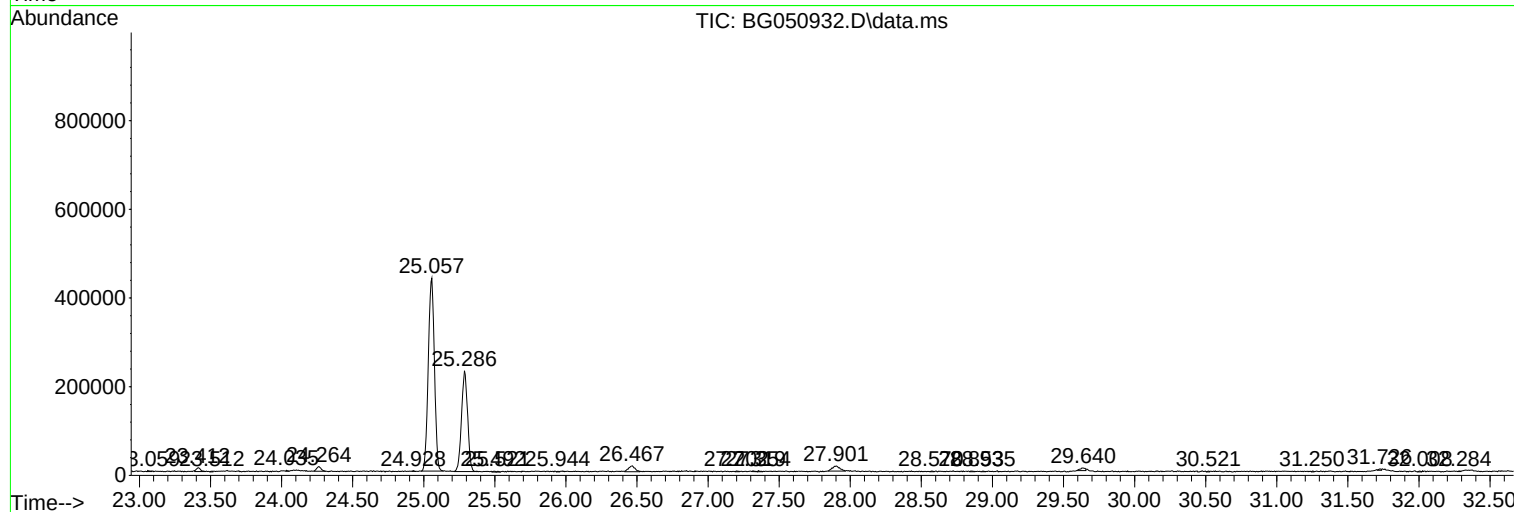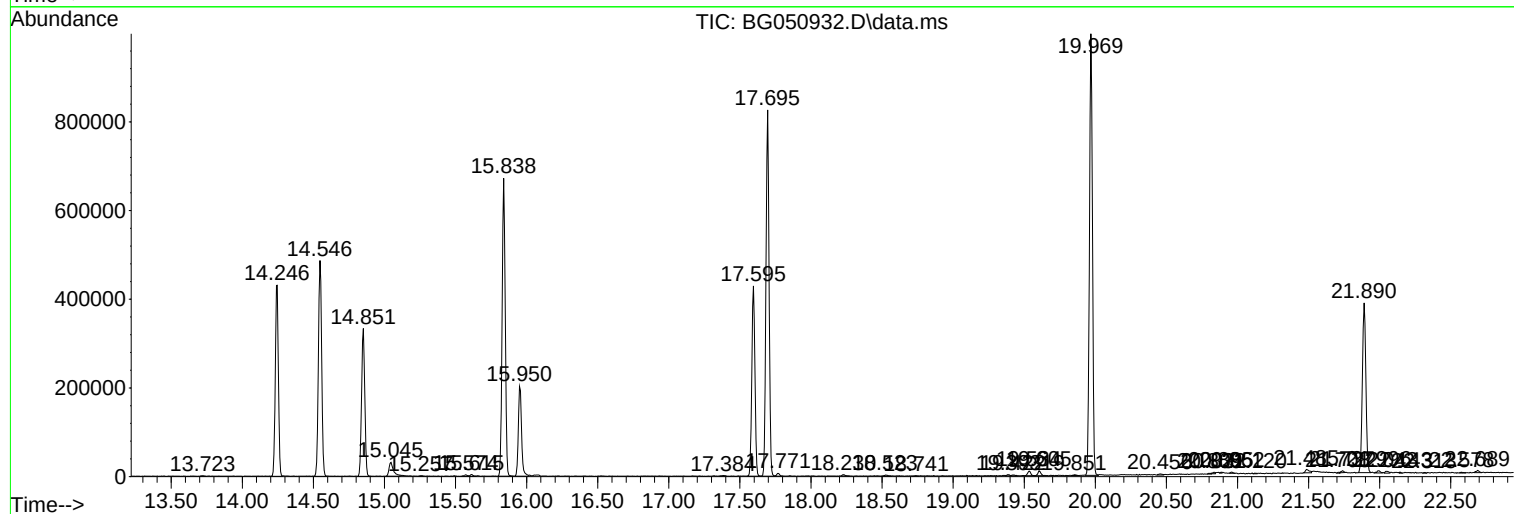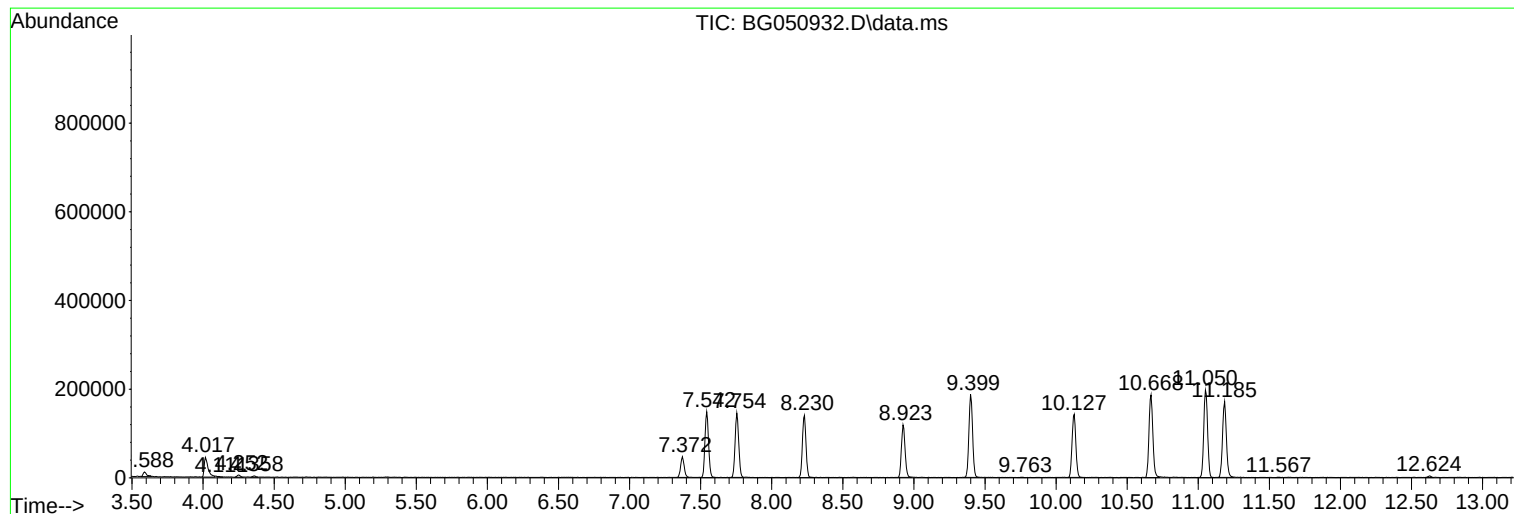

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050932.D
Acq On : 10 Nov 2021 7:22
Operator : CG/JU
Sample : M4532-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB859

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050932.D
Acq On : 10 Nov 2021 7:22
Operator : CG/JU
Sample : M4532-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB859

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc