

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050947.D
 Acq On : 10 Nov 2021 17:38
 Operator : CG/JU
 Sample : M4532-13DL 50X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB8F0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.626	18	23	33	rVB2	31753	53510	9.50%	1.839%
2	3.837	57	59	60	rBV2	764	799	0.14%	0.027%
3	3.920	71	73	77	rBV3	911	892	0.16%	0.031%
4	4.113	104	106	110	rBV3	743	1027	0.18%	0.035%
5	4.360	145	148	154	rVB3	2376	3585	0.64%	0.123%
6	4.725	207	210	214	rBV3	841	1055	0.19%	0.036%
7	4.901	239	240	242	rBV2	996	798	0.14%	0.027%
8	5.048	264	265	268	rBV3	770	659	0.12%	0.023%
9	5.383	320	322	324	rVB2	973	771	0.14%	0.027%
10	5.412	324	327	329	rBV2	634	861	0.15%	0.030%
11	5.841	397	400	402	rVB2	740	822	0.15%	0.028%
12	6.235	464	467	471	rVB3	640	749	0.13%	0.026%
13	6.487	507	510	513	rBV4	1257	1548	0.27%	0.053%
14	6.869	574	575	578	rBV2	598	656	0.12%	0.023%
15	7.363	655	659	661	rBV3	499	707	0.13%	0.024%
16	7.545	686	690	697	rVB5	3101	5652	1.00%	0.194%
17	7.603	697	700	702	rBV2	947	1185	0.21%	0.041%
18	7.762	723	727	732	rVB3	1687	2684	0.48%	0.092%
19	8.103	783	785	788	rVB3	815	963	0.17%	0.033%
20	8.226	799	806	814	rBV	122190	218717	38.84%	7.518%
21	8.408	835	837	842	rVB3	781	810	0.14%	0.028%
22	8.455	843	845	848	rBV3	668	694	0.12%	0.024%
23	8.943	924	928	931	rBV3	648	1013	0.18%	0.035%
24	9.166	965	966	969	rBV3	723	762	0.14%	0.026%
25	9.354	996	998	1000	rVB2	826	716	0.13%	0.025%
26	9.413	1003	1008	1009	rBV2	2979	3130	0.56%	0.108%
27	9.607	1040	1041	1045	rBV3	751	1072	0.19%	0.037%
28	9.965	1101	1102	1106	rBV3	766	661	0.12%	0.023%
29	10.036	1110	1114	1118	rVB3	688	976	0.17%	0.034%
30	10.077	1118	1121	1123	rBV3	614	658	0.12%	0.023%
31	10.130	1127	1130	1133	rBV3	1046	1254	0.22%	0.043%
32	10.330	1163	1164	1167	rBV	812	784	0.14%	0.027%
33	10.424	1178	1180	1185	rBV5	533	741	0.13%	0.025%
34	10.576	1205	1206	1210	rVB3	667	668	0.12%	0.023%
35	10.647	1215	1218	1220	rVB3	768	934	0.17%	0.032%
36	10.676	1220	1223	1225	rBV2	675	743	0.13%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050947.D
 Acq On : 10 Nov 2021 17:38
 Operator : CG/JU
 Sample : M4532-13DL 50X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GB8F0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	10.712	1225	1229	1230	rBV3	909	920	0.16%	0.032%
38	10.988	1271	1276	1277	rBV3	696	852	0.15%	0.029%
39	11.052	1280	1287	1299	rVV	169757	325363	57.78%	11.184%
40	11.129	1299	1300	1305	rVB3	678	836	0.15%	0.029%
41	11.282	1325	1326	1331	rVB2	636	702	0.12%	0.024%
42	11.511	1363	1365	1369	rBV3	639	765	0.14%	0.026%
43	12.568	1543	1545	1548	rVB2	710	703	0.12%	0.024%
44	12.609	1548	1552	1553	rBV2	640	690	0.12%	0.024%
45	12.880	1595	1598	1600	rVB2	669	658	0.12%	0.023%
46	12.921	1600	1605	1607	rBV3	735	1103	0.20%	0.038%
47	13.232	1654	1658	1660	rBV3	582	738	0.13%	0.025%
48	13.996	1786	1788	1791	rVB2	722	849	0.15%	0.029%
49	14.208	1820	1824	1827	rBV5	472	851	0.15%	0.029%
50	14.255	1827	1832	1841	rVV2	5483	11143	1.98%	0.383%
51	14.331	1843	1845	1849	rVB2	880	912	0.16%	0.031%
52	14.548	1875	1882	1888	rVB	8411	13666	2.43%	0.470%
53	14.848	1926	1933	1943	rBV	293610	463740	82.35%	15.940%
54	15.012	1956	1961	1962	rBV3	460	707	0.13%	0.024%
55	15.571	2053	2056	2058	rBV2	798	714	0.13%	0.025%
56	15.847	2095	2103	2113	rBV2	10222	19517	3.47%	0.671%
57	16.323	2183	2184	2187	rVB3	682	666	0.12%	0.023%
58	16.458	2204	2207	2210	rBV3	604	908	0.16%	0.031%
59	16.810	2262	2267	2268	rBV4	693	1024	0.18%	0.035%
60	17.069	2309	2311	2314	rVB2	749	687	0.12%	0.024%
61	17.098	2314	2316	2318	rBV2	894	782	0.14%	0.027%
62	17.380	2361	2364	2368	rBV5	1138	1768	0.31%	0.061%
63	17.592	2393	2400	2412	rBV	343729	559369	99.34%	19.227%
64	17.698	2412	2418	2429	rVB2	12704	23442	4.16%	0.806%
65	17.868	2445	2447	2448	rBV	775	659	0.12%	0.023%
66	17.886	2448	2450	2453	rVB2	920	950	0.17%	0.033%
67	18.173	2495	2499	2502	rVB4	827	1226	0.22%	0.042%
68	18.485	2549	2552	2554	rBV3	590	737	0.13%	0.025%
69	18.732	2593	2594	2597	rBV3	868	750	0.13%	0.026%
70	19.125	2657	2661	2662	rBV3	633	734	0.13%	0.025%
71	19.343	2695	2698	2700	rBV2	1070	1024	0.18%	0.035%
72	19.384	2703	2705	2707	rVB3	948	699	0.12%	0.024%
73	19.589	2739	2740	2744	rBV4	827	947	0.17%	0.033%
74	19.678	2753	2755	2759	rVB3	1192	1121	0.20%	0.039%
75	19.725	2759	2763	2765	rBV4	1120	1460	0.26%	0.050%
76	19.830	2779	2781	2785	rBV3	862	1261	0.22%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050947.D
Acq On : 10 Nov 2021 17:38
Operator : CG/JU
Sample : M4532-13DL 50X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8F0DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION

77	19.971	2800	2805	2812	rVB2	15384	24612	4.37%	0.846%
78	20.265	2853	2855	2857	rBV2	1167	1035	0.18%	0.036%
79	20.676	2923	2925	2926	rBV2	1483	879	0.16%	0.030%
80	20.988	2976	2978	2979	rBV2	1857	1229	0.22%	0.042%

81	21.887	3124	3131	3143	rVB2	324663	563109	100.00%	19.356%
82	25.277	3699	3708	3723	rVB2	189396	559525	99.36%	19.232%




Sum of corrected areas: 2909288

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050947.D
Acq On : 10 Nov 2021 17:38
Operator : CG/JU
Sample : M4532-13DL 50X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8F0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

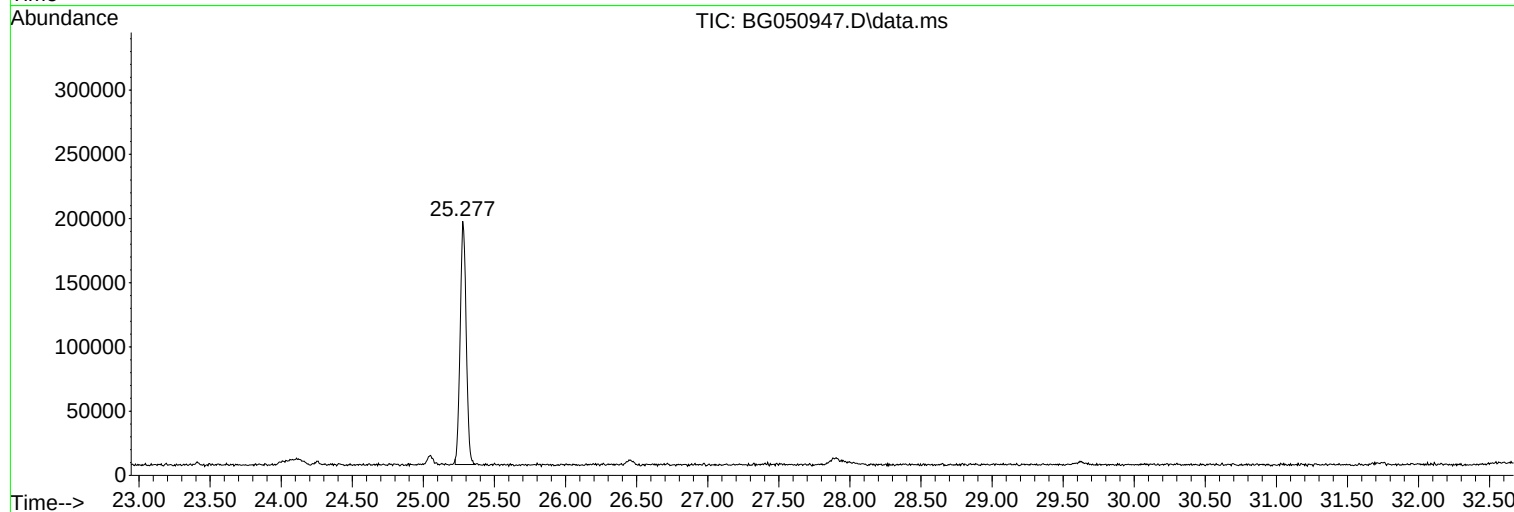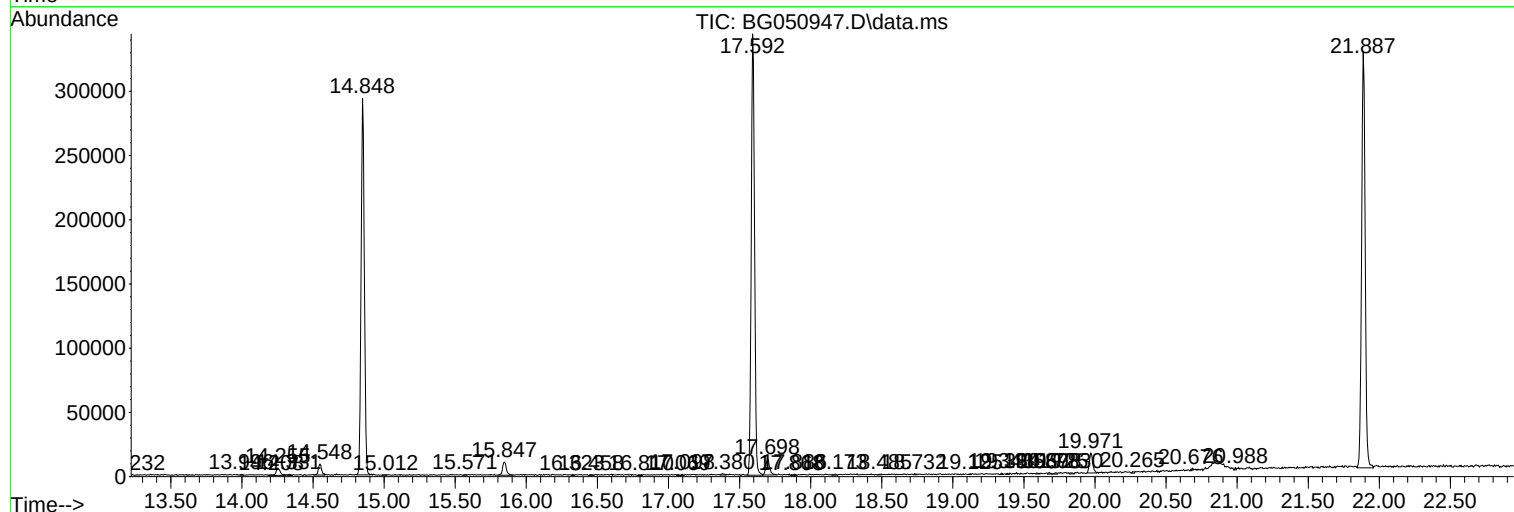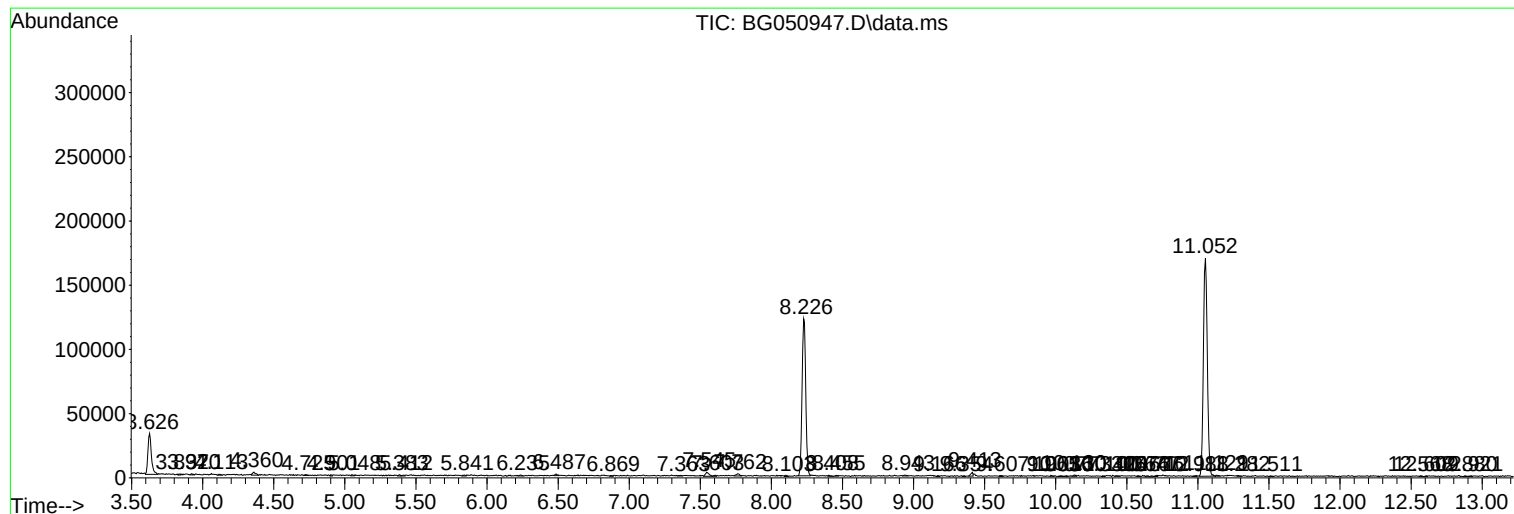

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050947.D
Acq On : 10 Nov 2021 17:38
Operator : CG/JU
Sample : M4532-13DL 50X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8F0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050947.D
Acq On : 10 Nov 2021 17:38
Operator : CG/JU
Sample : M4532-13DL 50X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GB8F0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------