

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050956.D
 Acq On : 11 Nov 2021 00:29
 Operator : CG/JU
 Sample : M4445-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.588	13	17	24	rVB2	9076	15215	1.18%	0.139%
2	4.017	86	90	102	rBV	21524	43839	3.41%	0.400%
3	4.246	125	129	138	rVB3	4384	7198	0.56%	0.066%
4	4.358	143	148	152	rVB3	2194	3157	0.25%	0.029%
5	5.292	301	307	312	rBV3	2353	4495	0.35%	0.041%
6	7.301	645	649	653	rVB4	1235	1931	0.15%	0.018%
7	7.372	653	661	672	rBV	37113	71204	5.54%	0.649%
8	7.542	683	690	701	rVB	123486	210775	16.39%	1.921%
9	7.754	719	726	734	rBV	117060	205175	15.95%	1.870%
10	8.224	798	806	816	rVB	116359	209013	16.25%	1.905%
11	8.923	917	925	935	rVB	99345	179011	13.92%	1.632%
12	9.399	995	1006	1019	rBV	152994	278989	21.69%	2.543%
13	9.763	1062	1068	1072	rVB	7543	11005	0.86%	0.100%
14	10.127	1122	1130	1139	rVB	114629	212026	16.48%	1.933%
15	10.668	1214	1222	1234	rBV	153274	296589	23.06%	2.704%
16	11.050	1278	1287	1296	rVB	176036	323964	25.19%	2.953%
17	11.185	1302	1310	1322	rBV	140195	274792	21.36%	2.505%
18	12.248	1485	1491	1496	rBV	7575	9983	0.78%	0.091%
19	12.630	1550	1556	1560	rBV2	2326	4163	0.32%	0.038%
20	14.240	1822	1830	1843	rBV	397824	589792	45.85%	5.376%
21	14.546	1875	1882	1893	rBV	415065	662259	51.49%	6.037%
22	14.851	1927	1934	1943	rVB	290103	471191	36.63%	4.295%
23	15.045	1961	1967	1982	rBV3	24405	59698	4.64%	0.544%
24	15.257	2000	2003	2007	rVB2	1355	1361	0.11%	0.012%
25	15.838	2094	2102	2111	rBV	582387	898717	69.87%	8.192%
26	15.950	2115	2121	2130	rBV	173004	268626	20.88%	2.449%
27	16.079	2138	2143	2148	rVB4	2129	2641	0.21%	0.024%
28	17.319	2351	2354	2356	rBV2	1217	1408	0.11%	0.013%
29	17.378	2361	2364	2369	rVB2	1348	1970	0.15%	0.018%
30	17.595	2394	2401	2408	rBV	374631	584852	45.47%	5.331%
31	17.695	2410	2418	2426	rBV	702186	1099637	85.49%	10.024%
32	18.230	2505	2509	2512	rVB4	1529	1873	0.15%	0.017%
33	19.358	2698	2701	2705	rBV4	1794	2479	0.19%	0.023%
34	19.534	2726	2731	2737	rVV2	9424	13522	1.05%	0.123%
35	19.605	2739	2743	2749	rVB2	8946	13847	1.08%	0.126%
36	19.969	2795	2805	2815	rBV	885152	1286297	100.00%	11.726%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050956.D
 Acq On : 11 Nov 2021 00:29
 Operator : CG/JU
 Sample : M4445-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	20.180	2838	2841	2845	rBV4	1520	1645	0.13%	0.015%
38	20.456	2883	2888	2896	rBV4	9350	15142	1.18%	0.138%
39	20.545	2901	2903	2905	rBV2	2055	1574	0.12%	0.014%
40	20.644	2916	2920	2921	rVB3	1421	1447	0.11%	0.013%
41	20.680	2924	2926	2929	rBV3	1483	1654	0.13%	0.015%
42	20.838	2946	2953	2954	rBV6	5642	10202	0.79%	0.093%
43	20.897	2961	2963	2967	rVB5	3315	3376	0.26%	0.031%
44	20.962	2970	2974	2977	rVV	15046	18222	1.42%	0.166%
45	21.003	2977	2981	2985	rVB6	2309	4075	0.32%	0.037%
46	21.167	3008	3009	3012	rBV2	1408	1616	0.13%	0.015%
47	21.279	3026	3028	3031	rVB4	1463	1414	0.11%	0.013%
48	21.397	3046	3048	3051	rBV4	1290	1577	0.12%	0.014%
49	21.485	3058	3063	3068	rBV2	19006	29764	2.31%	0.271%
50	21.702	3099	3100	3102	rBV2	1574	1370	0.11%	0.012%
51	21.737	3104	3106	3110	rVB5	3892	3741	0.29%	0.034%
52	21.820	3118	3120	3124	rBV5	1945	2188	0.17%	0.020%
53	21.890	3125	3132	3141	rVB	339578	573445	44.58%	5.227%
54	22.049	3154	3159	3163	rBV2	15769	22093	1.72%	0.201%
55	22.278	3196	3198	3200	rVB3	1927	1594	0.12%	0.015%
56	22.413	3220	3221	3223	rBV2	2706	1891	0.15%	0.017%
57	22.683	3262	3267	3273	rVB3	14196	24454	1.90%	0.223%
58	22.813	3287	3289	3292	rVB4	1904	1693	0.13%	0.015%
59	22.912	3302	3306	3308	rBV5	1556	2375	0.18%	0.022%
60	23.077	3331	3334	3339	rVB6	3470	5277	0.41%	0.048%
61	23.412	3385	3391	3395	rVV5	12077	24541	1.91%	0.224%
62	23.612	3419	3425	3432	rVB2	17573	36445	2.83%	0.332%
63	23.741	3443	3447	3448	rBV3	1682	2221	0.17%	0.020%
64	23.864	3467	3468	3472	rBV4	1238	1484	0.12%	0.014%
65	23.894	3472	3473	3476	rBV2	1819	1896	0.15%	0.017%
66	24.252	3528	3534	3544	rBV4	13106	31823	2.47%	0.290%
67	24.446	3565	3567	3569	rBV2	2189	1471	0.11%	0.013%
68	24.563	3585	3587	3590	rVB3	2577	1869	0.15%	0.017%
69	24.945	3648	3652	3654	rBV5	1700	2436	0.19%	0.022%
70	25.051	3658	3670	3682	rVV2	397792	1144751	89.00%	10.435%
71	25.280	3697	3709	3723	rVB2	185849	584240	45.42%	5.326%
72	25.445	3735	3737	3738	rBV2	2806	2066	0.16%	0.019%
73	25.921	3816	3818	3819	rBV2	2205	1327	0.10%	0.012%
74	26.244	3872	3873	3875	rBV2	2009	1765	0.14%	0.016%
75	26.397	3896	3899	3901	rBV4	2104	2965	0.23%	0.027%
76	26.455	3902	3909	3919	rVB5	10436	30079	2.34%	0.274%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
 Data File : BG050956.D
 Acq On : 11 Nov 2021 00:29
 Operator : CG/JU
 Sample : M4445-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

77	26.655	3939	3943	3944	rBV4	1867	2620	0.20%	0.024%
78	27.119	4021	4022	4025	rVB3	2600	2021	0.16%	0.018%
79	27.807	4136	4139	4140	rBV3	1870	2211	0.17%	0.020%
80	27.854	4144	4147	4148	rBV3	3839	3390	0.26%	0.031%
81	27.877	4148	4151	4152	rBV3	3977	4864	0.38%	0.044%
82	28.071	4182	4184	4189	rBV6	1315	1886	0.15%	0.017%
83	28.318	4224	4226	4229	rBV4	1899	1684	0.13%	0.015%
84	28.935	4329	4331	4334	rBV3	1576	1556	0.12%	0.014%
85	29.328	4395	4398	4399	rBV3	1762	1577	0.12%	0.014%
86	29.434	4414	4416	4420	rVB5	1698	1919	0.15%	0.017%
87	29.910	4495	4497	4498	rBV2	2099	1379	0.11%	0.013%
88	30.004	4511	4513	4516	rBV3	1542	2340	0.18%	0.021%
89	30.410	4579	4582	4586	rBV5	1969	3223	0.25%	0.029%
90	30.674	4625	4627	4628	rBV2	2315	1739	0.14%	0.016%
91	30.909	4666	4667	4668	rBV	2654	1468	0.11%	0.013%
92	31.579	4779	4781	4784	rBV3	1733	1860	0.14%	0.017%
93	31.679	4794	4798	4799	rBV3	2143	2485	0.19%	0.023%
94	31.696	4799	4801	4802	rBV2	1622	1411	0.11%	0.013%
95	31.714	4802	4804	4806	rVV3	2204	2331	0.18%	0.021%
96	32.190	4882	4885	4887	rBV3	2376	2170	0.17%	0.020%




Sum of corrected areas: 10970036

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050956.D
Acq On : 11 Nov 2021 00:29
Operator : CG/JU
Sample : M4445-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

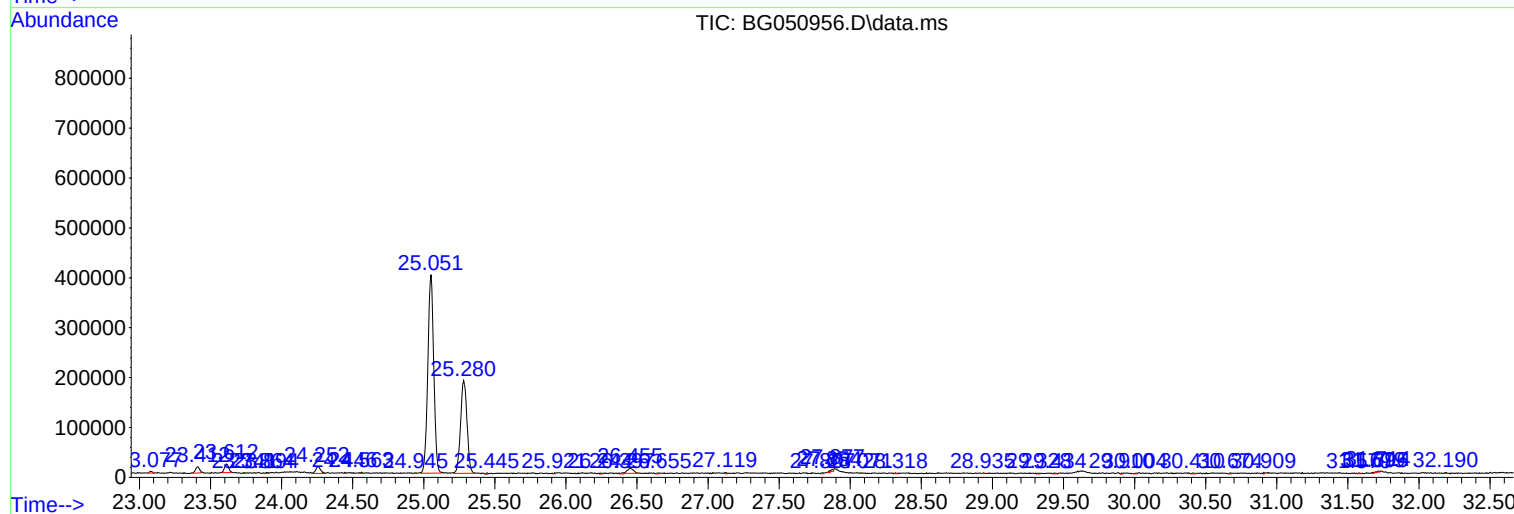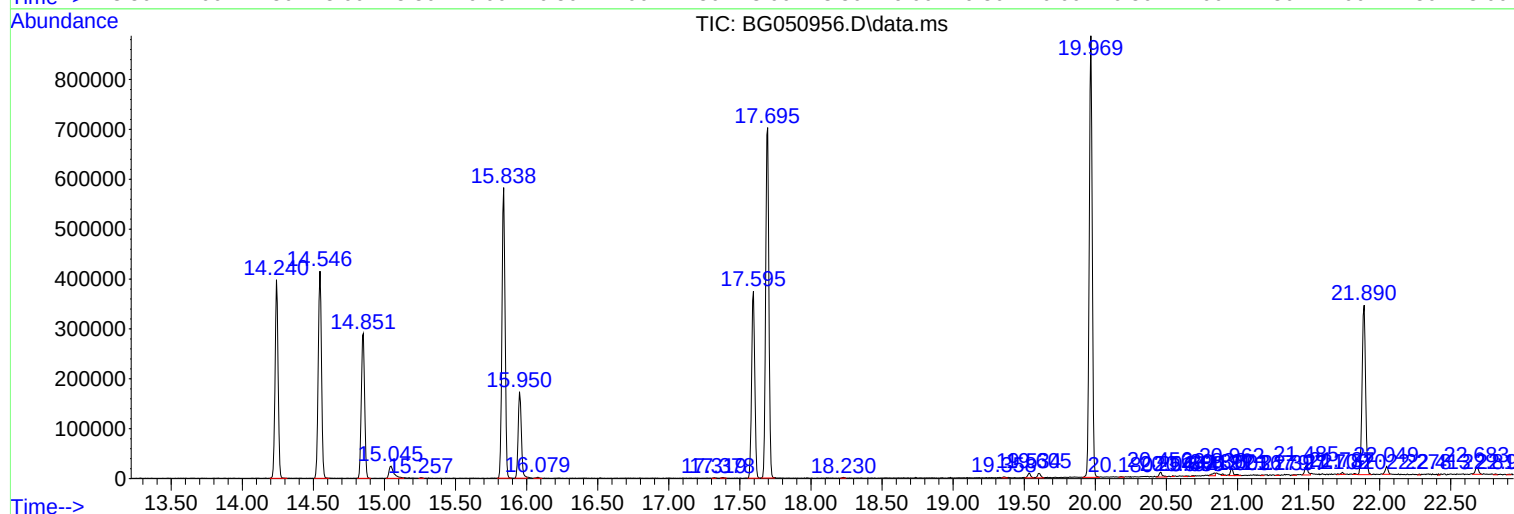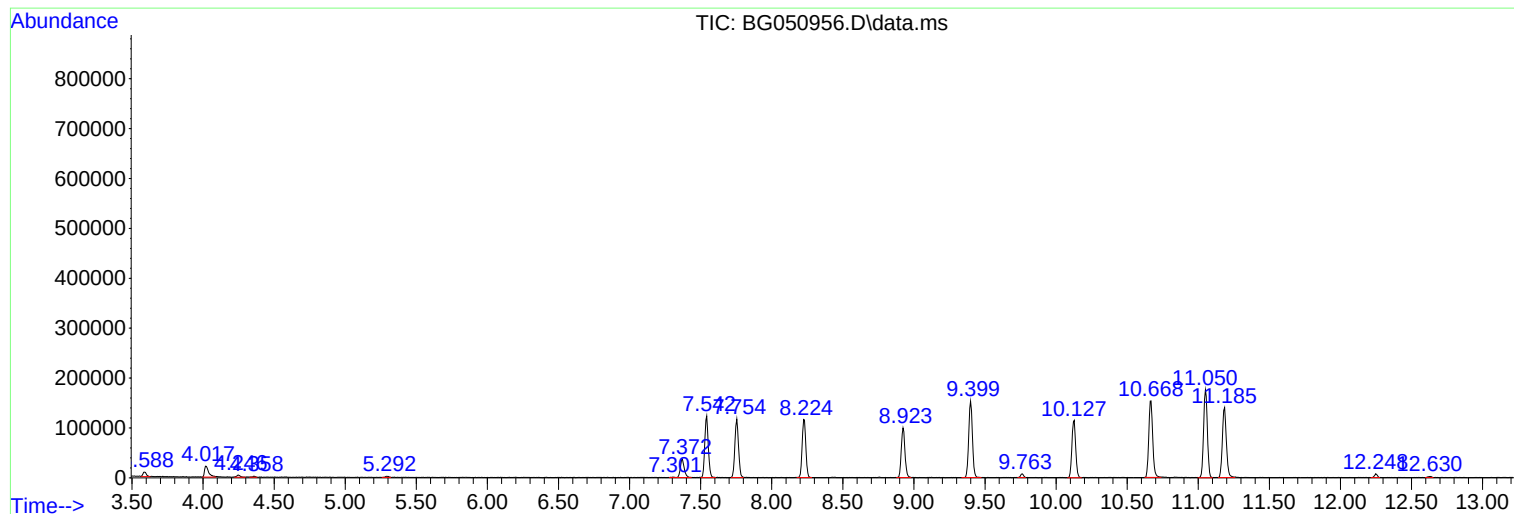

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050956.D
Acq On : 11 Nov 2021 00:29
Operator : CG/JU
Sample : M4445-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110821\
Data File : BG050956.D
Acq On : 11 Nov 2021 00:29
Operator : CG/JU
Sample : M4445-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc