

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111020\
 Data File : BG047267.D
 Acq On : 10 Nov 2020 12:08
 Operator : CG/JU
 Sample : L4649-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7Z9

Quant Time: Nov 10 12:50:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 10 10:50:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	52438	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	215205	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	156799	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.39	188	384262	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	411704	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	418642	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.40	96	9215	7.09	ng/uL	0.00
5) Phenol-d5	7.16	99	146901	32.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	90428	34.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	117267	33.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	120116	33.08	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	59915	33.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	69086	32.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	128123	31.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	169171	48.25	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	432830	33.57	ng/ul	0.00
47) Acenaphthylene-d8	14.34	160	510434	33.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	64280	31.67	ng/ul	0.00
58) Fluorene-d10	15.63	176	385606	32.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.75	200	78821	29.74	ng/ul	0.00
71) Anthracene-d10	17.49	188	612029	32.86	ng/ul	0.00
79) Pyrene-d10	19.77	212	773191	32.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.62	264	766260	33.29	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	14.08	163	31303	2.419	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111020\
Data File : BG047267.D
Acq On : 10 Nov 2020 12:08
Operator : CG/JU
Sample : L4649-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7Z9

Quant Time: Nov 10 12:50:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 10 10:50:02 2020
Response via : Initial Calibration

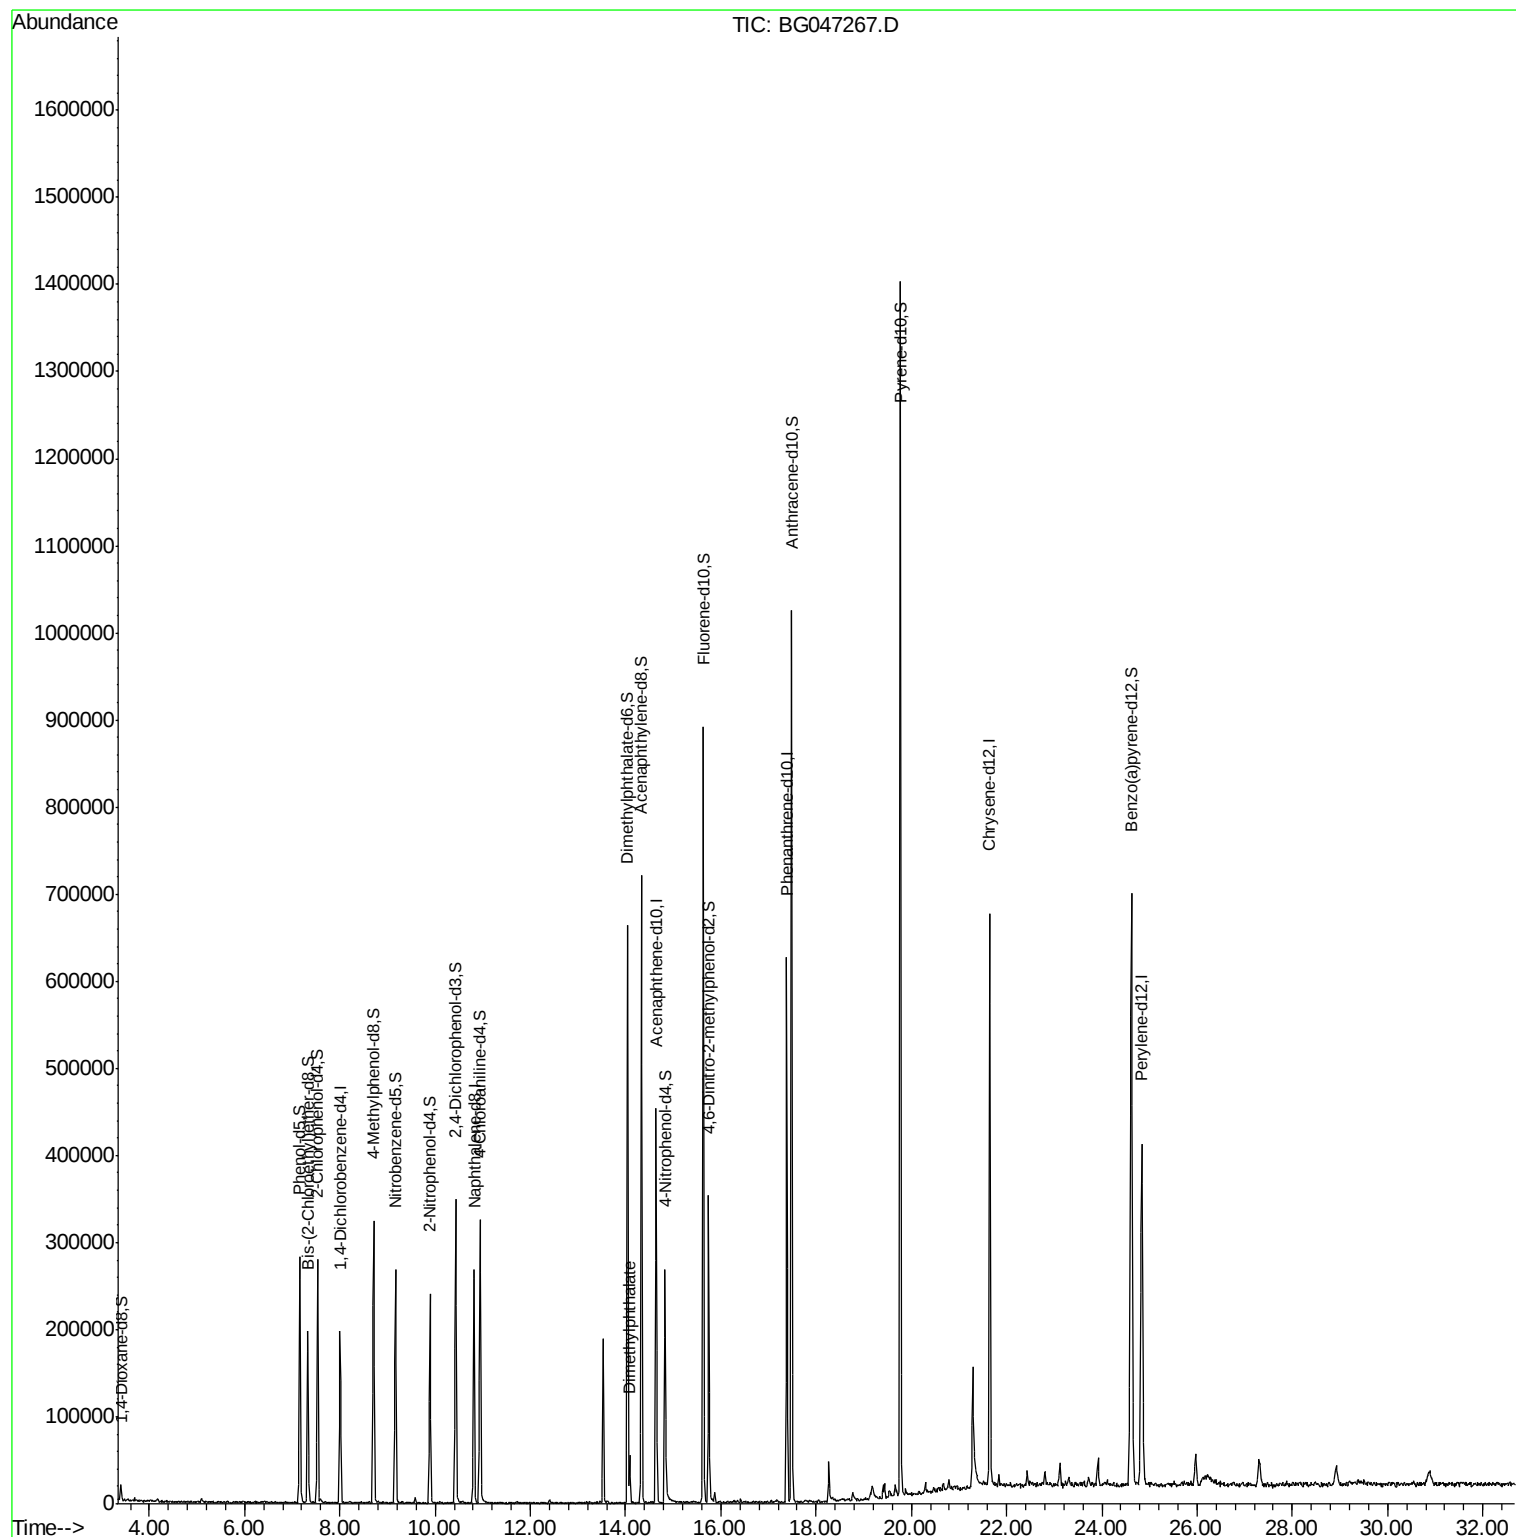

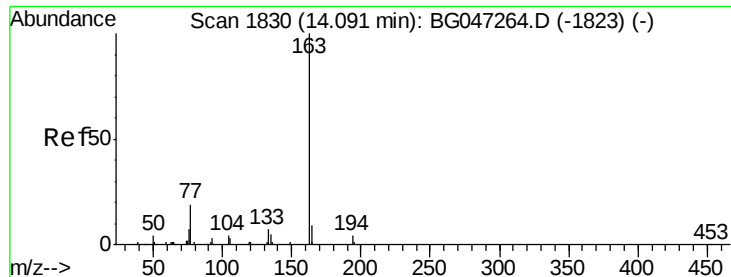

#45

Dimethylphthalate

Concen: 2.419 ng/ul

RT: 14.08 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BG047267.D

Acq: 10 Nov 2020 12:08

Instrument :

BNA_G

ClientSampleId :

CB7Z9

Tot Ion:163 Resp: 31303

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.0

164 11.6 7.2 10.8#

