
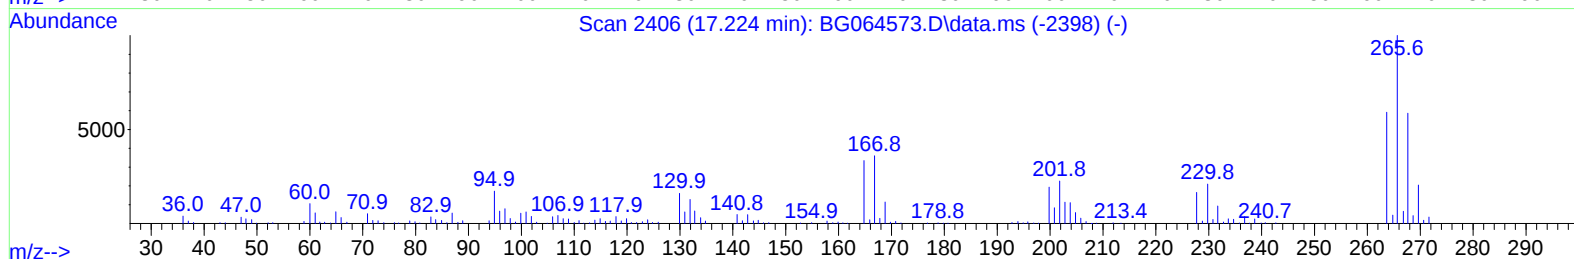
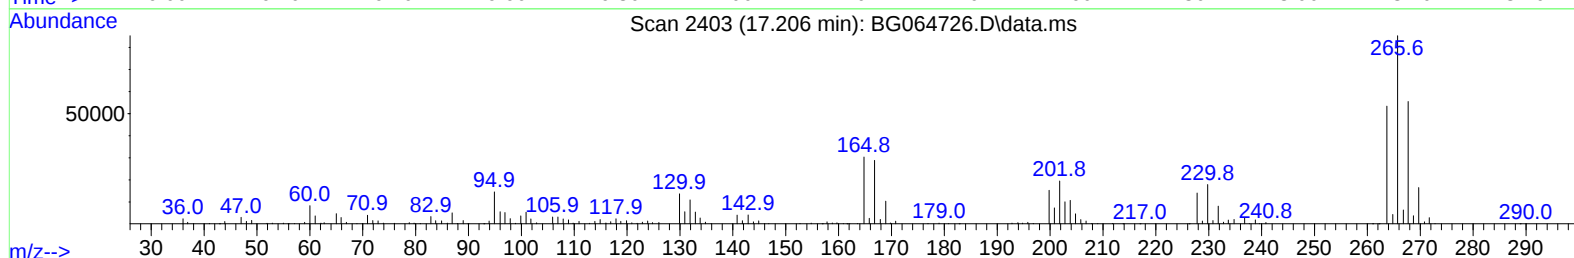


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111025\
Data File : BG064726.D
Acq On : 10 Nov 2025 8:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 09:45:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

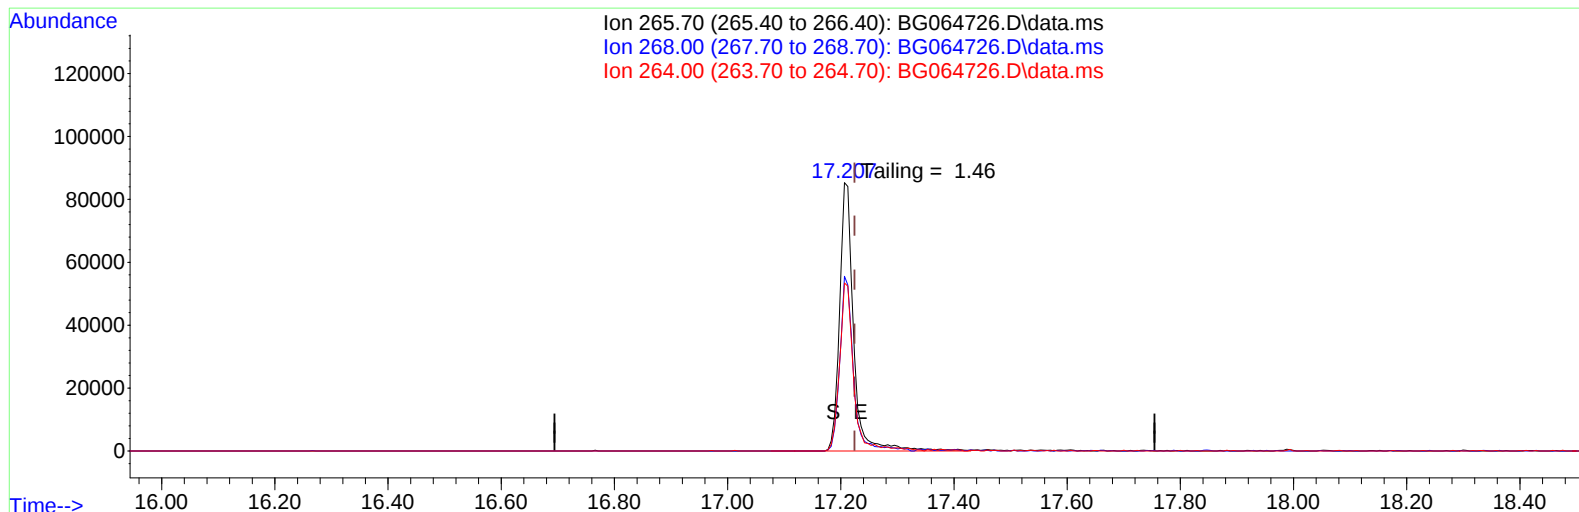

TIC: BG064726.D\data.ms

(70) Pentachlorophenol (C)




17.206min (-0.018) 284159.15 ng

response 146131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	69.51
264.00	59.10	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111025\
Data File : BG064726.D
Acq On : 10 Nov 2025 8:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 09:45:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

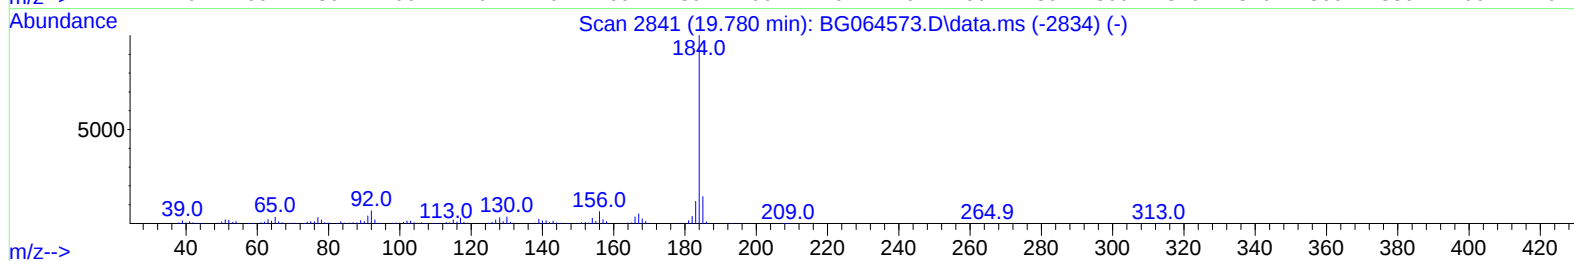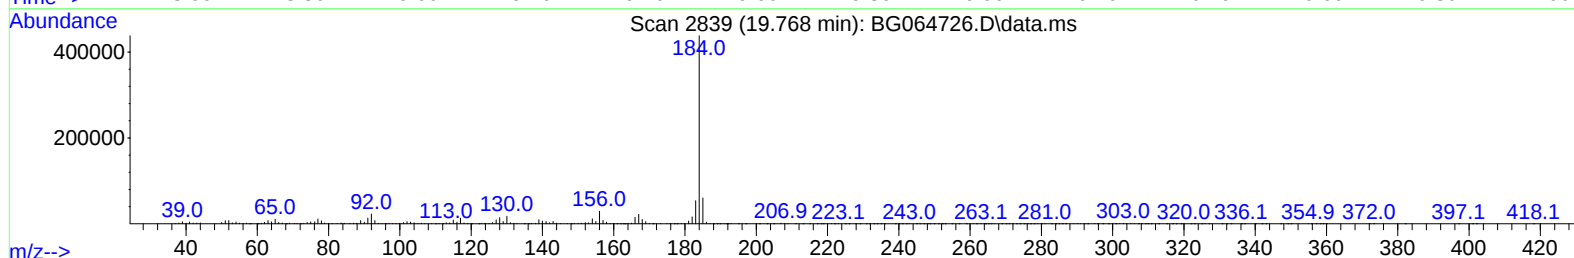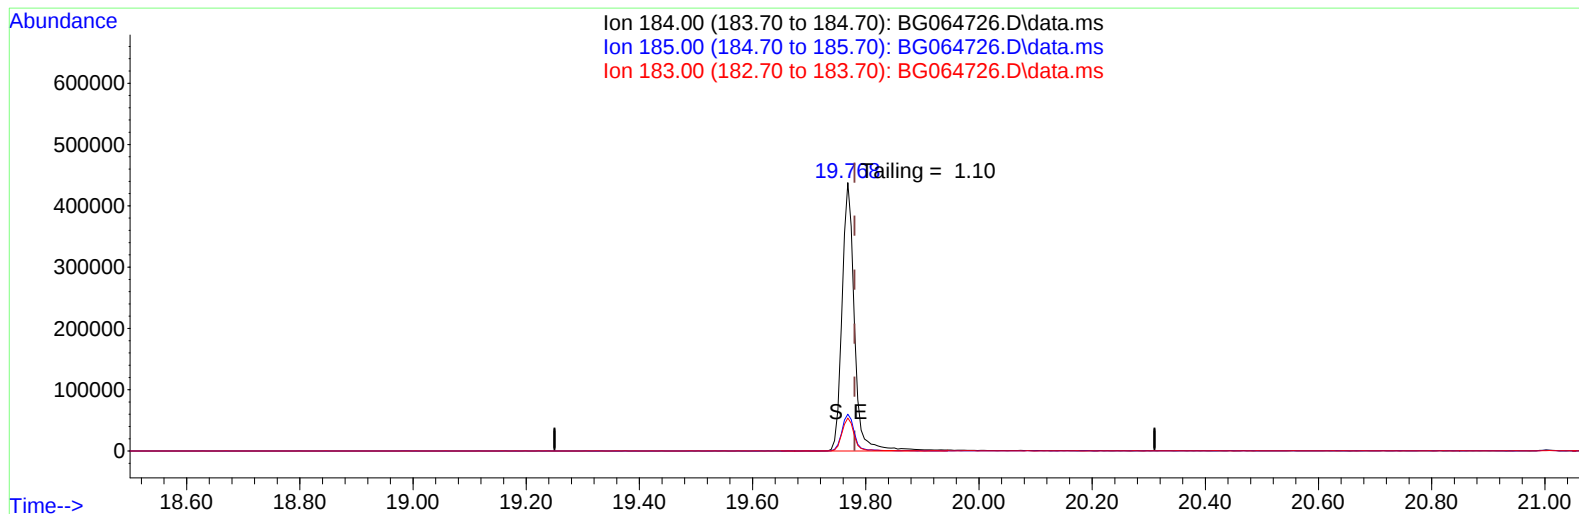

TIC: BG064726.D\data.ms

(77) Benzidine**19.768min (-0.012) 38234.27 ng****response 667296**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.72
183.00	11.80	12.32
0.00	0.00	0.00