


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111025\
Data File : BG064726.D
Acq On : 10 Nov 2025 8:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 03 18:16:26 2025

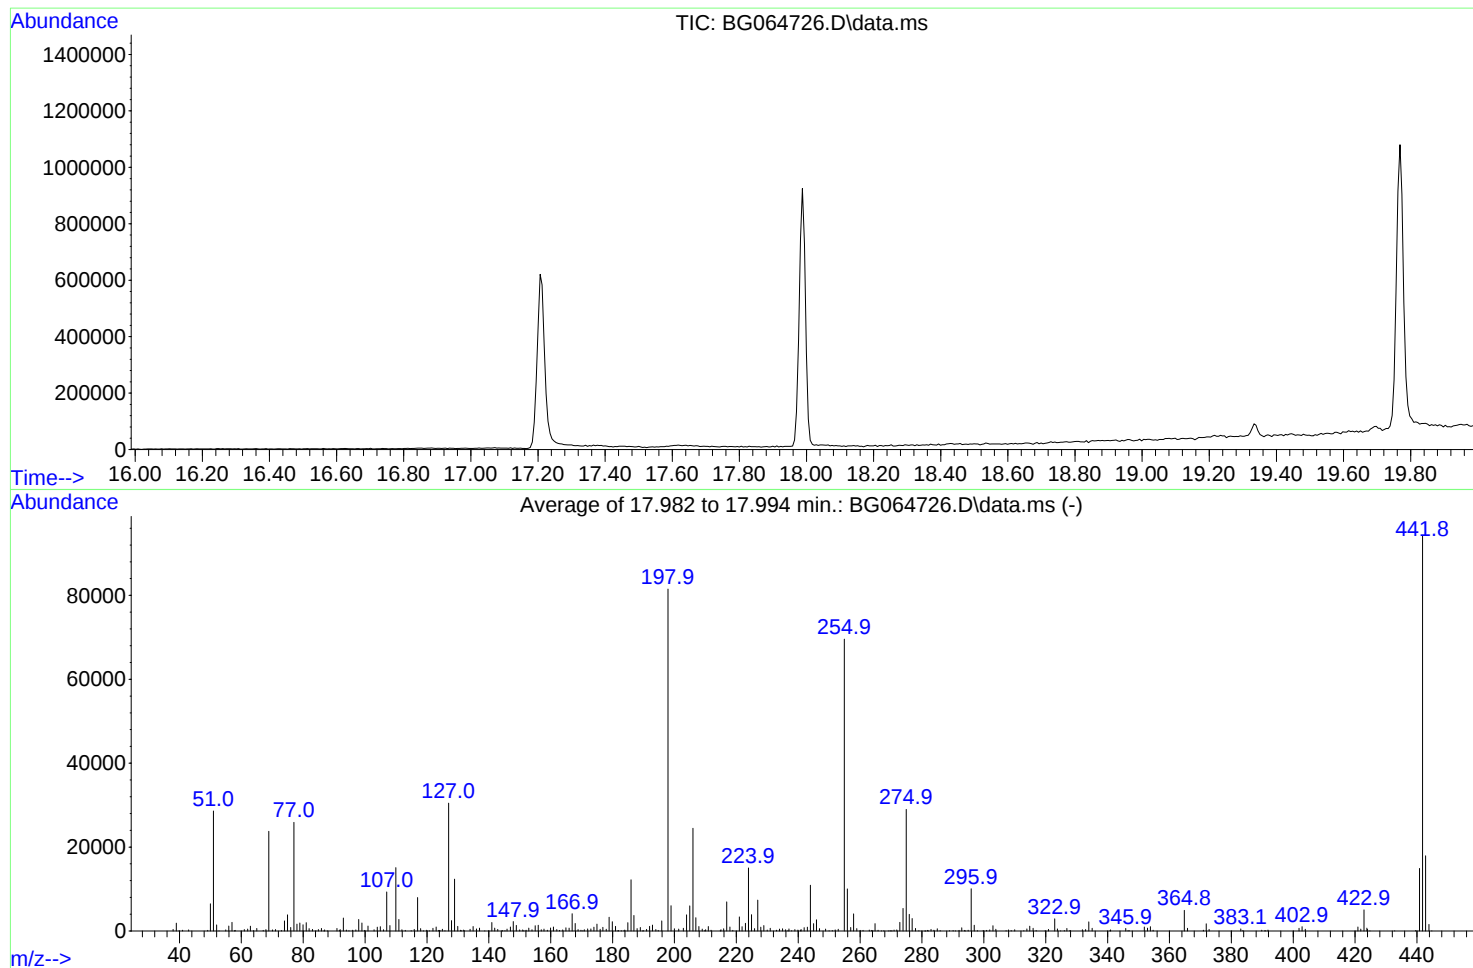

AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	328	PASS
69	69	100	100	100.0	23745	PASS
70	69	0.00	2	1.1	266	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81512	PASS
199	198	5	9	7.4	6014	PASS
365	198	1	100	6.1	4939	PASS
441	443	0.01	150	83.2	14901	PASS
442	442	100	100	100.0	94109	PASS
443	442	15	24	19.0	17917	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/10/2025	BNA_G	<u>BG064726.D</u>
Compound Name	Response	Retention Time
DDT	378036	21.008
DDD	6710	20.62
DDE		19.695
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6710	384746	1.74

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111025\
Data File : BG064726.D
Acq On : 10 Nov 2025 8:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 10 09:45:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

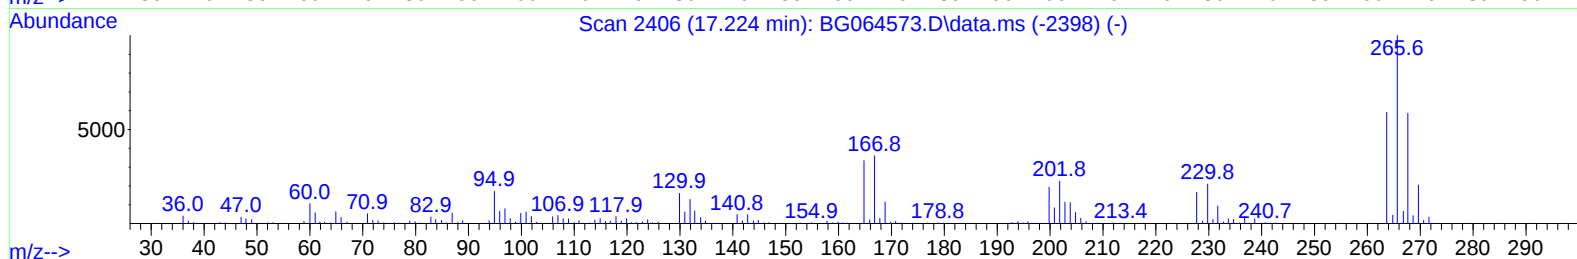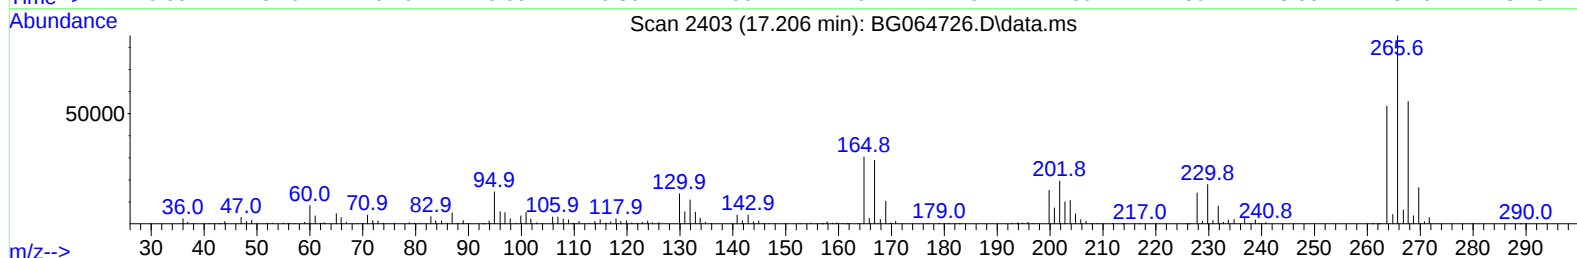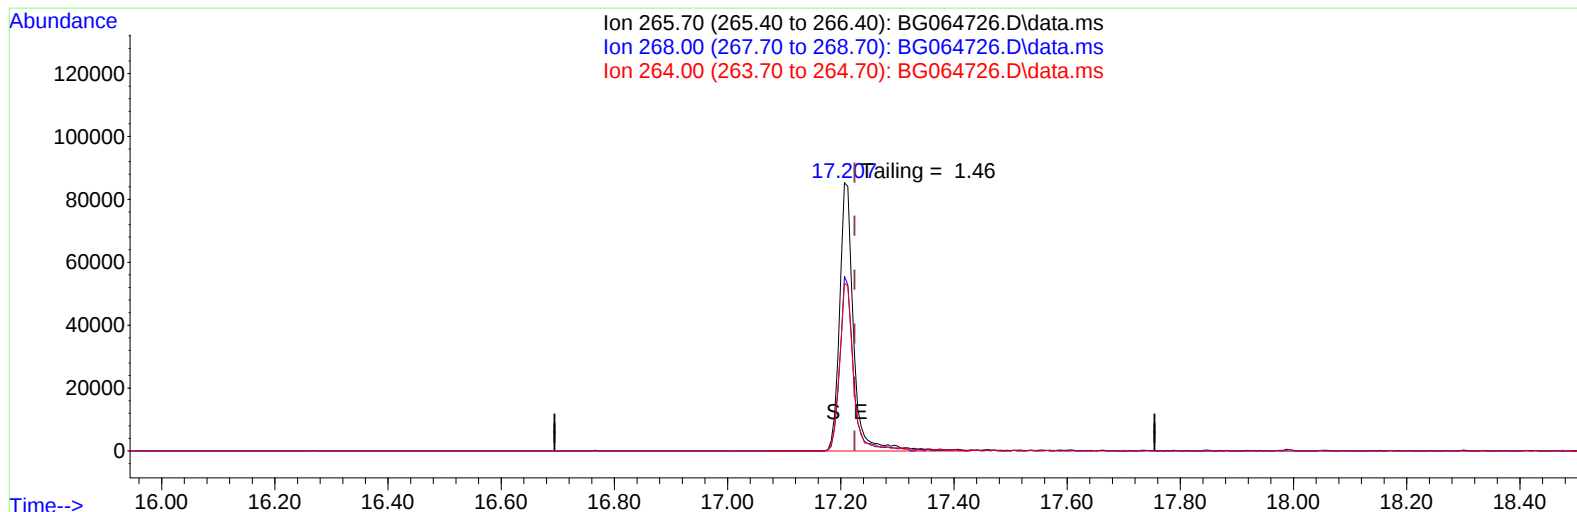

TIC: BG064726.D\data.ms

(70) Pentachlorophenol (C)

17.206min (-0.018) 284159.15 ng




response 146131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	69.51
264.00	59.10	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111025\
Data File : BG064726.D
Acq On : 10 Nov 2025 8:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 10 09:45:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 03 18:16:26 2025
Response via : Initial Calibration

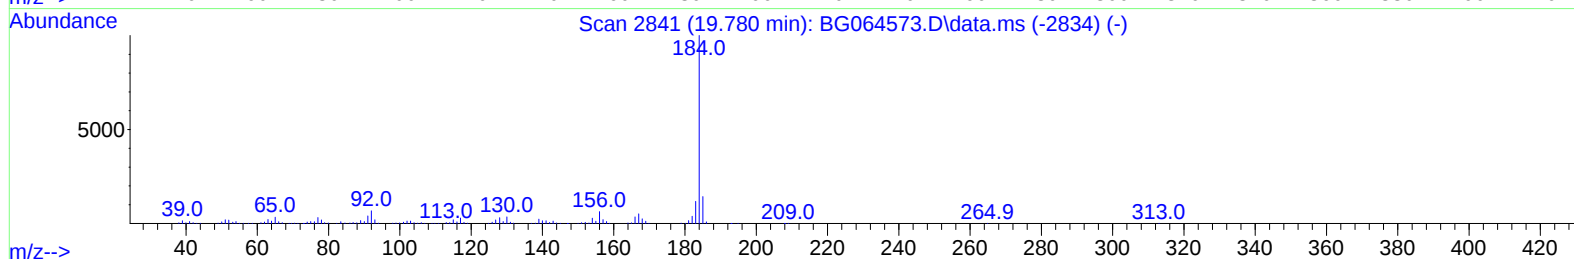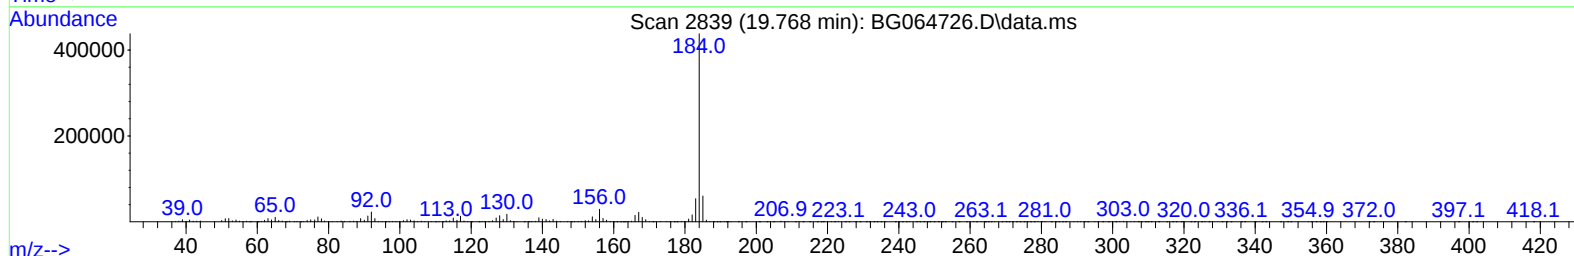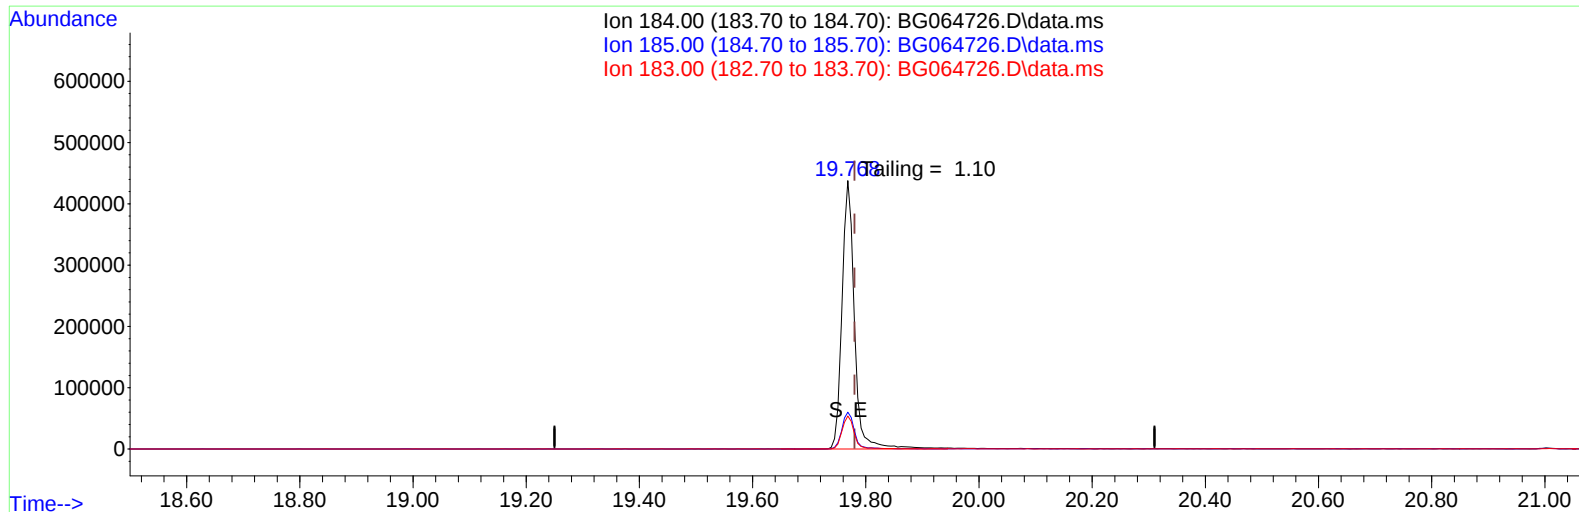

TIC: BG064726.D\data.ms

(77) Benzidine

19.768min (-0.012) 38234.27 ng

response 667296

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.72
183.00	11.80	12.32
0.00	0.00	0.00