
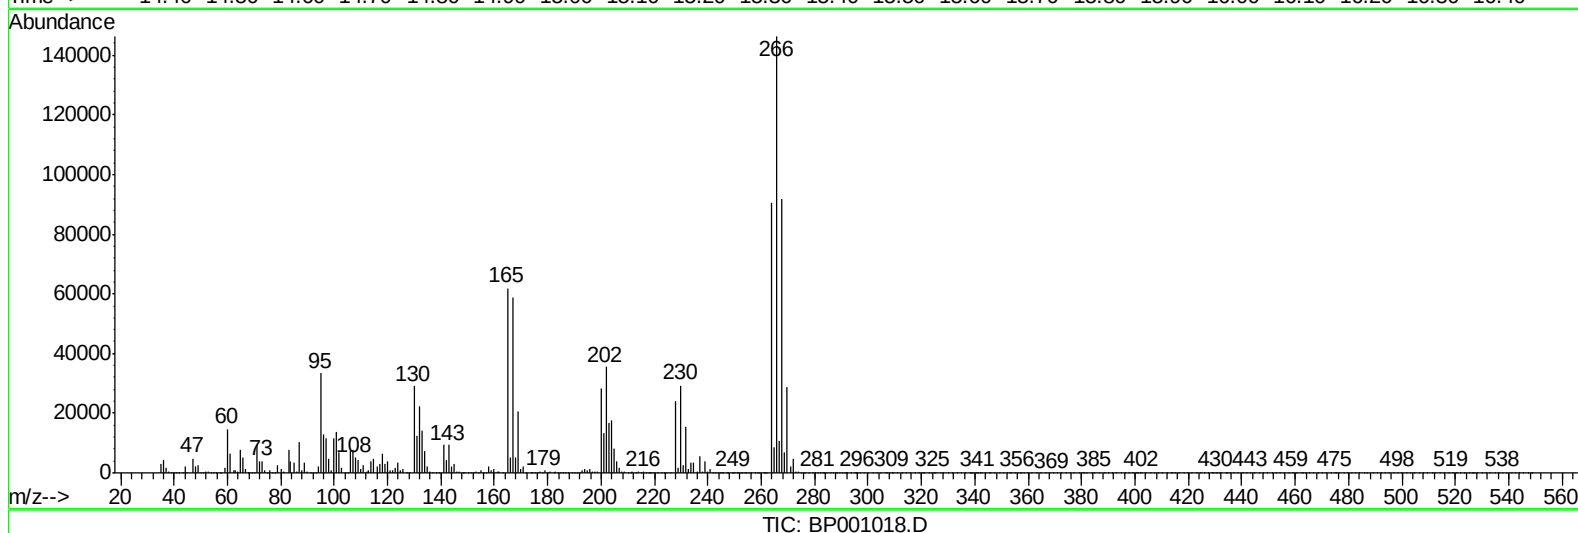


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP111119\
Data File : BP001018.D
Acq On : 11 Nov 2019 15:56
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:47:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 06 17:07:13 2019
Response via : Initial Calibration

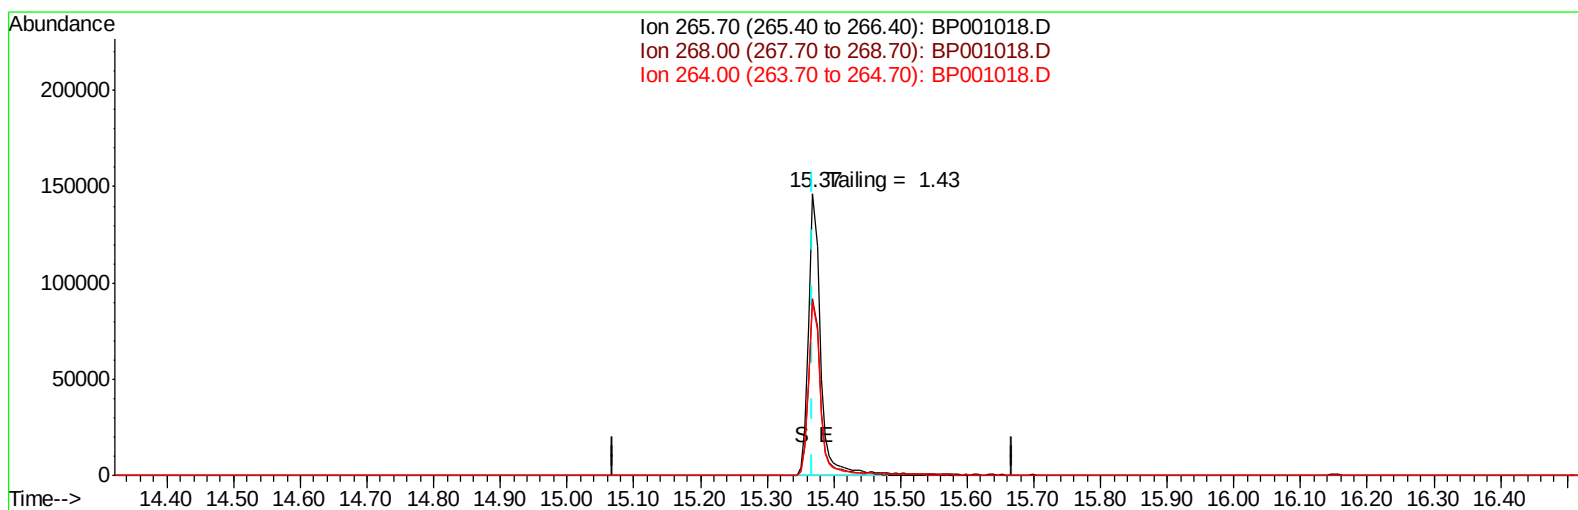

TIC: BP001018.D

(70) Pentachlorophenol (C)

15.369min (-0.000) 7272958.88ng



response 176663

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.87
264.00	63.30	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP111119\
 Data File : BP001018.D
 Acq On : 11 Nov 2019 15:56
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 12 08:47:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP110619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 06 17:07:13 2019
 Response via : Initial Calibration

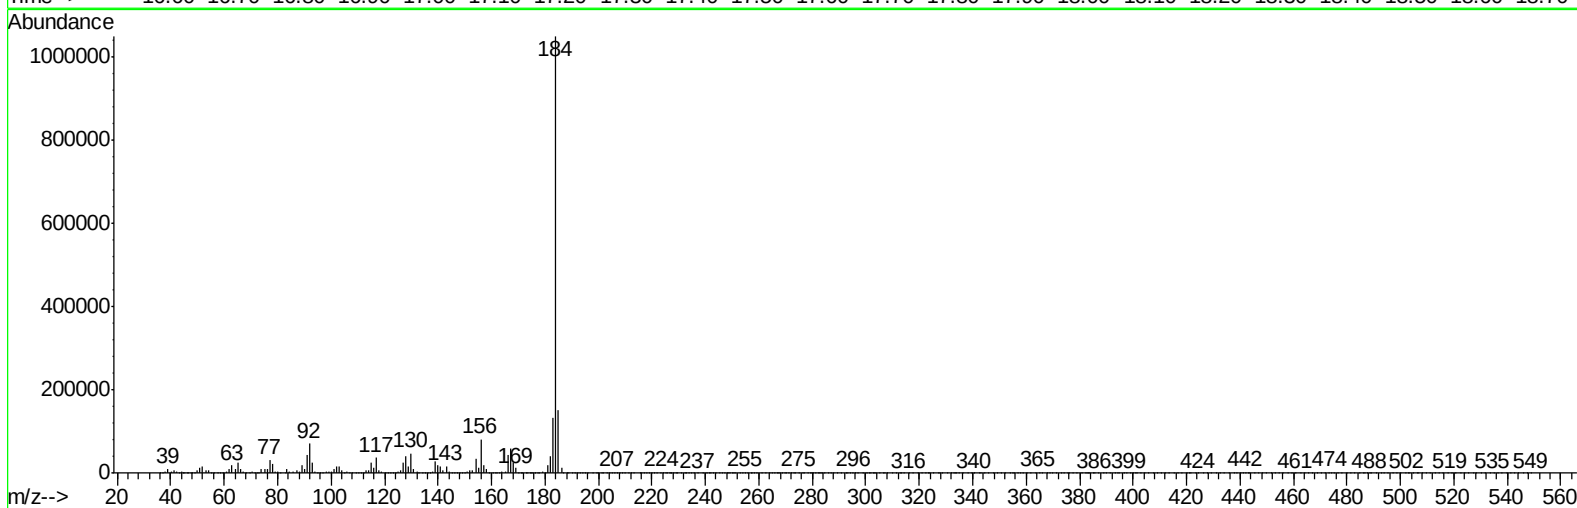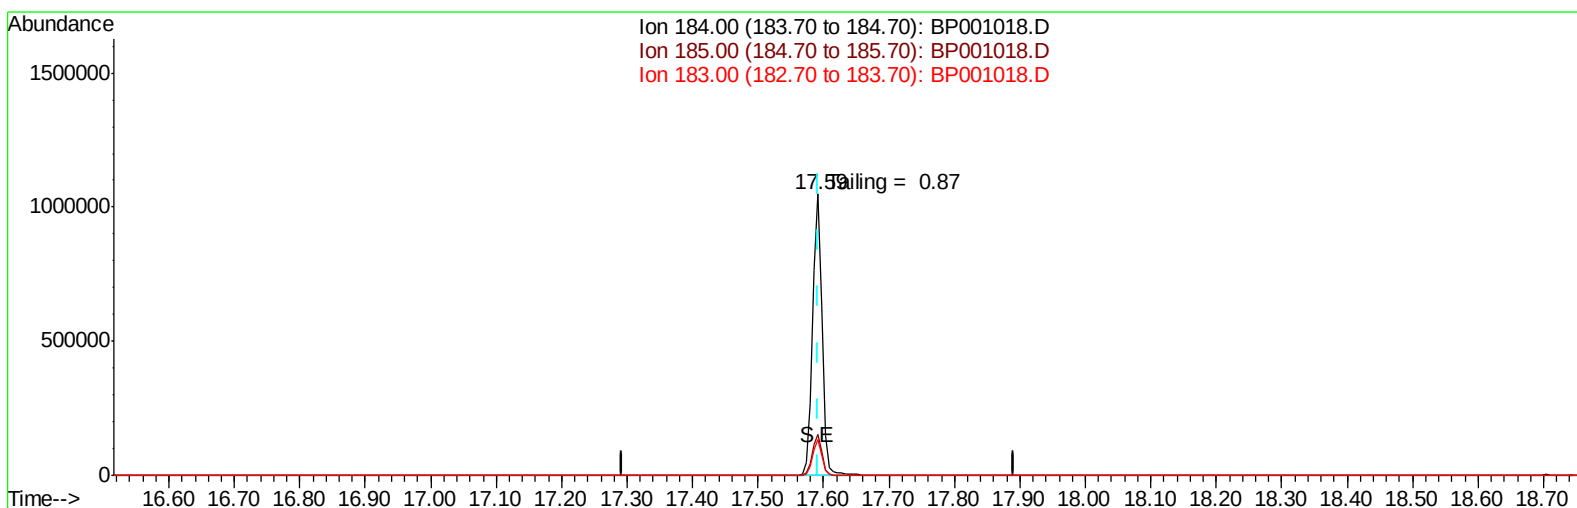

TIC: BP001018.D

(77) Benzidine

17.592min (-0.000) 22652.10ng



response 1067756

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.43
183.00	12.20	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043584.D
Acq On : 11 Nov 2019 15:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:48:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

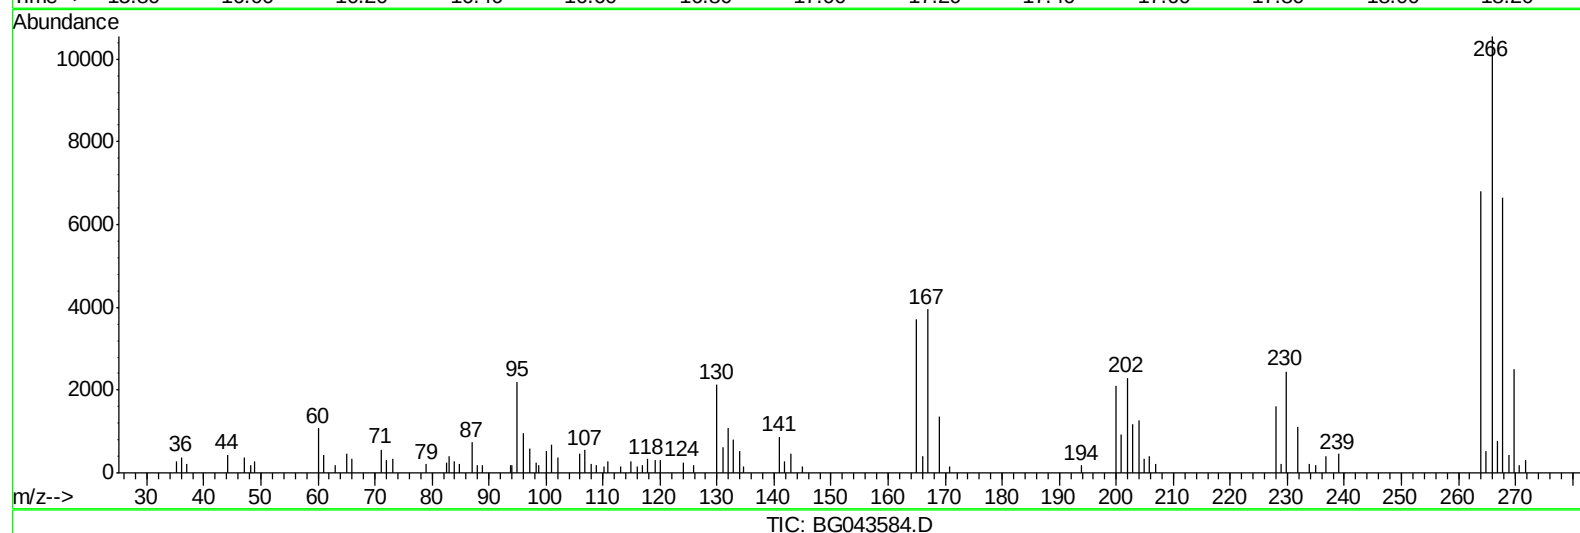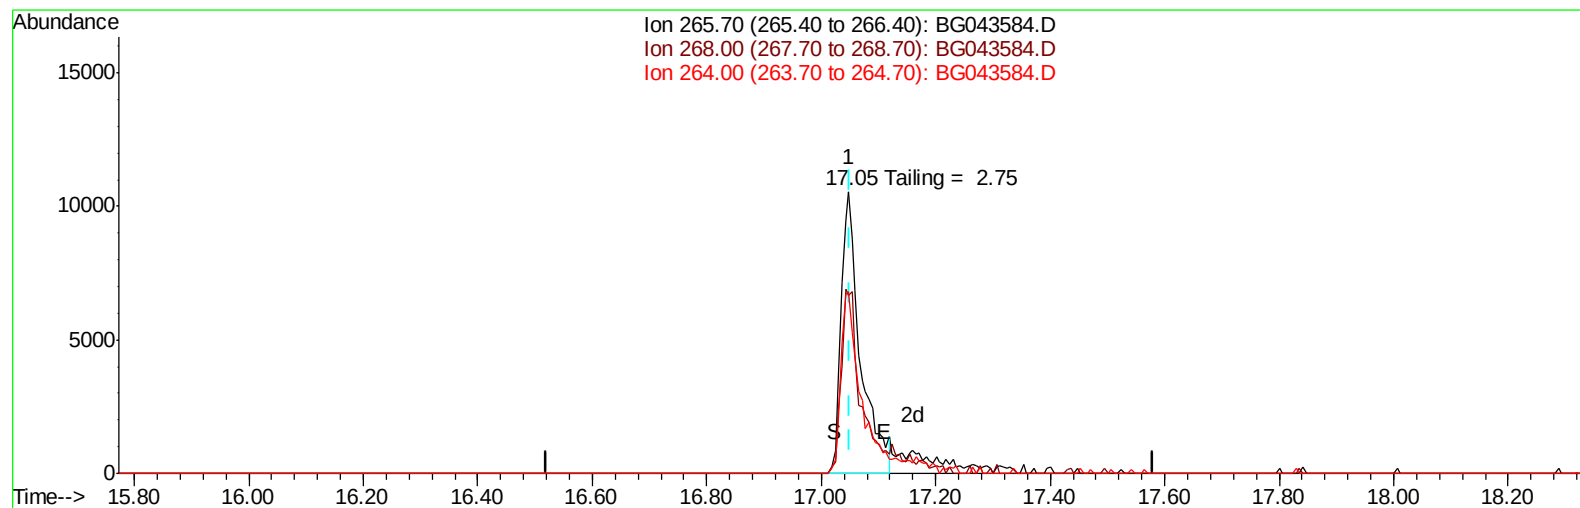

TIC: BG043584.D

(70) Pentachlorophenol (C)

17.048min (-0.002) 29878.81ng



response 25238

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	63.01
264.00	61.10	64.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043584.D
Acq On : 11 Nov 2019 15:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:48:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

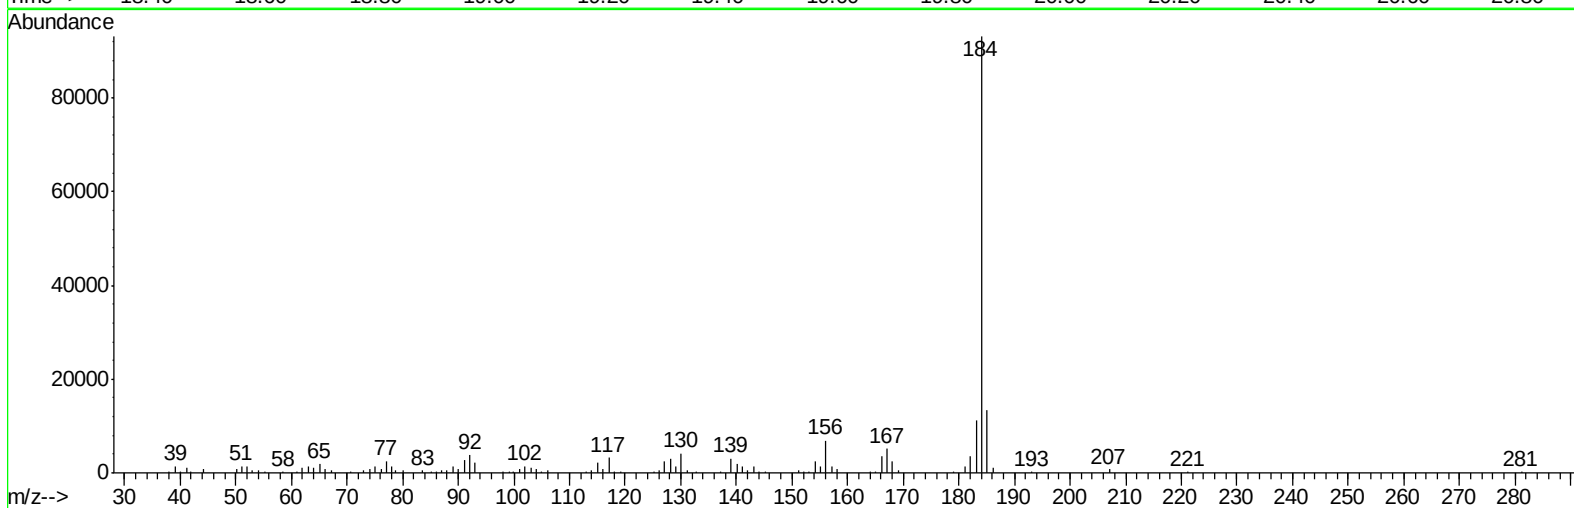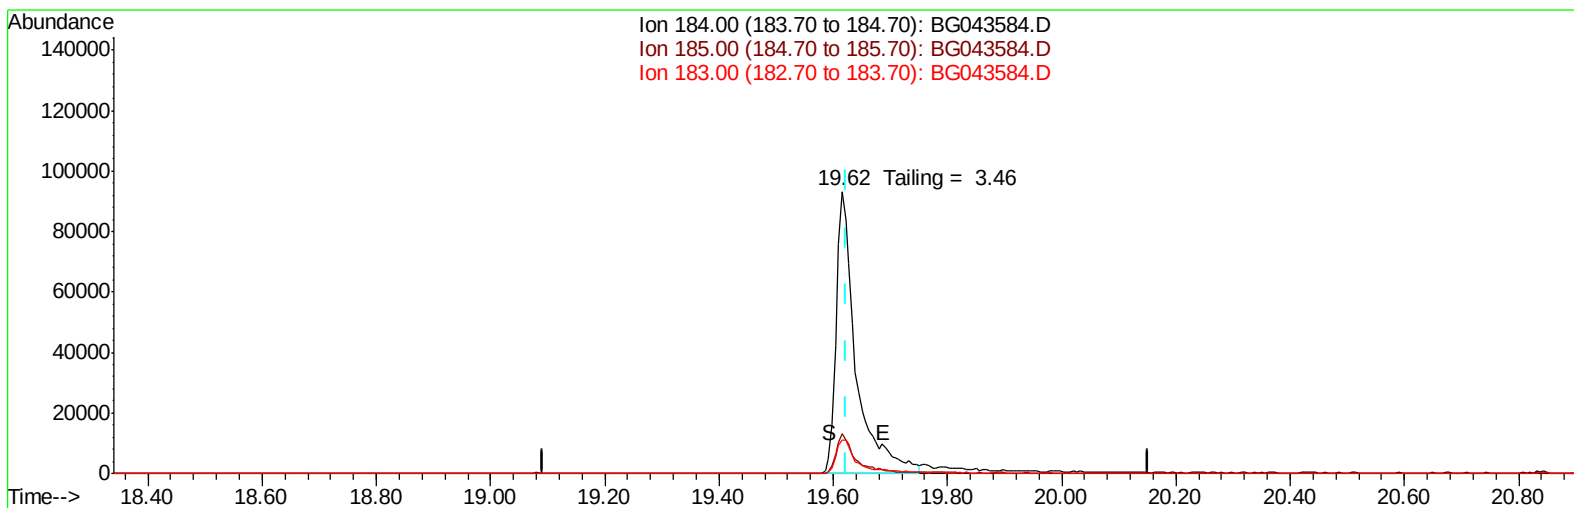

TIC: BG043584.D

(77) Benzidine

19.615min (-0.008) 186529.61ng



response 225238

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	14.23
183.00	12.50	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043584.D
Acq On : 11 Nov 2019 15:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:48:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

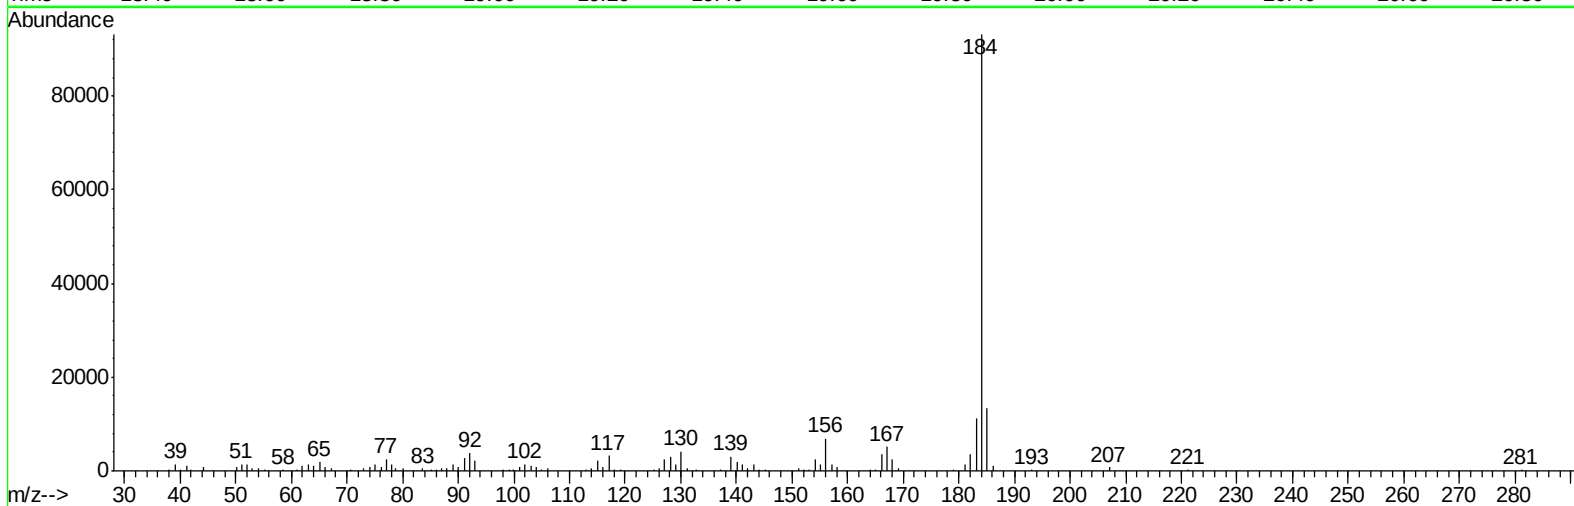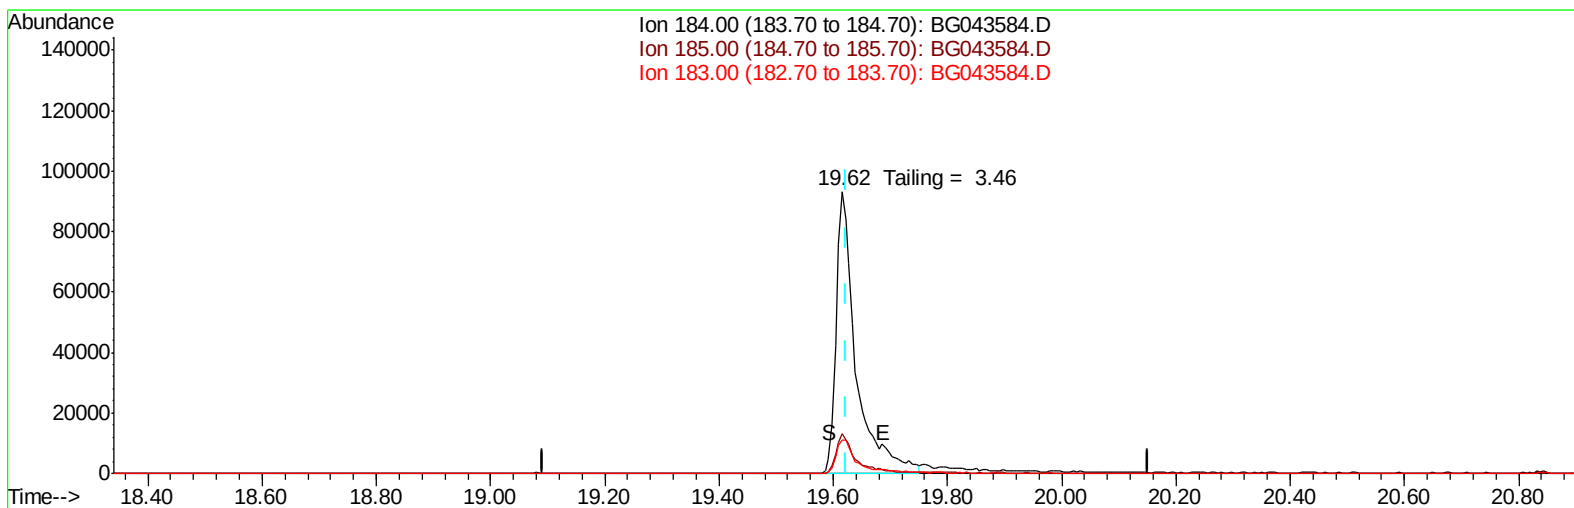

TIC: BG043584.D

(77) Benzidine

19.615min (-0.008) 186529.61ng



response 225238

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	14.23
183.00	12.50	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043602.D
Acq On : 12 Nov 2019 3:44
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:49:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

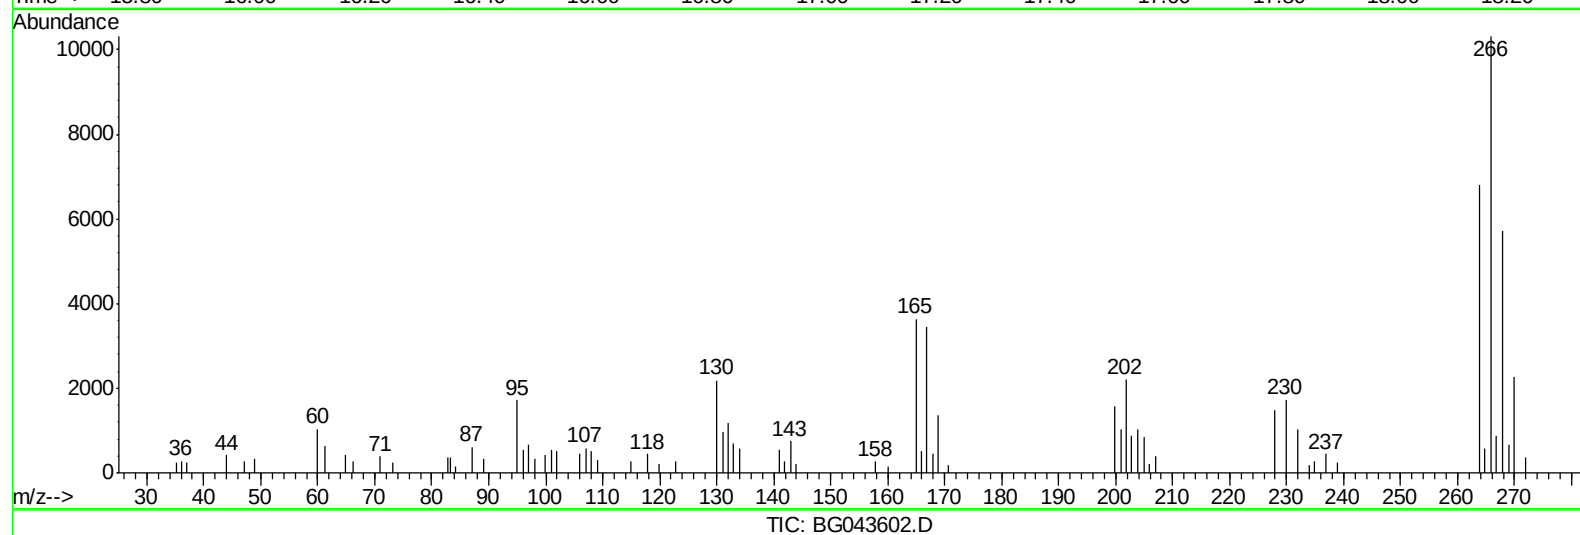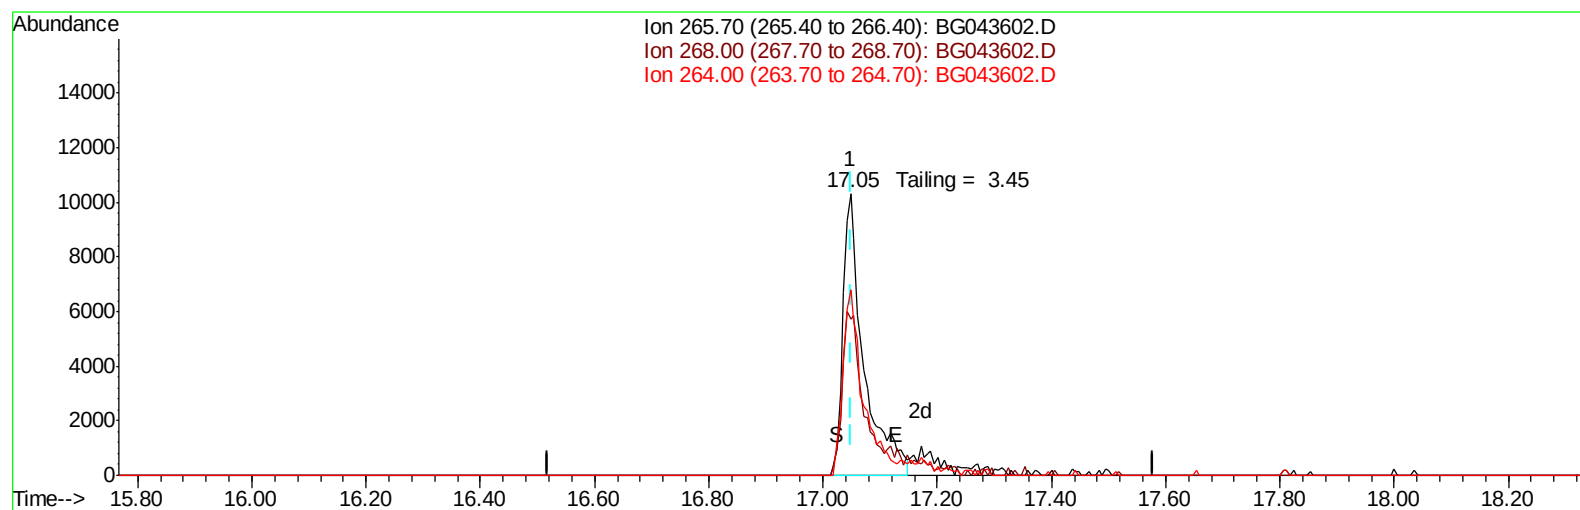

(70) Pentachlorophenol (C)

17.048min (-0.002) 58747.59ng



response 26052

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	55.50
264.00	61.10	66.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043602.D
Acq On : 12 Nov 2019 3:44
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:49:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

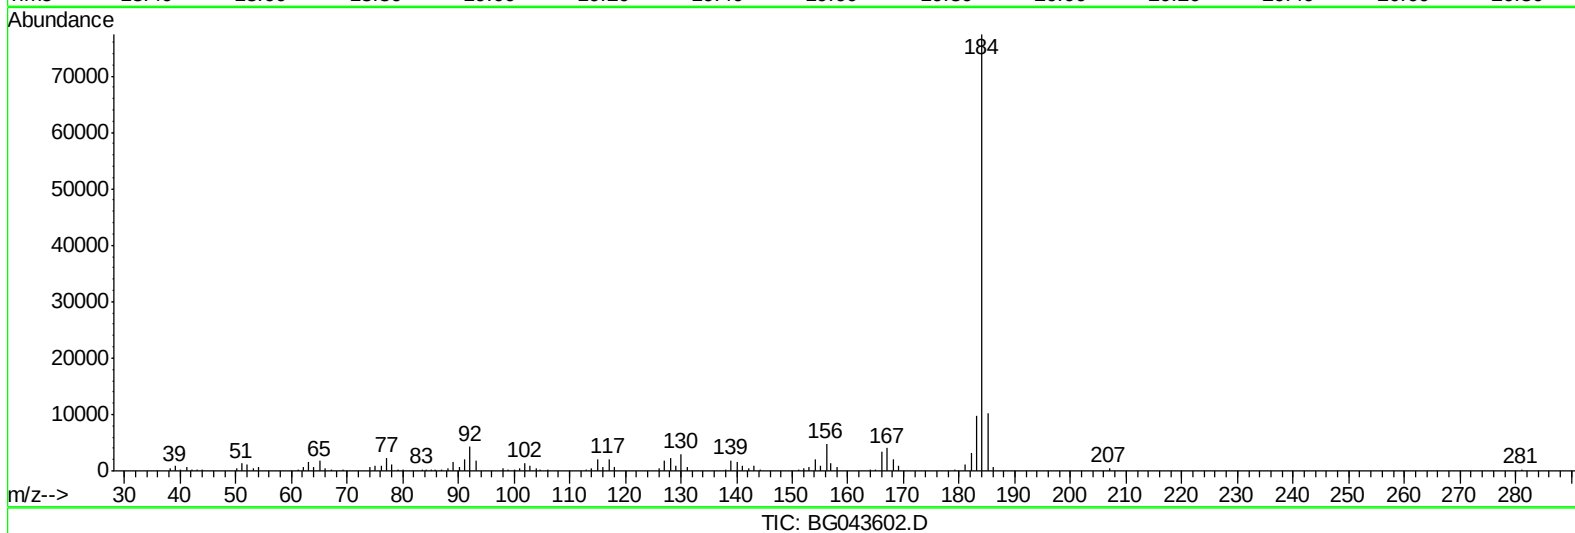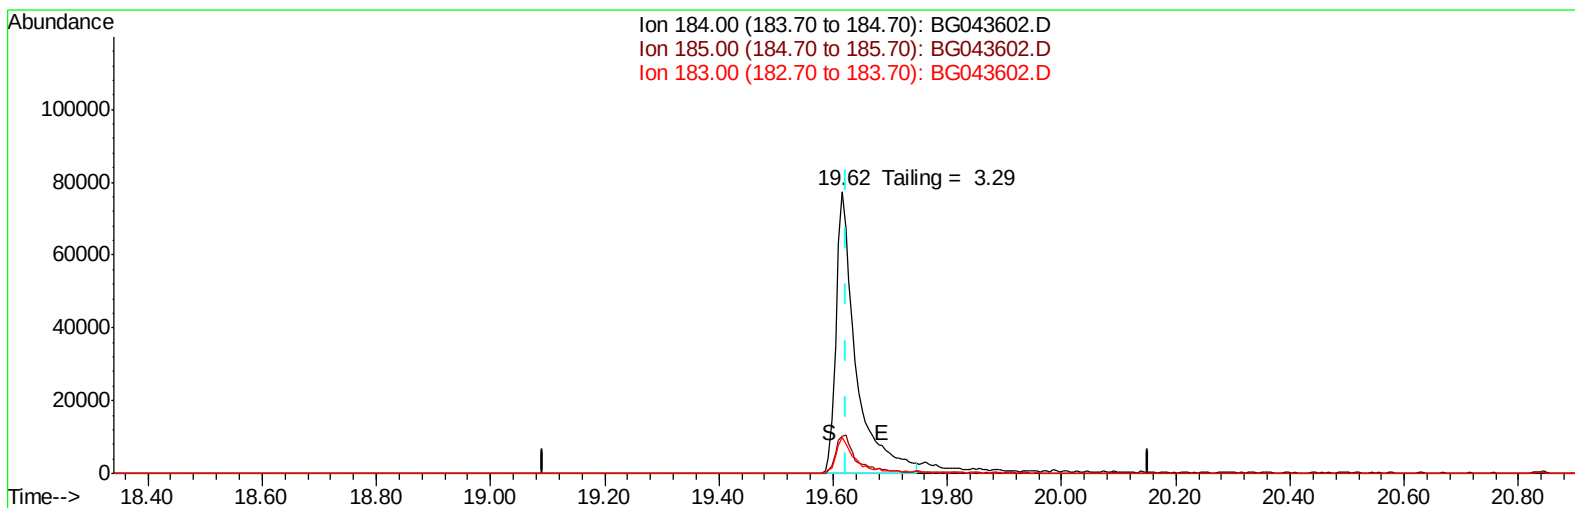

(77) Benzidine

19.615min (-0.008) 0.00ng



response 186972

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	13.25
183.00	12.50	12.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043584.D
Acq On : 11 Nov 2019 15:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:48:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

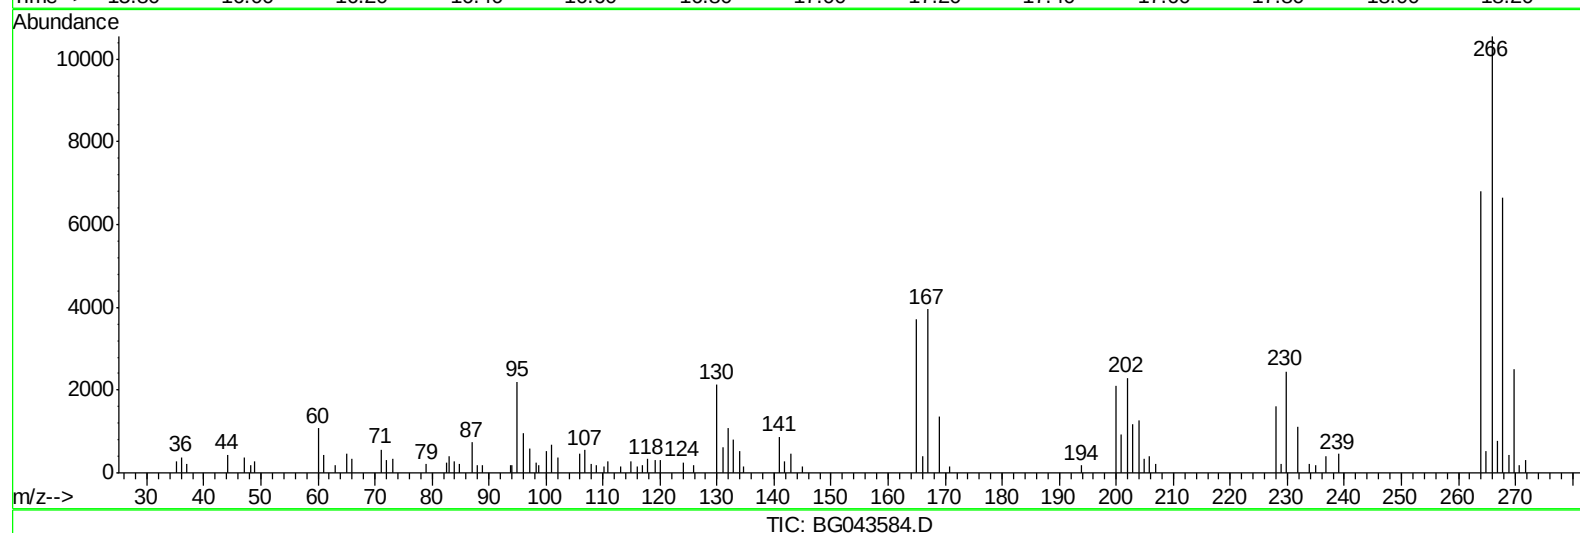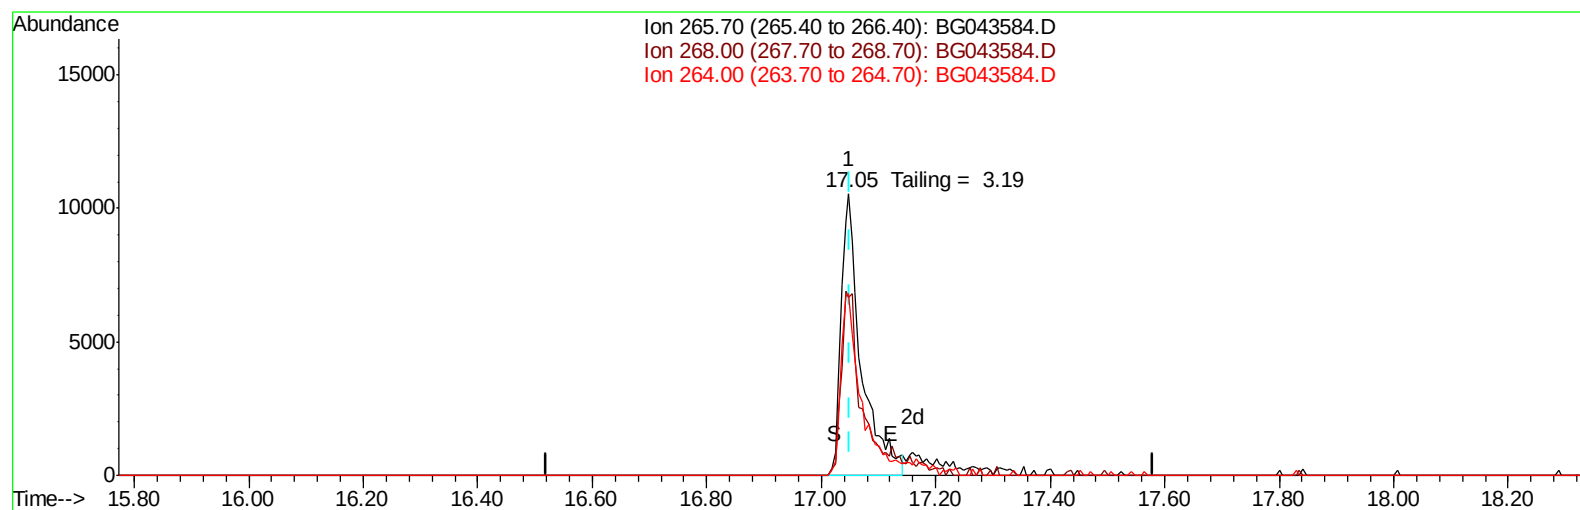

TIC: BG043584.D

(70) Pentachlorophenol (C)

17.048min (-0.002) 29878.81ng



response 25238

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	63.01
264.00	61.10	64.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111119\
Data File : BG043584.D
Acq On : 11 Nov 2019 15:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 12 08:48:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

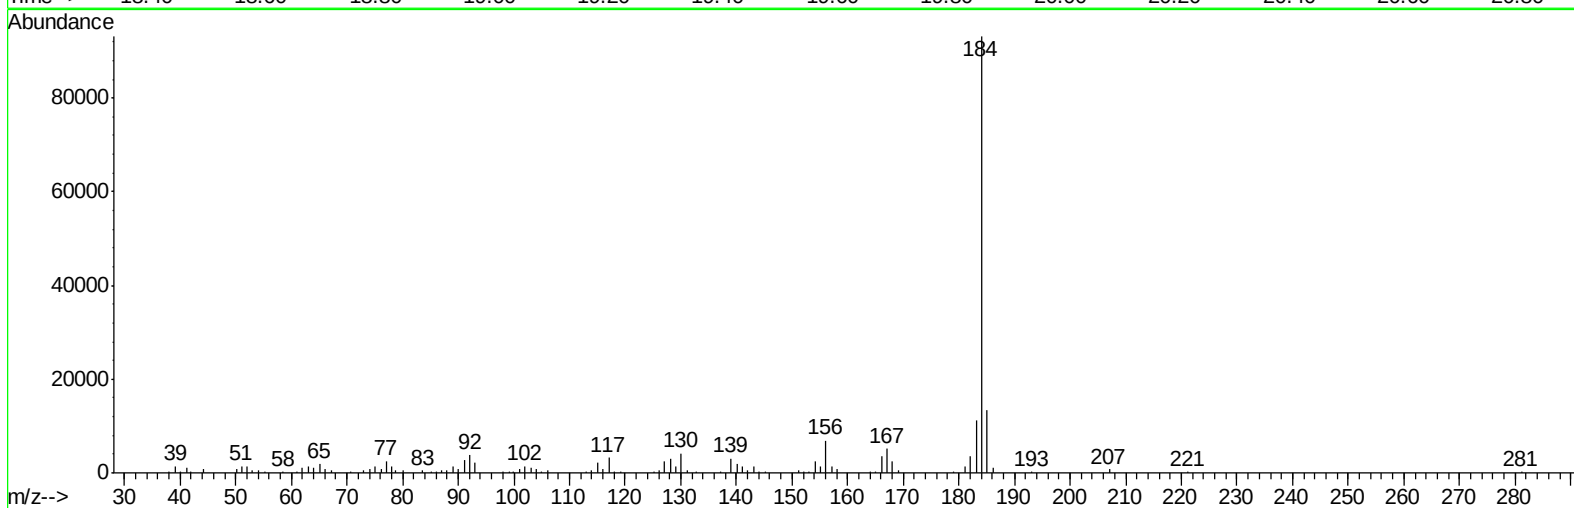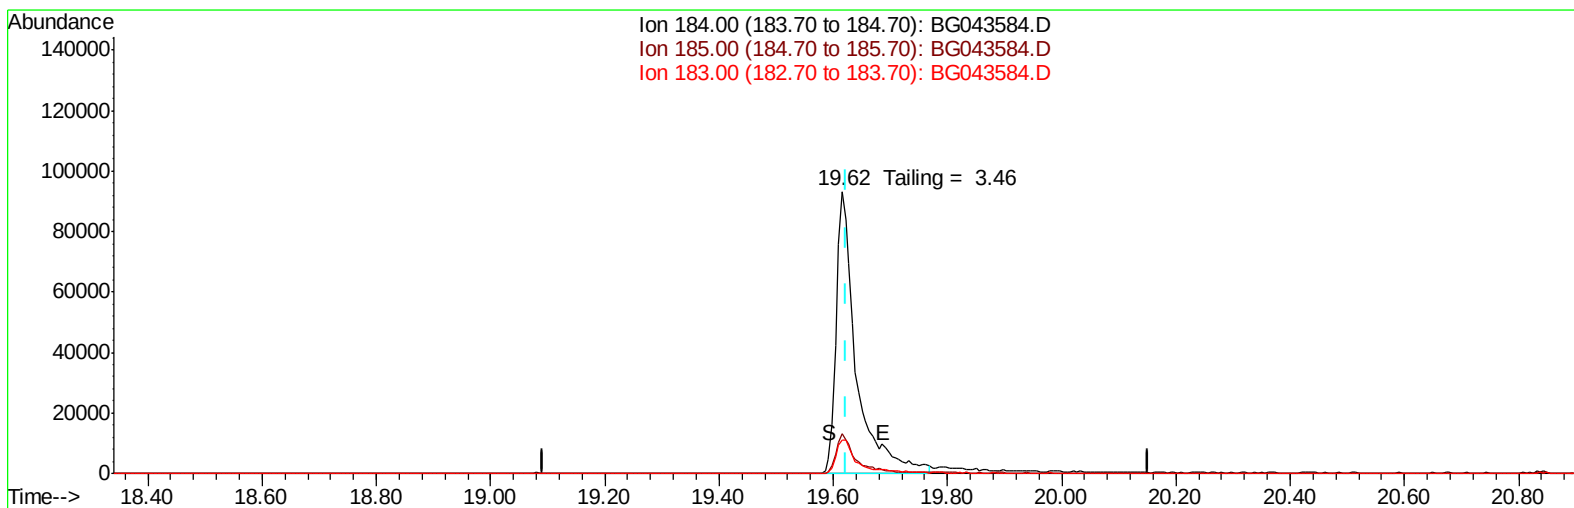

TIC: BG043584.D

(77) Benzidine

19.615min (-0.008) 186529.61ng

response 225238

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	14.23
183.00	12.50	11.99
0.00	0.00	0.00